

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029585.D
 Acq On : 10 Dec 2022 16:48
 Operator : SY/MD
 Sample : N5928-20 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029585.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	198543	199228	13.20%	1.597%
2	1.561	155	162	178	rVB	171436	198678	13.17%	1.592%
3	2.105	320	331	347	rBV	336059	481551	31.91%	3.859%
4	2.349	405	407	410	rVB2	310	143	0.01%	0.001%
5	2.503	450	455	466	rVB3	2869	4058	0.27%	0.033%
6	2.815	550	552	558	rVB2	223	130	0.01%	0.001%
7	2.902	577	579	581	rBV	208	120	0.01%	0.001%
8	3.262	688	691	694	rBV	172	150	0.01%	0.001%
9	3.314	705	707	708	rBV	139	45	0.00%	0.000%
10	3.323	708	710	713	rVV3	238	137	0.01%	0.001%
11	3.346	713	717	721	rVV2	205	204	0.01%	0.002%
12	3.407	733	736	743	rVB2	161	184	0.01%	0.001%
13	3.458	748	752	756	rBV	192	149	0.01%	0.001%
14	3.651	809	812	816	rVB	326	228	0.02%	0.002%
15	3.674	816	819	821	rBV2	192	135	0.01%	0.001%
16	3.873	871	881	934	rBV2	121736	376046	24.92%	3.013%
17	4.339	1009	1026	1059	rBV	235281	581883	38.56%	4.663%
18	4.635	1116	1118	1121	rVB	333	184	0.01%	0.001%
19	4.651	1121	1123	1127	rVB2	236	132	0.01%	0.001%
20	4.680	1127	1132	1135	rBV2	388	374	0.02%	0.003%
21	4.745	1150	1152	1154	rBV	222	131	0.01%	0.001%
22	4.780	1161	1163	1170	rVB2	335	305	0.02%	0.002%
23	4.812	1170	1173	1175	rBV2	193	86	0.01%	0.001%
24	4.828	1175	1178	1181	rVB2	179	106	0.01%	0.001%
25	4.847	1181	1184	1192	rBV2	224	232	0.02%	0.002%
26	4.880	1192	1194	1195	rBV2	160	52	0.00%	0.000%
27	4.928	1207	1209	1214	rBV2	236	160	0.01%	0.001%
28	5.040	1226	1244	1279	rBV2	573896	1508950	100.00%	12.092%
29	5.394	1352	1354	1356	rBV2	273	160	0.01%	0.001%
30	5.426	1361	1364	1365	rBV2	180	97	0.01%	0.001%
31	5.442	1366	1369	1372	rBV2	188	153	0.01%	0.001%
32	5.555	1402	1404	1405	rBV	152	62	0.00%	0.000%
33	5.609	1408	1421	1451	rBV	582095	1180368	78.22%	9.459%
34	5.902	1502	1512	1528	rVB5	5059	10354	0.69%	0.083%
35	6.063	1547	1562	1596	rBV	328611	675468	44.76%	5.413%
36	6.310	1637	1639	1641	rVB	229	100	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029585.D
 Acq On : 10 Dec 2022 16:48
 Operator : SY/MD
 Sample : N5928-20 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.326	1641	1644	1648	rVB2	490	272	0.02%	0.002%
38	6.365	1652	1656	1660	rBV2	358	380	0.03%	0.003%
39	6.433	1675	1677	1680	rVB2	145	64	0.00%	0.001%
40	6.474	1686	1690	1692	rBV2	182	134	0.01%	0.001%
41	6.519	1700	1704	1705	rBV2	277	183	0.01%	0.001%
42	6.545	1709	1712	1714	rBV2	142	87	0.01%	0.001%
43	6.625	1731	1737	1738	rBV4	818	916	0.06%	0.007%
44	6.748	1771	1775	1777	rBV2	253	163	0.01%	0.001%
45	6.770	1777	1782	1787	rVB2	390	280	0.02%	0.002%
46	6.796	1787	1790	1792	rBV2	223	149	0.01%	0.001%
47	6.812	1793	1795	1799	rVB2	284	196	0.01%	0.002%
48	6.883	1814	1817	1821	rBV2	95	86	0.01%	0.001%
49	6.908	1823	1825	1826	rVB	145	39	0.00%	0.000%
50	6.979	1834	1847	1875	rBV	150743	278305	18.44%	2.230%
51	7.256	1929	1933	1937	rBV3	515	514	0.03%	0.004%
52	7.307	1937	1949	1980	rBV	708655	1243805	82.43%	9.967%
53	7.613	2034	2044	2063	rBV	105877	186103	12.33%	1.491%
54	7.854	2117	2119	2121	rBV2	463	279	0.02%	0.002%
55	8.031	2172	2174	2177	rBV2	254	112	0.01%	0.001%
56	8.082	2180	2190	2222	rBV	406352	742503	49.21%	5.950%
57	8.571	2340	2342	2345	rBV3	269	129	0.01%	0.001%
58	8.596	2348	2350	2351	rBV	254	102	0.01%	0.001%
59	8.683	2375	2377	2381	rVB2	213	86	0.01%	0.001%
60	8.712	2381	2386	2387	rBV	281	173	0.01%	0.001%
61	8.732	2391	2392	2396	rVB2	252	122	0.01%	0.001%
62	8.844	2414	2427	2463	rBV	845751	1400284	92.80%	11.221%
63	9.169	2523	2528	2531	rBV3	373	338	0.02%	0.003%
64	9.294	2564	2567	2570	rVB2	394	176	0.01%	0.001%
65	9.310	2570	2572	2578	rVB2	178	132	0.01%	0.001%
66	9.358	2584	2587	2588	rBV	183	107	0.01%	0.001%
67	9.381	2590	2594	2596	rVV	445	332	0.02%	0.003%
68	9.397	2597	2599	2605	rVV2	245	167	0.01%	0.001%
69	9.429	2606	2609	2611	rVB2	229	127	0.01%	0.001%
70	9.445	2612	2614	2620	rBV2	271	183	0.01%	0.001%
71	9.474	2620	2623	2624	rBV	222	130	0.01%	0.001%
72	9.580	2653	2656	2658	rBV2	226	129	0.01%	0.001%
73	9.674	2681	2685	2689	rBV2	277	239	0.02%	0.002%
74	9.799	2722	2724	2726	rBV	171	88	0.01%	0.001%
75	9.886	2747	2751	2754	rBV3	175	146	0.01%	0.001%
76	9.899	2754	2755	2756	rVB	181	37	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029585.D
 Acq On : 10 Dec 2022 16:48
 Operator : SY/MD
 Sample : N5928-20 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.924	2761	2763	2765	rVV	175	77	0.01%	0.001%
78	10.092	2811	2815	2816	rBV	170	109	0.01%	0.001%
79	10.162	2827	2837	2841	rBV	21316	30613	2.03%	0.245%
80	10.204	2842	2850	2871	rVB	482081	751923	49.83%	6.026%
81	10.342	2892	2893	2896	rBV	223	117	0.01%	0.001%
82	10.358	2896	2898	2900	rVV	376	156	0.01%	0.001%
83	10.522	2948	2949	2951	rBV	200	101	0.01%	0.001%
84	10.567	2954	2963	2981	rVB2	9870	15900	1.05%	0.127%
85	10.696	3001	3003	3004	rBV	173	56	0.00%	0.000%
86	10.911	3068	3070	3073	rBV	204	118	0.01%	0.001%
87	11.021	3100	3104	3109	rBV3	466	421	0.03%	0.003%
88	11.063	3115	3117	3119	rVB2	303	81	0.01%	0.001%
89	11.236	3159	3171	3203	rBV	917959	1435277	95.12%	11.502%
90	11.612	3276	3288	3312	rBV	737263	1164047	77.14%	9.328%
91	11.902	3376	3378	3381	rBV	213	162	0.01%	0.001%
92	11.924	3383	3385	3388	rVB	467	226	0.01%	0.002%
93	11.969	3397	3399	3402	rBV2	274	174	0.01%	0.001%
94	12.005	3407	3410	3414	rBV2	245	185	0.01%	0.001%
95	12.027	3414	3417	3420	rBV3	358	234	0.02%	0.002%
96	12.040	3420	3421	3424	rBV2	260	157	0.01%	0.001%
97	12.963	3703	3708	3709	rBV2	416	322	0.02%	0.003%




Sum of corrected areas: 12478796

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029585.D
Acq On : 10 Dec 2022 16:48
Operator : SY/MD
Sample : N5928-20 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 79 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

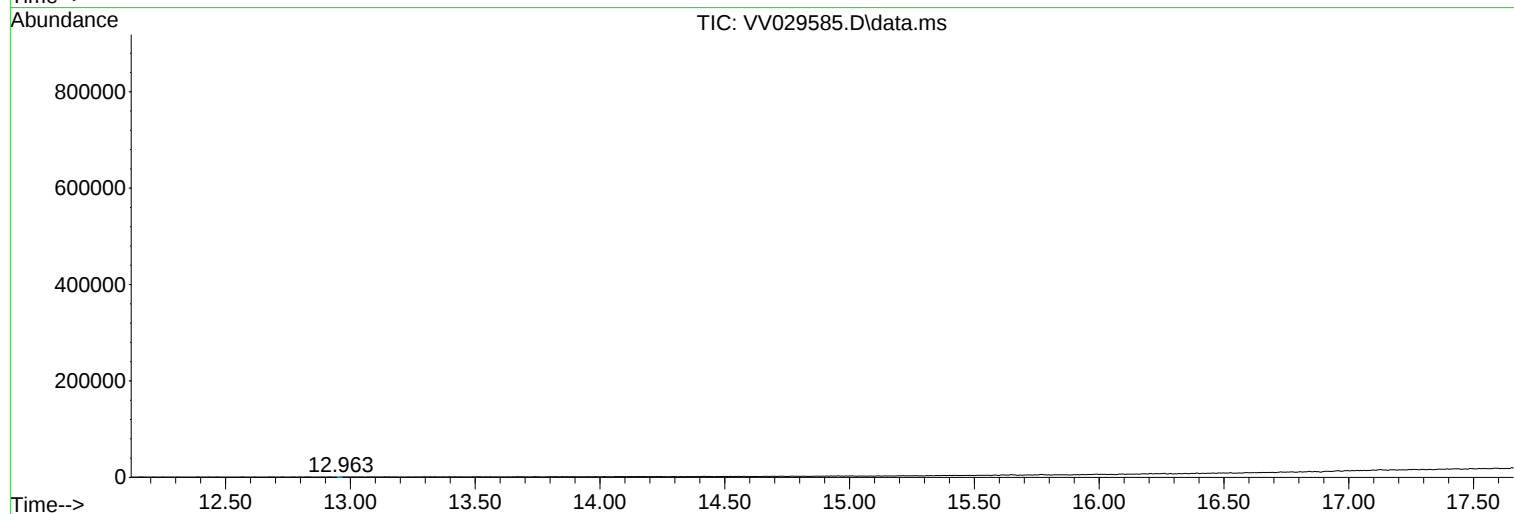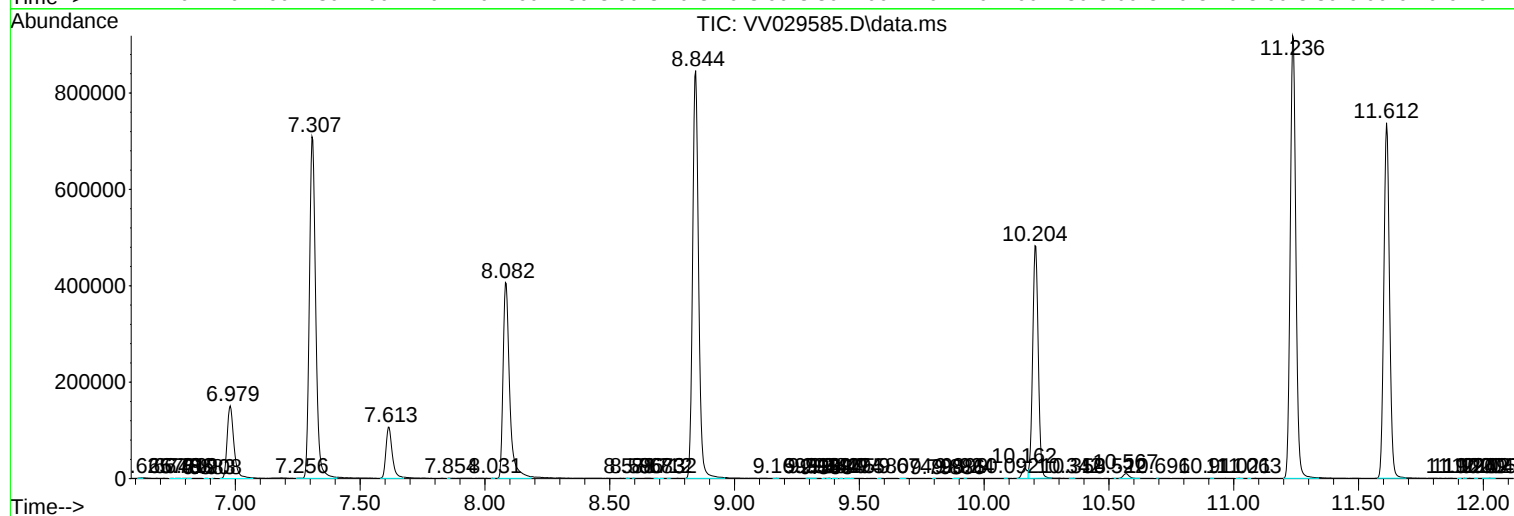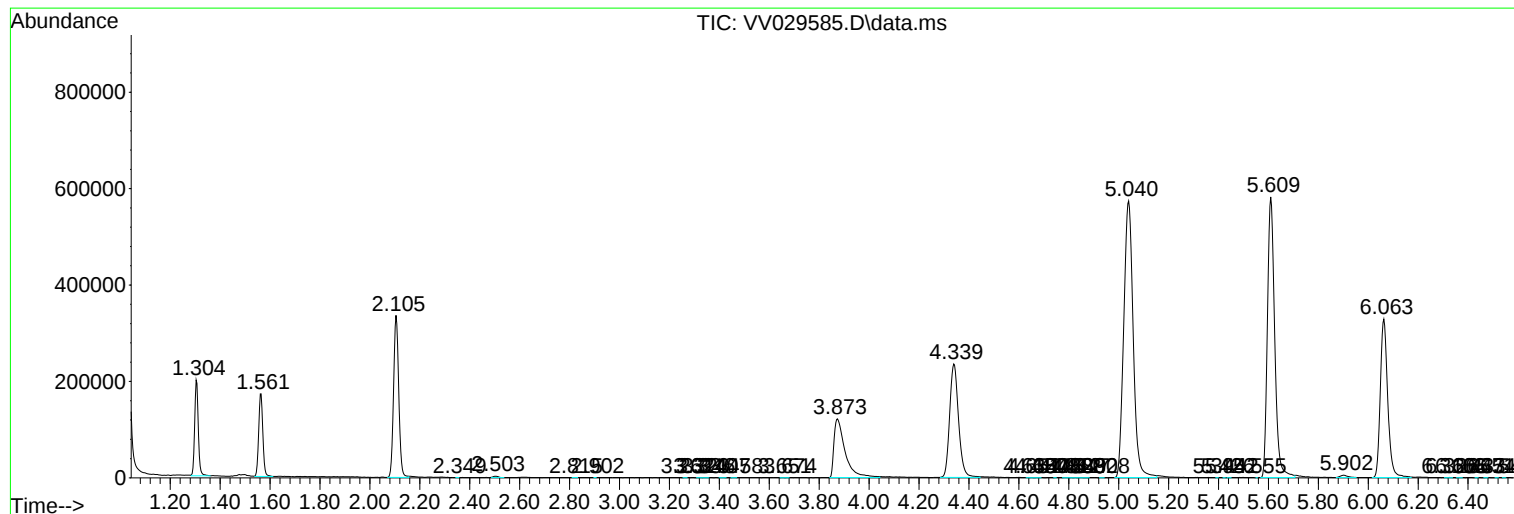

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029585.D
Acq On : 10 Dec 2022 16:48
Operator : SY/MD
Sample : N5928-20 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 79 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029585.D
Acq On : 10 Dec 2022 16:48
Operator : SY/MD
Sample : N5928-20 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 79 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc