

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029586.D
 Acq On : 10 Dec 2022 17:12
 Operator : SY/MD
 Sample : N5928-21 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VV029586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	194665	195752	13.48%	1.610%
2	1.561	155	162	179	rVB	166002	191560	13.19%	1.576%
3	2.105	321	331	348	rBV	321583	462755	31.86%	3.807%
4	2.503	447	455	465	rBV2	3364	5240	0.36%	0.043%
5	2.712	518	520	523	rVB2	142	80	0.01%	0.001%
6	2.767	531	537	539	rBV4	477	484	0.03%	0.004%
7	3.191	658	669	684	rVB2	4529	9523	0.66%	0.078%
8	3.252	684	688	689	rBV	165	102	0.01%	0.001%
9	3.387	728	730	731	rBV	171	62	0.00%	0.001%
10	3.465	748	754	760	rBV2	281	305	0.02%	0.003%
11	3.593	788	794	796	rBV2	240	223	0.02%	0.002%
12	3.693	822	825	826	rBV	153	66	0.00%	0.001%
13	3.786	851	854	856	rBV2	135	69	0.00%	0.001%
14	3.873	870	881	930	rBV2	118917	374869	25.81%	3.084%
15	4.339	1010	1026	1054	rBV2	225322	560985	38.62%	4.615%
16	4.600	1093	1107	1122	rBV4	11591	28862	1.99%	0.237%
17	4.686	1132	1134	1136	rBV	221	86	0.01%	0.001%
18	4.703	1137	1139	1141	rVV	249	109	0.01%	0.001%
19	4.764	1155	1158	1161	rBV2	213	174	0.01%	0.001%
20	4.844	1180	1183	1189	rVB2	228	205	0.01%	0.002%
21	4.870	1189	1191	1193	rBV	146	90	0.01%	0.001%
22	4.886	1193	1196	1198	rBV2	120	73	0.01%	0.001%
23	4.940	1209	1213	1214	rBV	179	122	0.01%	0.001%
24	4.969	1218	1222	1224	rBV	106	93	0.01%	0.001%
25	5.040	1226	1244	1279	rBV2	555052	1452508	100.00%	11.950%
26	5.436	1363	1367	1369	rBV3	209	199	0.01%	0.002%
27	5.609	1408	1421	1465	rBV	563479	1151495	79.28%	9.473%
28	6.063	1548	1562	1599	rBV	313083	647445	44.57%	5.326%
29	6.304	1635	1637	1638	rBV	287	128	0.01%	0.001%
30	6.342	1648	1649	1650	rBV	128	37	0.00%	0.000%
31	6.352	1650	1652	1655	rVV2	134	85	0.01%	0.001%
32	6.387	1660	1663	1667	rVB2	183	157	0.01%	0.001%
33	6.468	1684	1688	1691	rBV3	219	189	0.01%	0.002%
34	6.503	1696	1699	1702	rBV2	174	119	0.01%	0.001%
35	6.616	1729	1734	1736	rBV3	722	672	0.05%	0.006%
36	6.706	1759	1762	1767	rVB4	389	301	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029586.D
 Acq On : 10 Dec 2022 17:12
 Operator : SY/MD
 Sample : N5928-21 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.728	1767	1769	1772	rVB	314	142	0.01%	0.001%
38	6.751	1772	1776	1779	rBV2	170	146	0.01%	0.001%
39	6.767	1779	1781	1784	rVB	165	68	0.00%	0.001%
40	6.792	1786	1789	1792	rBV2	115	78	0.01%	0.001%
41	6.815	1794	1796	1799	rVB2	309	162	0.01%	0.001%
42	6.870	1812	1813	1816	rVB	168	44	0.00%	0.000%
43	6.883	1816	1817	1820	rVB	136	34	0.00%	0.000%
44	6.902	1821	1823	1824	rBV	188	69	0.00%	0.001%
45	6.979	1832	1847	1882	rBV	143557	269925	18.58%	2.221%
46	7.137	1893	1896	1898	rBV2	473	272	0.02%	0.002%
47	7.310	1937	1950	1984	rBV	667583	1199212	82.56%	9.866%
48	7.612	2034	2044	2061	rBV	103482	180946	12.46%	1.489%
49	7.735	2078	2082	2086	rBV3	364	390	0.03%	0.003%
50	7.863	2121	2122	2125	rBV	232	82	0.01%	0.001%
51	8.082	2180	2190	2226	rBV	406861	728019	50.12%	5.989%
52	8.400	2287	2289	2292	rBV2	331	174	0.01%	0.001%
53	8.574	2340	2343	2345	rVB2	260	107	0.01%	0.001%
54	8.661	2368	2370	2374	rBV2	263	179	0.01%	0.001%
55	8.702	2379	2383	2386	rVV2	358	217	0.01%	0.002%
56	8.722	2386	2389	2392	rVV	199	161	0.01%	0.001%
57	8.741	2392	2395	2398	rVV2	310	181	0.01%	0.001%
58	8.767	2398	2403	2408	rVB	7594	5474	0.38%	0.045%
59	8.844	2415	2427	2447	rBV	824058	1349255	92.89%	11.100%
60	9.172	2527	2529	2530	rBV	153	60	0.00%	0.000%
61	9.185	2531	2533	2535	rVB2	197	80	0.01%	0.001%
62	9.320	2574	2575	2576	rVB2	109	21	0.00%	0.000%
63	9.333	2576	2579	2580	rBV	181	118	0.01%	0.001%
64	9.390	2594	2597	2600	rBV2	362	212	0.01%	0.002%
65	9.458	2616	2618	2621	rVB2	251	120	0.01%	0.001%
66	9.519	2635	2637	2638	rVB2	197	57	0.00%	0.000%
67	9.551	2643	2647	2655	rBV2	426	508	0.03%	0.004%
68	9.779	2716	2718	2721	rVB2	199	132	0.01%	0.001%
69	9.850	2738	2740	2744	rBV	203	186	0.01%	0.002%
70	9.963	2772	2775	2778	rBV	227	150	0.01%	0.001%
71	10.162	2827	2837	2841	rBV2	20968	30084	2.07%	0.247%
72	10.207	2842	2851	2878	rVB	462298	737853	50.80%	6.070%
73	10.374	2899	2903	2911	rVB3	522	595	0.04%	0.005%
74	10.471	2930	2933	2935	rBV	172	119	0.01%	0.001%
75	10.503	2941	2943	2944	rBV	168	86	0.01%	0.001%
76	10.567	2955	2963	2974	rBV	9791	15130	1.04%	0.124%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029586.D
 Acq On : 10 Dec 2022 17:12
 Operator : SY/MD
 Sample : N5928-21 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ90

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.702	3004	3005	3007	rBV2	195	73	0.01%	0.001%
78	10.738	3013	3016	3019	rBV	185	91	0.01%	0.001%
79	10.841	3044	3048	3053	rVB3	571	451	0.03%	0.004%
80	10.869	3053	3057	3062	rBV2	238	244	0.02%	0.002%
81	10.911	3067	3070	3072	rVV2	364	197	0.01%	0.002%
82	10.969	3086	3088	3092	rVB	509	236	0.02%	0.002%
83	11.017	3101	3103	3106	rVB2	283	110	0.01%	0.001%
84	11.040	3106	3110	3113	rBV2	287	285	0.02%	0.002%
85	11.120	3133	3135	3137	rVB2	215	87	0.01%	0.001%
86	11.140	3138	3141	3143	rBV2	235	173	0.01%	0.001%
87	11.236	3159	3171	3196	rBV	898345	1404757	96.71%	11.557%
88	11.455	3236	3239	3240	rBV	328	225	0.02%	0.002%
89	11.612	3275	3288	3310	rBV	722404	1140485	78.52%	9.383%
90	11.844	3358	3360	3363	rBV3	259	115	0.01%	0.001%
91	12.066	3426	3429	3434	rBV3	401	302	0.02%	0.002%
92	12.130	3446	3449	3454	rBV2	324	286	0.02%	0.002%
93	12.474	3551	3556	3562	rBV2	398	619	0.04%	0.005%
94	13.117	3751	3756	3758	rBV3	573	497	0.03%	0.004%




Sum of corrected areas: 12155305

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029586.D
Acq On : 10 Dec 2022 17:12
Operator : SY/MD
Sample : N5928-21 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 80 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

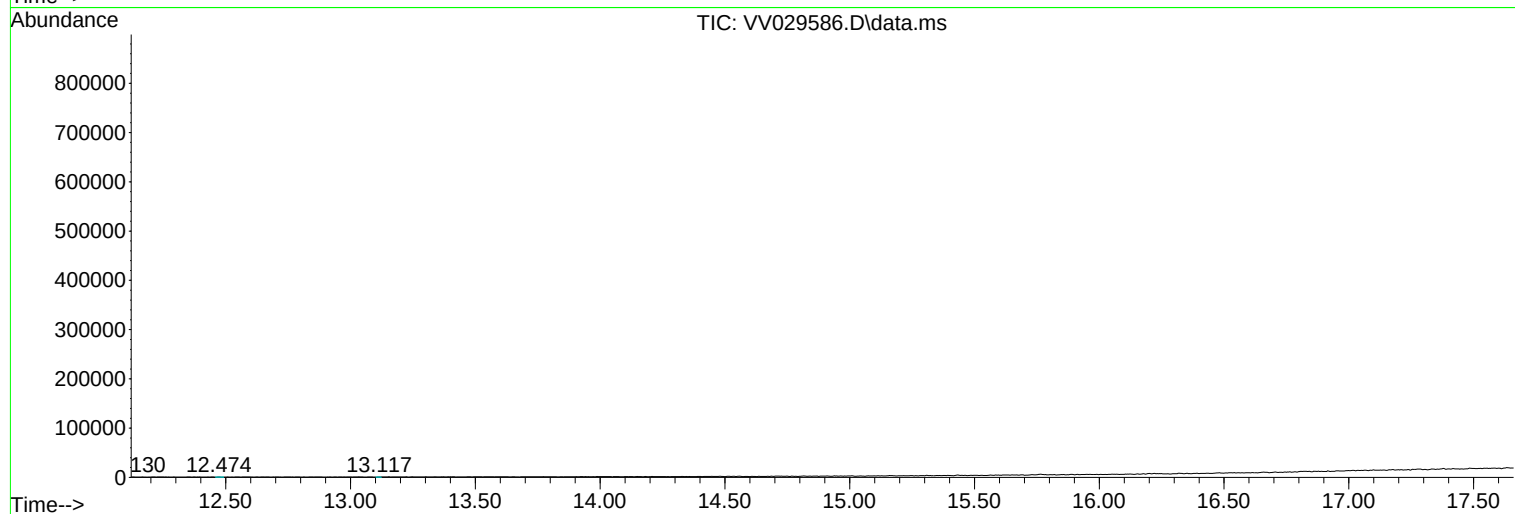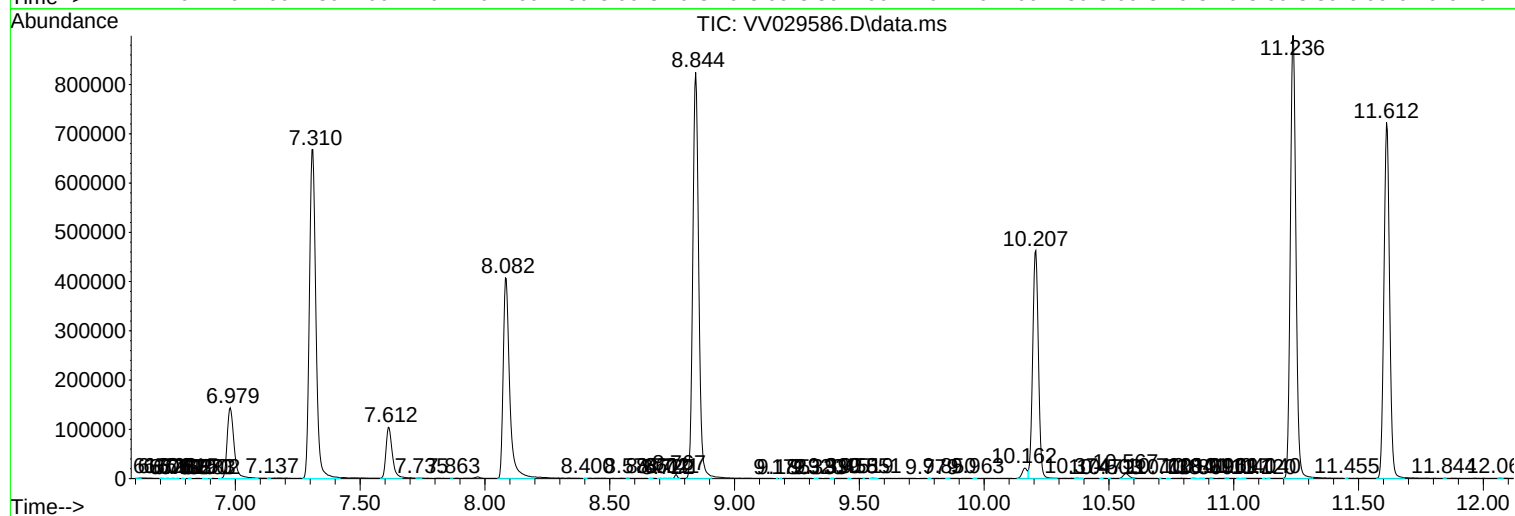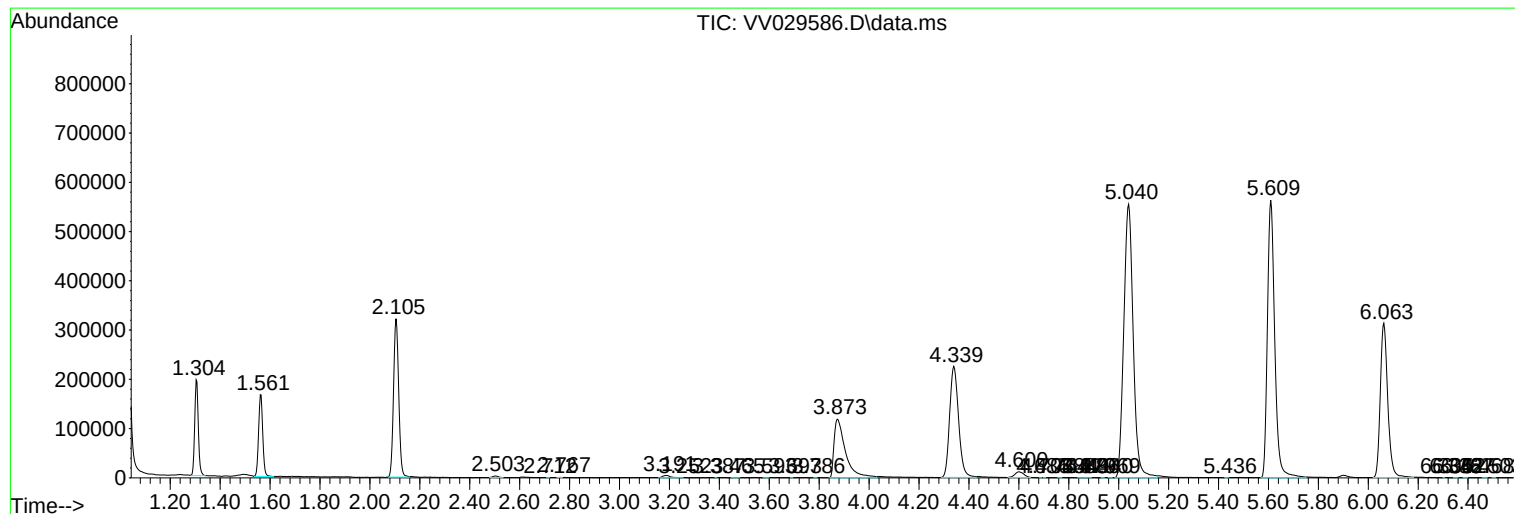

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029586.D
Acq On : 10 Dec 2022 17:12
Operator : SY/MD
Sample : N5928-21 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 80 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029586.D
Acq On : 10 Dec 2022 17:12
Operator : SY/MD
Sample : N5928-21 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 80 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------