


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029510.D
Acq On : 09 Dec 2022 08:50
Operator : SY/MD
Sample : BFB353
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB353

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Title : VOC Analysis
Last Update : Sat Dec 10 07:45:47 2022

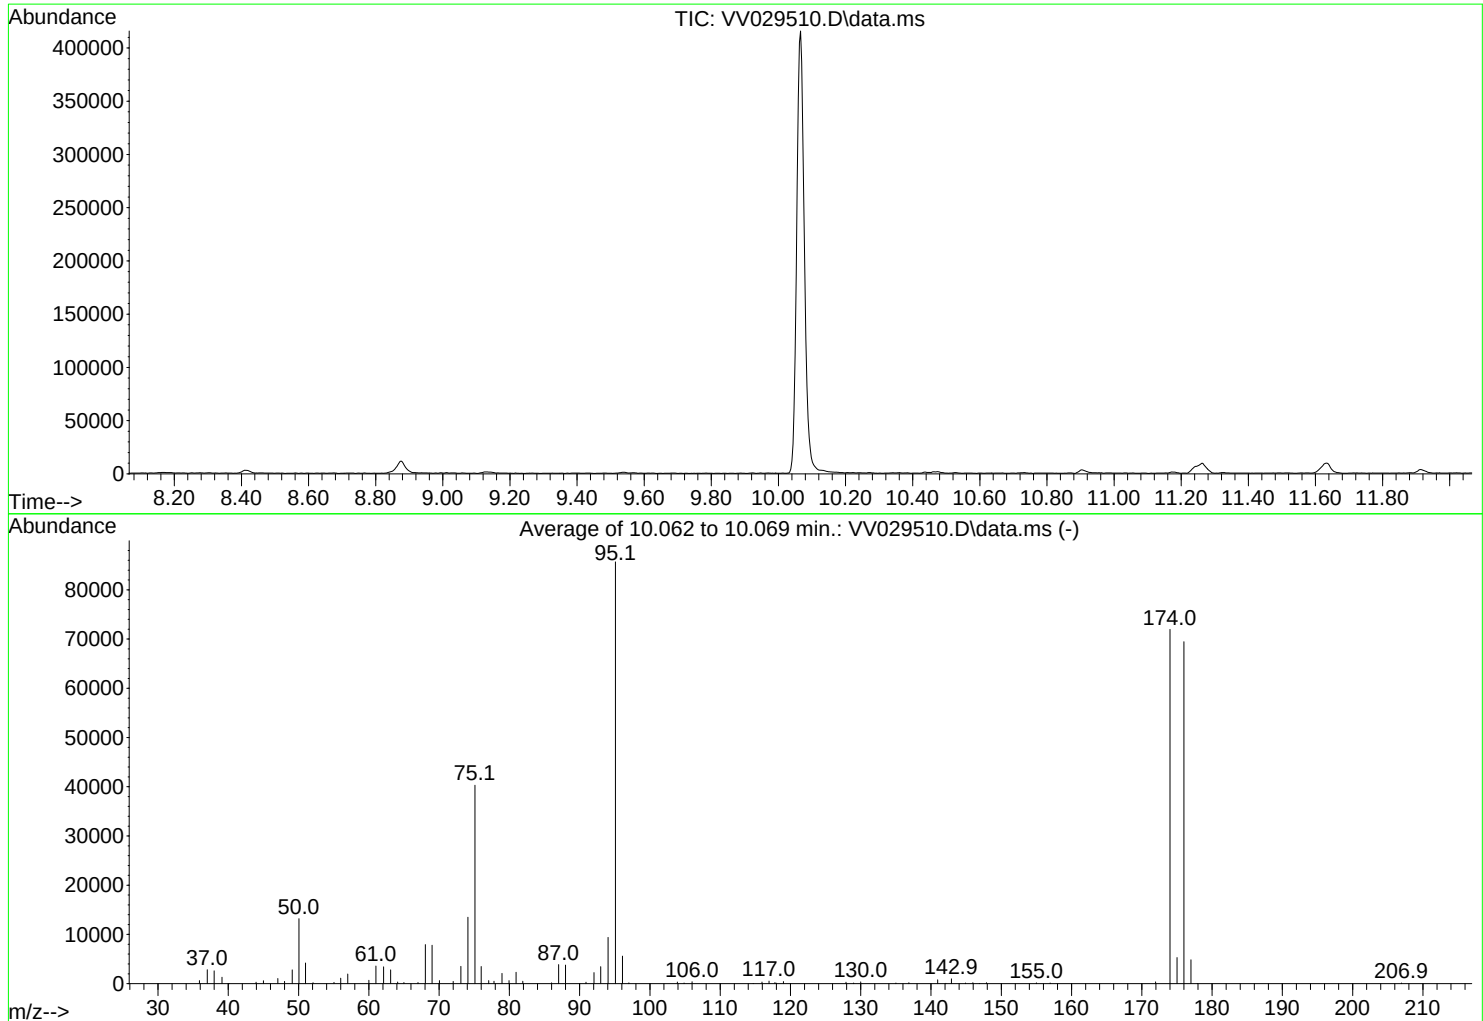

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	13213	PASS
75	95	30	80	47.0	40301	PASS
95	95	100	100	100.0	85688	PASS
96	95	5	9	6.5	5586	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.0	71960	PASS
175	174	5	9	7.3	5288	PASS
176	174	95	105	96.5	69456	PASS
177	176	5	10	7.0	4853	PASS

m/z	Abundance
40.00	222.0
44.00	366.0

Instrument :
MSVOA_V
ClientSampleId :
BFB353

m/z	Abundance
35.90	603.0
37.00	2973.0
38.00	2691.0
39.10	1231.0
40.00	238.0
43.90	629.0
45.00	628.0
47.00	1105.0
48.00	495.0
49.10	2912.0
50.00	13606.0
51.00	4436.0
52.10	216.0
55.00	281.0
56.00	1111.0
57.00	1971.0
60.00	716.0
61.00	3624.0
62.10	3578.0
63.10	2745.0
64.20	286.0
65.00	277.0
67.00	254.0
68.00	8216.0
69.00	7899.0
70.10	677.0
72.00	322.0
73.10	3613.0
74.10	13470.0
75.10	40864.0
76.00	3594.0
77.10	633.0
77.80	442.0
78.90	2201.0
80.00	677.0
80.90	2242.0
81.90	547.0
86.00	184.0
87.00	3966.0
88.00	4058.0
90.90	276.0
92.00	2298.0
93.00	3647.0
94.00	9462.0
95.10	87608.0
96.10	5634.0
97.00	184.0
103.90	361.0
104.80	134.0
106.00	399.0
116.00	357.0
117.00	559.0
117.80	328.0
119.00	465.0
127.90	319.0
129.00	140.0
130.00	350.0
135.00	130.0
136.90	191.0
141.00	803.0
142.10	106.0
142.90	966.0
144.90	113.0
146.00	190.0
147.90	230.0
155.00	175.0
157.10	131.0
172.10	355.0
174.00	70480.0
175.00	5294.0
176.00	68112.0
177.00	4729.0
177.90	121.0
206.90	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB353

m/z	Abundance
35.90	662.0
37.00	2921.0
38.00	2698.0
39.10	1335.0
40.00	238.0
43.90	659.0
45.00	597.0
47.10	1060.0
48.00	467.0
49.10	2923.0
50.10	13719.0
51.00	4299.0
52.10	204.0
55.10	277.0
56.00	1135.0
57.00	1986.0
60.00	684.0
61.00	3746.0
62.10	3526.0
63.10	2920.0
64.10	327.0
65.00	249.0
67.00	261.0
68.10	8194.0
69.00	8030.0
70.10	666.0
72.00	470.0
73.10	3623.0
74.10	14005.0
75.10	41688.0
76.00	3584.0
77.10	627.0
77.80	490.0
78.90	2173.0
80.00	614.0
81.00	2419.0
81.90	502.0
86.00	188.0
87.00	4005.0
88.00	3857.0
90.90	293.0
92.10	2333.0
93.00	3538.0
94.10	9687.0
95.10	88344.0
96.10	5807.0
97.00	172.0
103.90	340.0
104.90	153.0
106.00	402.0
115.90	357.0
117.00	504.0
117.80	352.0
119.00	442.0
127.90	302.0
129.00	146.0
130.00	368.0
135.00	146.0
136.80	201.0
140.90	808.0
142.10	112.0
142.90	1025.0
144.90	136.0
146.00	189.0
147.90	219.0
155.00	178.0
156.90	132.0
171.90	357.0
174.00	74520.0
175.00	5455.0
176.00	71680.0
177.00	5084.0
207.00	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB353

m/z	Abundance
35.90	634.0
37.00	2628.0
38.00	2407.0
39.10	1317.0
40.00	242.0
44.00	693.0
45.00	527.0
47.00	964.0
48.00	423.0
49.10	2586.0
50.10	12315.0
51.00	3850.0
52.00	150.0
55.10	216.0
56.00	1031.0
57.00	1896.0
60.00	627.0
61.00	3401.0
62.10	3158.0
63.10	2702.0
64.00	330.0
65.00	208.0
67.00	217.0
68.10	7409.0
69.00	7493.0
70.00	549.0
72.00	570.0
73.10	3295.0
74.10	12986.0
75.10	38352.0
76.00	3283.0
77.00	562.0
77.80	515.0
79.00	1908.0
79.90	535.0
81.00	2293.0
81.90	448.0
86.00	157.0
87.00	3610.0
88.00	3381.0
90.90	285.0
92.00	2114.0
93.00	3161.0
94.00	9017.0
95.10	81112.0
96.10	5318.0
97.00	150.0
103.90	281.0
104.90	154.0
106.00	350.0
114.70	116.0
115.90	291.0
116.90	488.0
118.00	318.0
119.00	384.0
127.90	285.0
129.00	137.0
130.00	353.0
135.00	140.0
136.80	175.0
140.90	786.0
142.90	949.0
144.90	109.0
145.90	167.0
146.90	104.0
147.90	182.0
155.00	154.0
156.80	143.0
171.90	349.0
174.00	70880.0
175.00	5115.0
176.00	68576.0
177.00	4745.0
207.00	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB353