


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121018\
Data File : VV008885.D
Acq On : 10 Dec 2018 10:09
Operator : SY/MD
Sample : BFB57
Misc : 25.0ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB57

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR120518WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Dec 11 03:21:37 2018

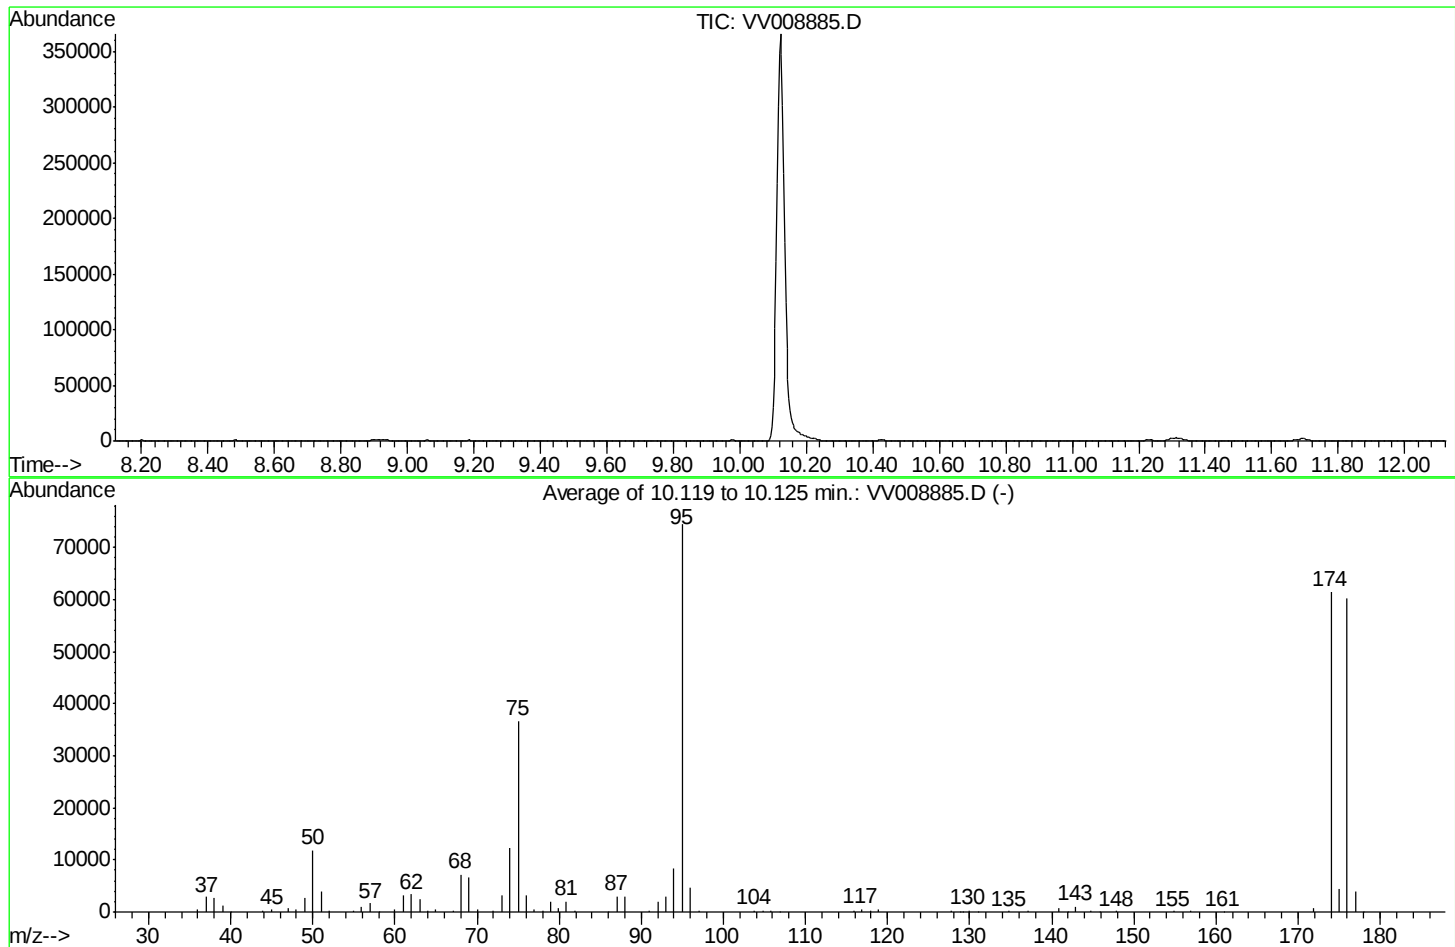

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	11926	PASS
75	95	30	80	49.3	36722	PASS
95	95	100	100	100.0	74461	PASS
96	95	5	9	6.4	4793	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.6	61530	PASS
175	174	5	9	7.4	4549	PASS
176	174	95	101	98.0	60322	PASS
177	176	5	9	6.6	4002	PASS

m/z	Abundance
36.00	540.0
37.00	2917.0
38.00	2613.0
39.00	1126.0
39.90	108.0
43.90	477.0
45.00	519.0
46.90	849.0
47.90	508.0
49.00	2690.0
50.00	11748.0
51.00	3852.0
52.00	160.0
54.90	189.0
55.90	940.0
57.00	1547.0
59.90	578.0
61.00	3257.0
62.00	3340.0
63.00	2615.0
64.00	296.0
65.00	393.0
67.00	168.0
68.00	7187.0
69.00	6798.0
70.00	443.0
72.00	284.0
73.00	3411.0
74.00	12409.0
75.00	36584.0
76.00	3102.0
77.00	422.0
78.00	323.0
78.90	2046.0
80.00	744.0
80.90	1970.0
81.90	349.0
87.00	3081.0
88.00	2719.0
90.90	320.0
92.00	1895.0
93.00	2969.0
94.00	8144.0
95.00	74376.0
96.00	4892.0
97.10	162.0
103.80	333.0
104.80	147.0
105.90	314.0
115.90	255.0
116.90	507.0
117.90	332.0
118.90	491.0
127.80	268.0
128.90	120.0
129.10	114.0
130.00	264.0
134.80	140.0
137.10	126.0
140.90	636.0
142.90	1002.0
144.80	204.0
147.90	172.0
154.80	158.0
156.90	134.0
160.90	116.0
171.90	729.0
174.00	59312.0
175.00	4598.0
176.00	58280.0
177.00	3859.0
177.90	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57

m/z	Abundance
44.00	191.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57

m/z	Abundance
35.90	447.0
37.10	2832.0
38.00	2576.0
39.00	1151.0
39.90	104.0
43.90	475.0
45.00	446.0
47.00	839.0
47.90	388.0
49.00	2710.0
50.00	11774.0
51.00	3650.0
52.10	160.0
54.90	142.0
56.00	946.0
57.00	1668.0
60.00	578.0
61.00	3137.0
62.00	3213.0
63.00	2450.0
64.10	411.0
64.90	432.0
67.10	170.0
68.00	6980.0
69.00	6575.0
70.00	541.0
71.90	263.0
73.00	3114.0
74.00	11759.0
75.00	35552.0
76.00	3066.0
77.00	380.0
78.10	303.0
79.00	2021.0
79.90	683.0
80.90	1988.0
81.80	369.0
85.90	135.0
87.00	2929.0
88.00	2813.0
90.90	329.0
92.00	1867.0
93.00	3026.0
94.00	8208.0
95.00	72120.0
96.00	4579.0
96.90	144.0
103.80	339.0
104.90	151.0
105.80	288.0
115.90	216.0
116.80	524.0
117.90	346.0
118.90	520.0
127.80	234.0
128.80	137.0
129.80	299.0
131.00	137.0
134.80	153.0
137.10	130.0
140.80	773.0
141.90	103.0
142.90	940.0
144.80	173.0
145.90	144.0
148.00	192.0
154.80	205.0
157.00	155.0
172.00	633.0
174.00	61752.0
175.00	4337.0
176.00	60320.0
177.00	4025.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57

m/z	Abundance
36.00	510.0
37.00	2985.0
38.00	2715.0
39.00	1214.0
43.90	499.0
45.00	495.0
46.90	887.0
47.90	475.0
49.00	2862.0
50.00	12258.0
51.00	3970.0
52.10	168.0
54.90	179.0
56.00	1023.0
57.00	1676.0
58.00	105.0
60.00	583.0
61.00	3389.0
62.00	3512.0
63.00	2559.0
64.00	353.0
64.90	417.0
67.10	160.0
68.00	7450.0
69.00	6811.0
70.00	492.0
71.90	278.0
73.00	3415.0
74.00	12628.0
75.00	38032.0
76.00	3252.0
77.00	446.0
78.10	353.0
78.90	2142.0
80.00	738.0
80.90	2036.0
81.80	374.0
85.90	120.0
87.00	3106.0
88.00	2983.0
90.90	354.0
92.00	1952.0
93.00	3147.0
94.00	8537.0
95.00	76888.0
96.00	4910.0
97.00	160.0
103.80	353.0
104.90	168.0
105.80	323.0
106.80	106.0
115.90	243.0
116.90	537.0
117.90	370.0
118.90	536.0
127.80	272.0
128.90	121.0
129.90	298.0
131.00	118.0
134.80	166.0
137.10	145.0
140.80	722.0
142.90	1047.0
144.80	204.0
145.90	115.0
148.00	193.0
154.90	190.0
157.00	127.0
171.90	708.0
174.00	63528.0
175.00	4714.0
176.00	62368.0
177.00	4123.0
178.00	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57