

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
 Data File : VV013986.D
 Acq On : 10 Dec 2019 14:34
 Operator : SY/MD
 Sample : K6202-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BZ3

Quant Time: Dec 11 01:25:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 11 00:25:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	731289	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	549693	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	220331	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	167576	39.62	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.24%
7) Chloroethane-d5	1.57	69	187726	42.52	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.04%
11) 1,1-Dichloroethene-d2	2.13	63	280068	29.95	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.90%#
21) 2-Butanone-d5	3.92	46	293208	98.49	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.49%
24) Chloroform-d	4.40	84	408931	46.04	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.08%
26) 1,2-Dichloroethane-d4	5.08	65	260220	46.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.46%
32) Benzene-d6	5.09	84	808794	56.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	113.56%
36) 1,2-Dichloropropane-d6	6.11	67	254986	59.64	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	119.28%
41) Toluene-d8	7.36	98	556053	42.82	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.64%
43) trans-1,3-Dichloropropene-	7.66	79	91036	43.76	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.52%
47) 2-Hexanone-d5	8.13	63	128905	80.74	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	80.74%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	263494	42.56	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.12%
64) 1,2-Dichlorobenzene-d4	11.67	152	218939	50.59	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.18%


Target Compounds					Ovalue
13) Acetone	2.18	43	93828	21.508 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121019\
Data File : VV013986.D
Acq On : 10 Dec 2019 14:34
Operator : SY/MD
Sample : K6202-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ3

Quant Time: Dec 11 01:25:43 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 11 00:25:42 2019
Response via : Initial Calibration

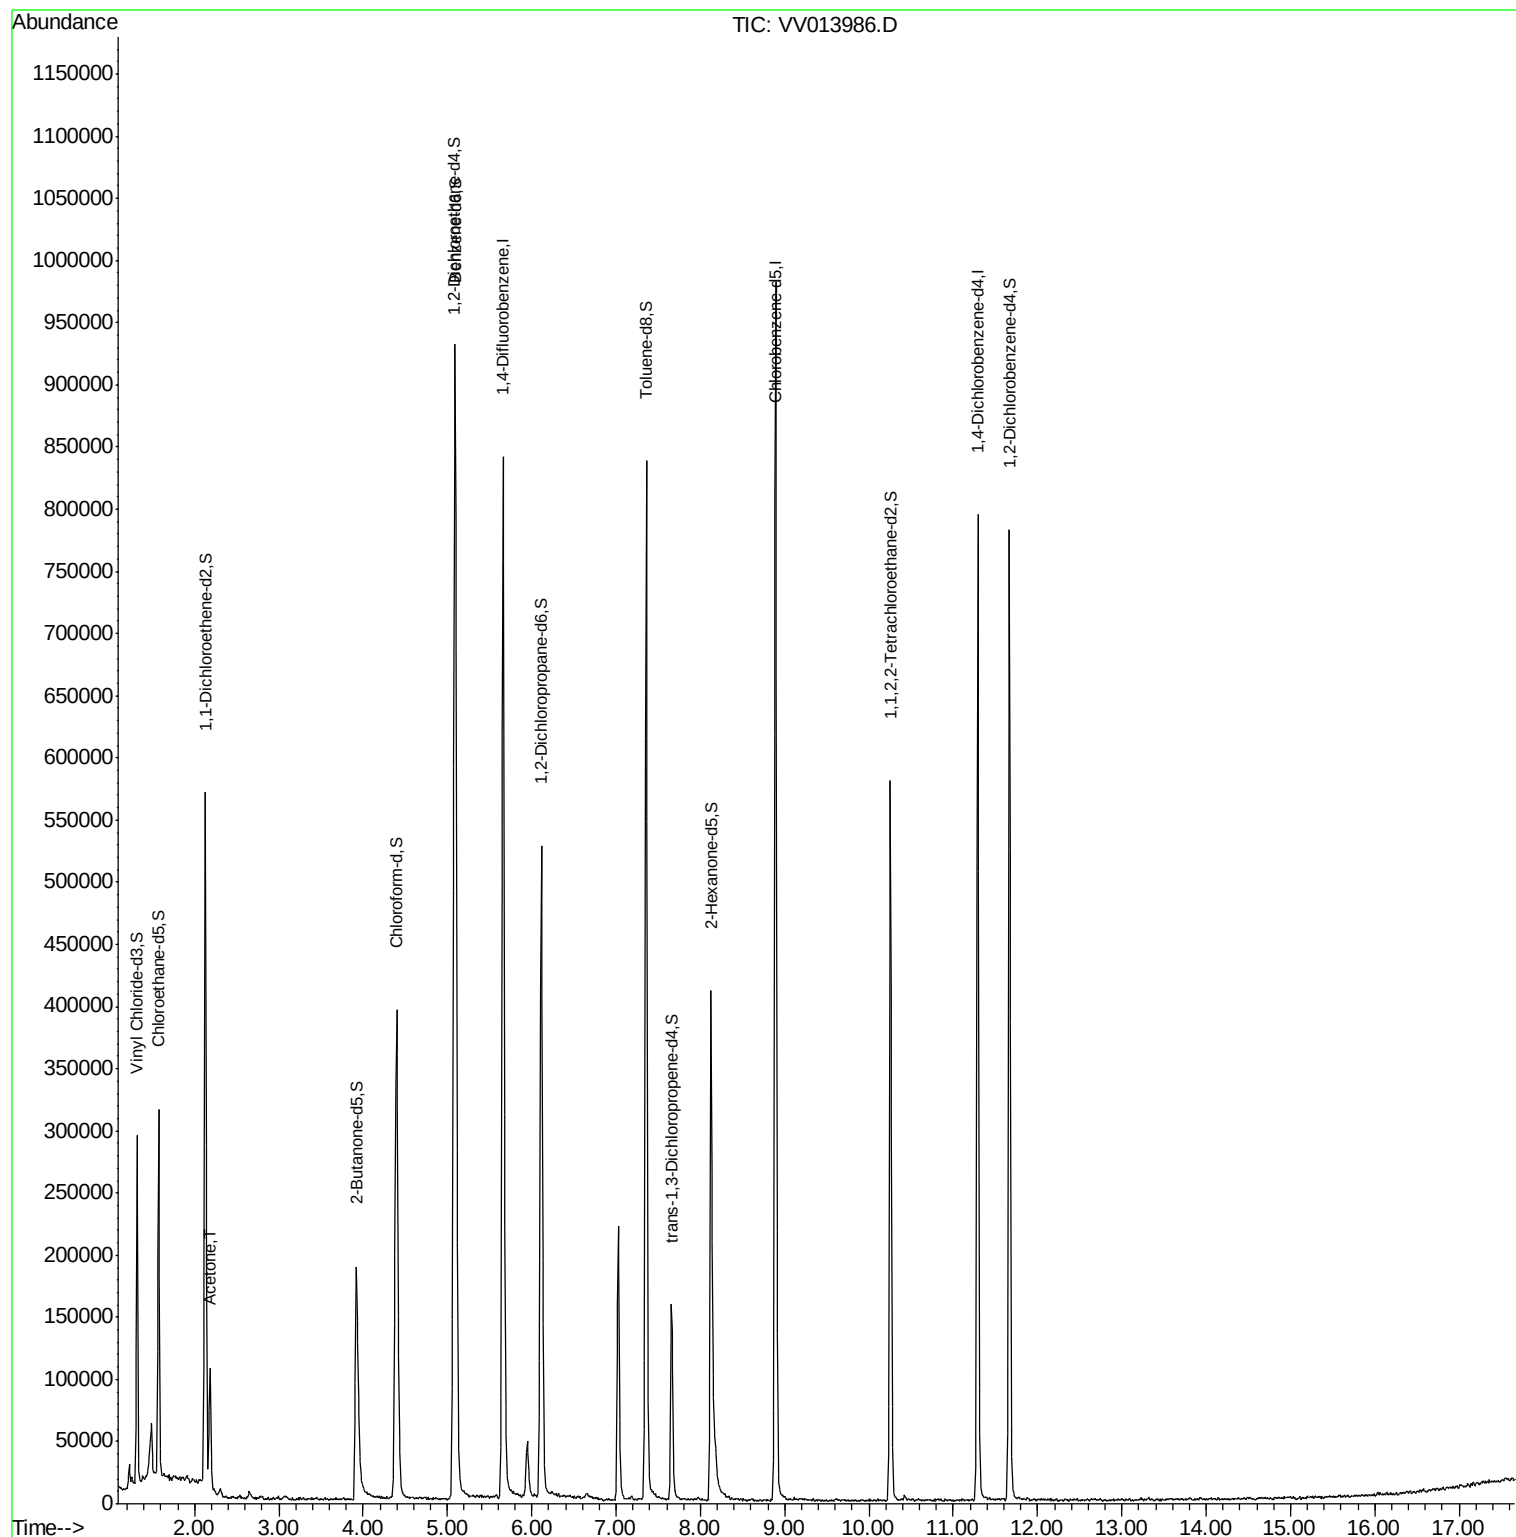

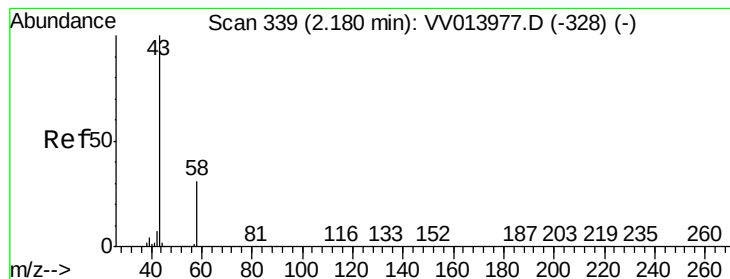

#13

Acetone

Concen: 21.508 ug/L

RT: 2.18 min Scan# 340

Delta R.T. 0.00 min

Lab File: VV013986.D

Acq: 10 Dec 2019 14:34


Instrument :
MSVOA_V
ClientSampleId :
C0BZ3

Tot Ion: 43 Resp: 93828

Ion Ratio Lower Upper

43 100

58 32.1 0.0 60.8

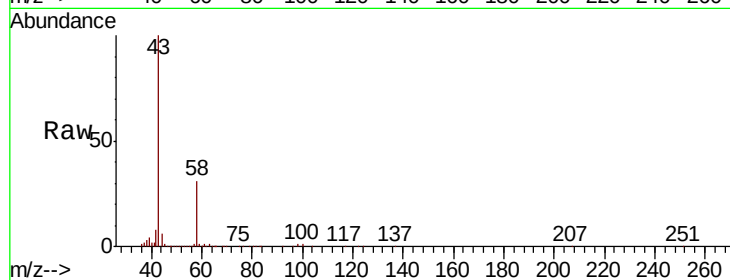

Abundance Ion 43.00 (42.70 to 43.70): VV0

Ion 58.00 (57.70 to 58.70): VV0

