

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
 Data File : VV013987.D
 Acq On : 10 Dec 2019 14:58
 Operator : SY/MD
 Sample : K6202-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BZ6

Quant Time: Dec 11 01:28:55 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 11 00:25:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	596826	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	539805	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	220119	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	157194	45.54	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	91.08%
7) Chloroethane-d5	1.57	69	175558	48.73	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.46%
11) 1,1-Dichloroethene-d2	2.13	63	258351	33.85	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.70%
21) 2-Butanone-d5	3.92	46	231870	95.44	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.44%
24) Chloroform-d	4.40	84	327491	45.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.36%
26) 1,2-Dichloroethane-d4	5.08	65	207596	45.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.38%
32) Benzene-d6	5.09	84	648668	46.37	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.74%
36) 1,2-Dichloropropane-d6	6.11	67	191444	45.60	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.20%
41) Toluene-d8	7.36	98	526520	41.29	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.58%
43) trans-1,3-Dichloropropene-	7.66	79	83308	40.78	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.56%
47) 2-Hexanone-d5	8.13	63	122839	78.35	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	78.35%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	249734	41.08	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	82.16%
64) 1,2-Dichlorobenzene-d4	11.67	152	210660	48.73	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.46%


Target Compounds					Ovalue
13) Acetone	2.18	43	69211	19.439 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
Data File : VV013987.D
Acq On : 10 Dec 2019 14:58
Operator : SY/MD
Sample : K6202-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ6

Quant Time: Dec 11 01:28:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 11 00:25:42 2019
Response via : Initial Calibration

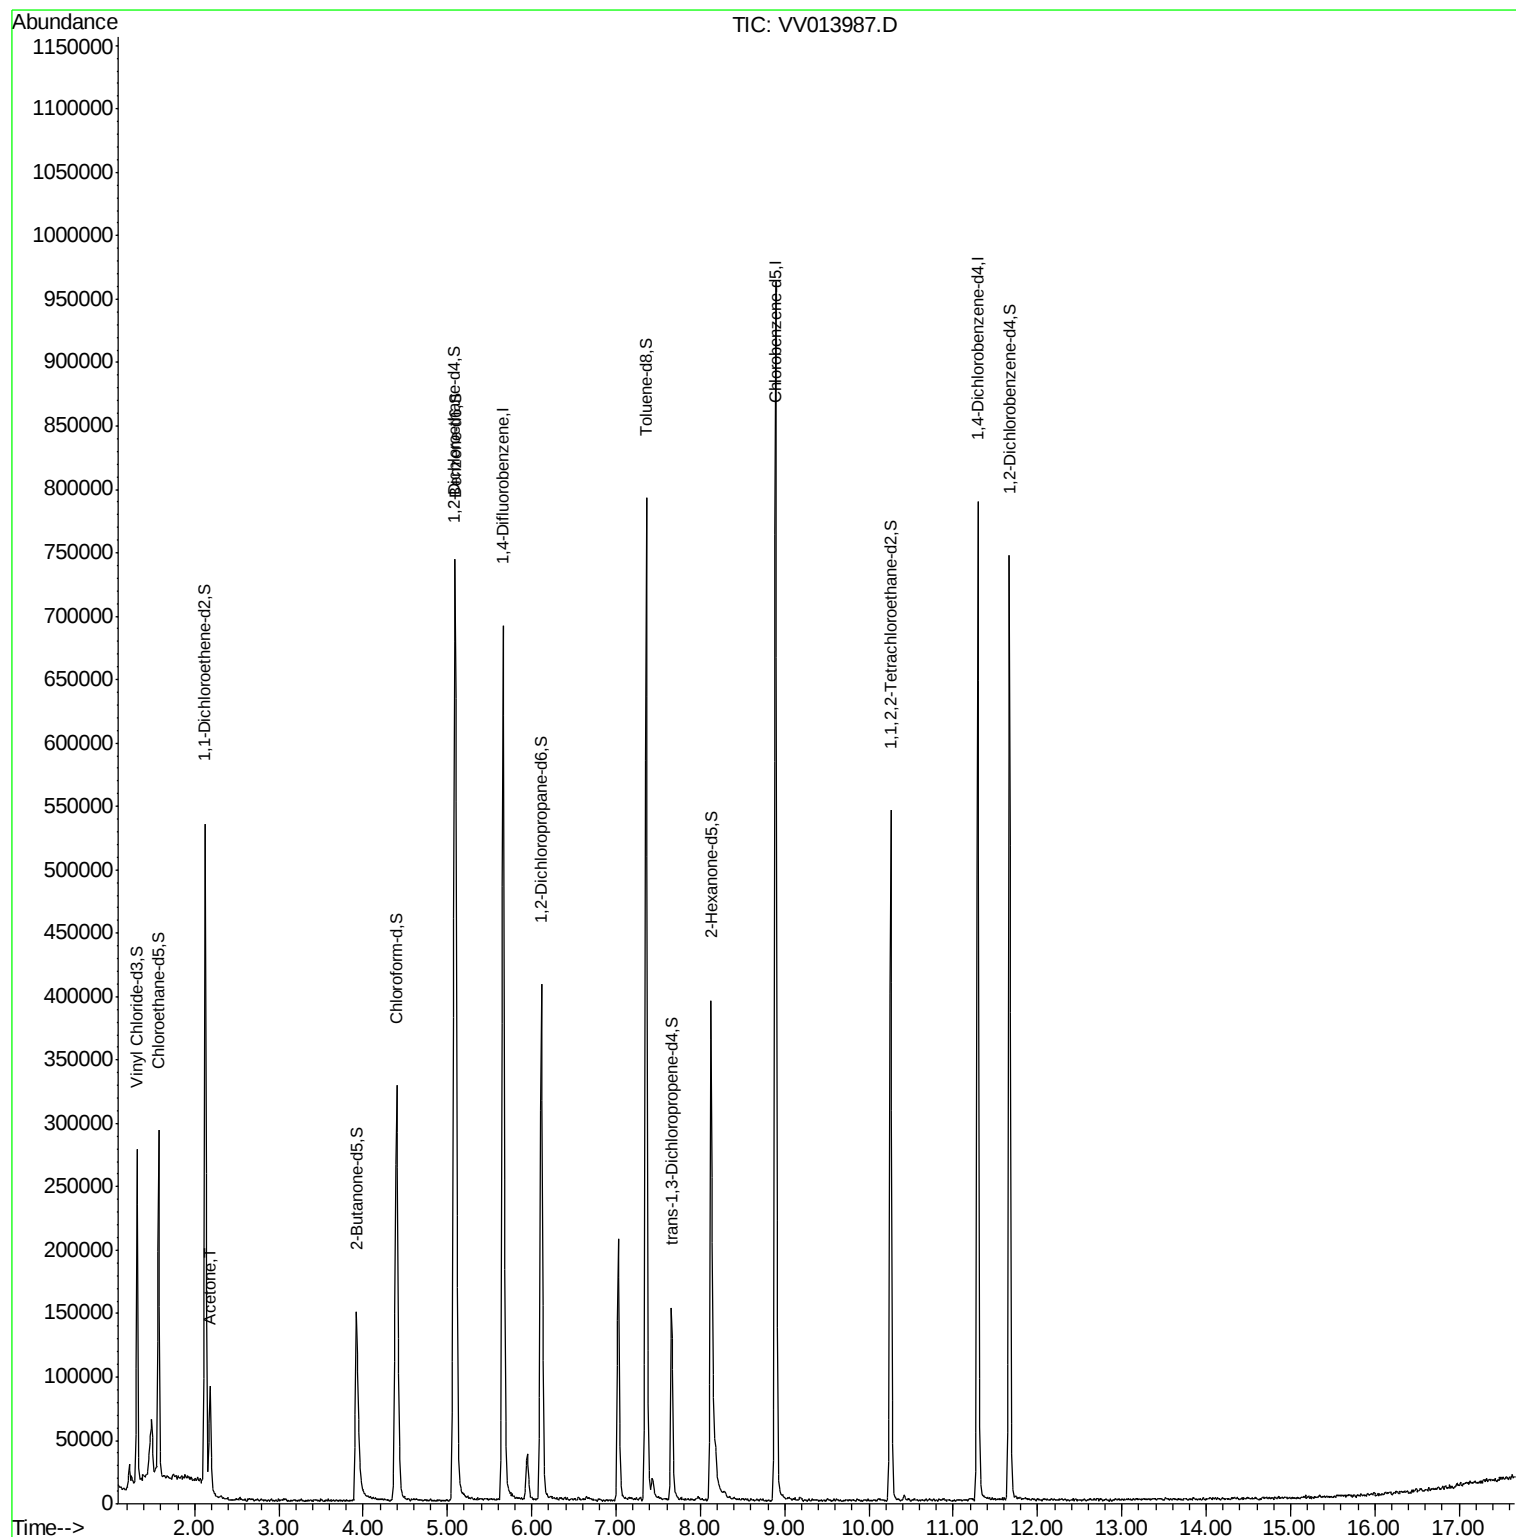

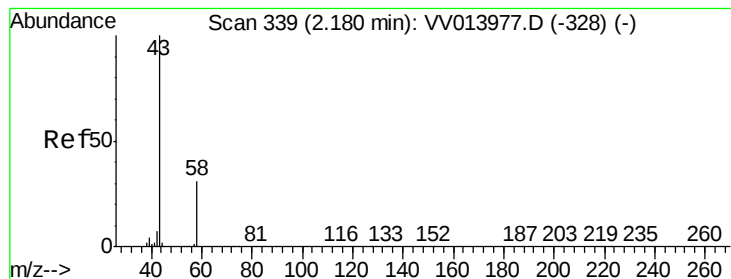

#13
Acetone
Concen: 19.439 ug/L
RT: 2.18 min Scan# 340
Delta R.T. 0.00 min
Lab File: VV013987.D
Acq: 10 Dec 2019 14:58

Instrument :
MSVOA_V
ClientSampleId :
C0BZ6

Tot Ion: 43 Resp: 69211
Ion Ratio Lower Upper
43 100
58 32.4 0.0 60.8

