

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
 Data File : VV013988.D
 Acq On : 10 Dec 2019 15:22
 Operator : SY/MD
 Sample : K6202-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C00

Quant Time: Dec 11 01:32:18 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 11 00:25:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	615426	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	571397	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	222872	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	159815	44.90	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.80%
7) Chloroethane-d5	1.57	69	175936	47.36	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.72%
11) 1,1-Dichloroethene-d2	2.13	63	266479	33.86	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.72%
21) 2-Butanone-d5	3.92	46	230657	92.07	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.07%
24) Chloroform-d	4.40	84	329759	44.12	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.24%
26) 1,2-Dichloroethane-d4	5.08	65	209716	44.28	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.56%
32) Benzene-d6	5.09	84	655493	44.27	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.54%
36) 1,2-Dichloropropane-d6	6.11	67	202603	45.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.18%
41) Toluene-d8	7.36	98	534598	39.61	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	79.22%#
43) trans-1,3-Dichloropropene-	7.66	79	86166	39.84	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.68%
47) 2-Hexanone-d5	8.13	63	124640	75.10	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	75.10%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	251165	39.03	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	78.06%
64) 1,2-Dichlorobenzene-d4	11.67	152	216849	49.54	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.08%


Target Compounds					Ovalue
13) Acetone	2.18	43	18818	5.126 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121019\
Data File : VV013988.D
Acq On : 10 Dec 2019 15:22
Operator : SY/MD
Sample : K6202-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C00

Quant Time: Dec 11 01:32:18 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 11 00:25:42 2019
Response via : Initial Calibration

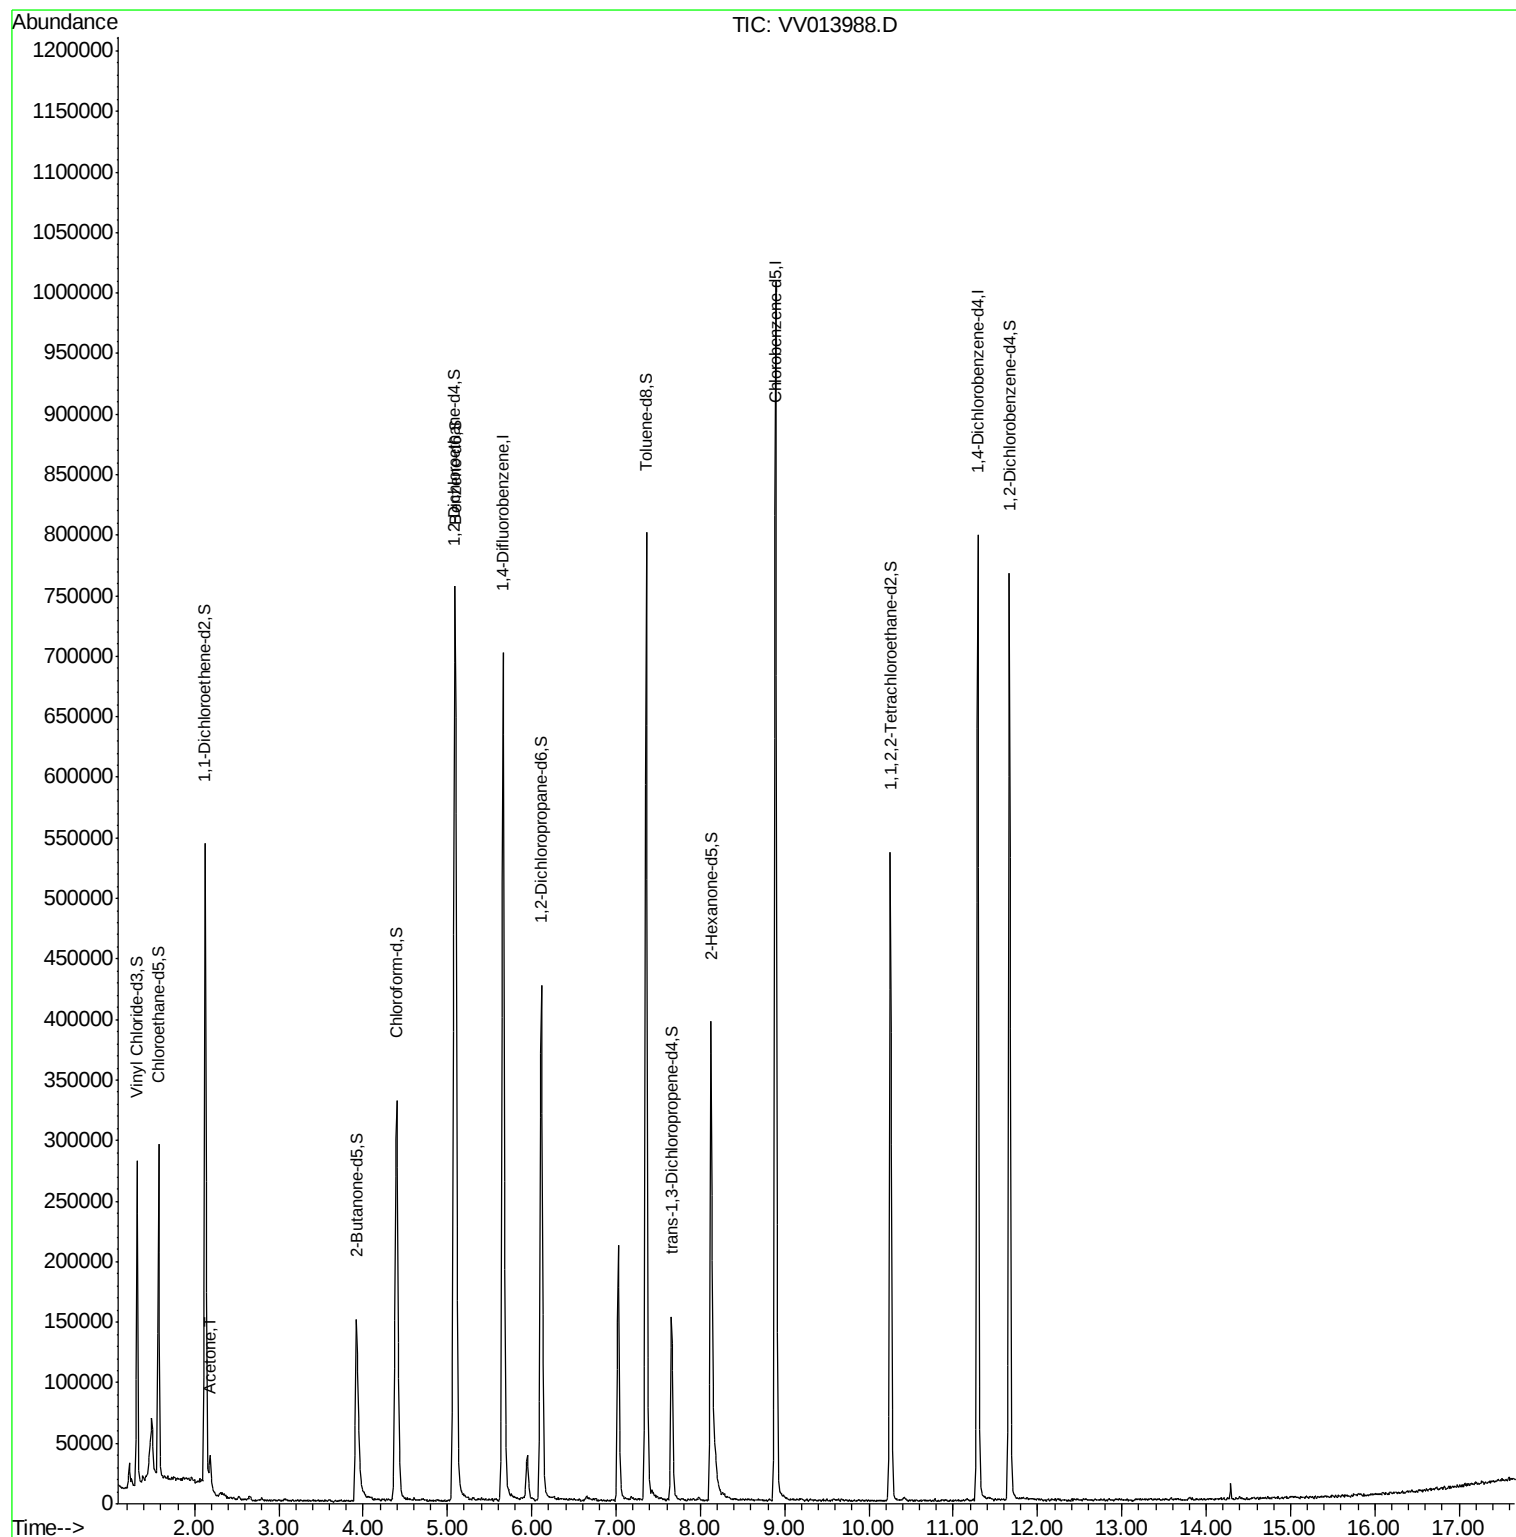

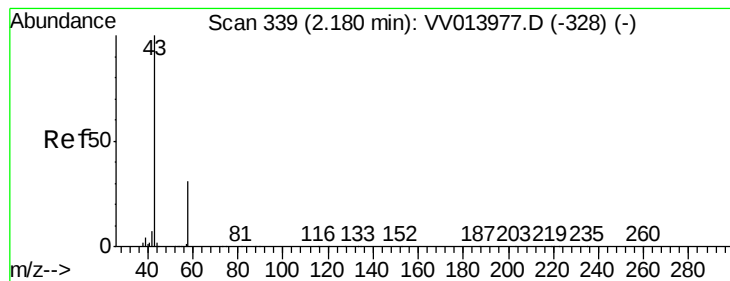

#13
 Acetone
 Concen: 5.126 ug/L
 RT: 2.18 min Scan# 340
 Delta R.T. 0.00 min
 Lab File: VV013988.D
 Acq: 10 Dec 2019 15:22

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C00

Tot Ion: 43 Resp: 18818
 Ion Ratio Lower Upper
 43 100
 58 31.3 0.0 60.8

