

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
 Data File : VV013990.D
 Acq On : 10 Dec 2019 16:11
 Operator : SY/MD
 Sample : K6202-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C04

Quant Time: Dec 11 02:19:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 11 00:25:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	591642	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	557452	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	230478	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	158213	46.24	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.48%
7) Chloroethane-d5	1.57	69	182911	51.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	102.42%
11) 1,1-Dichloroethene-d2	2.13	63	268666	35.51	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.02%
21) 2-Butanone-d5	3.92	46	282983	117.50	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	117.50%
24) Chloroform-d	4.40	84	371054	51.64	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.28%
26) 1,2-Dichloroethane-d4	5.08	65	218834	48.06	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.12%
32) Benzene-d6	5.09	84	680653	47.12	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.24%
36) 1,2-Dichloropropane-d6	6.11	67	200436	46.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.46%
41) Toluene-d8	7.35	98	546119	41.47	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.94%
43) trans-1,3-Dichloropropene-	7.66	79	86047	40.78	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.56%
47) 2-Hexanone-d5	8.13	63	131676	81.33	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	81.33%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	271969	43.32	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.64%
64) 1,2-Dichlorobenzene-d4	11.67	152	223764	49.43	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.86%


Target Compounds					Ovalue
13) Acetone	2.18	43	7339	2.079 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121019\
Data File : VV013990.D
Acq On : 10 Dec 2019 16:11
Operator : SY/MD
Sample : K6202-10
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C04

Quant Time: Dec 11 02:19:20 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 11 00:25:42 2019
Response via : Initial Calibration

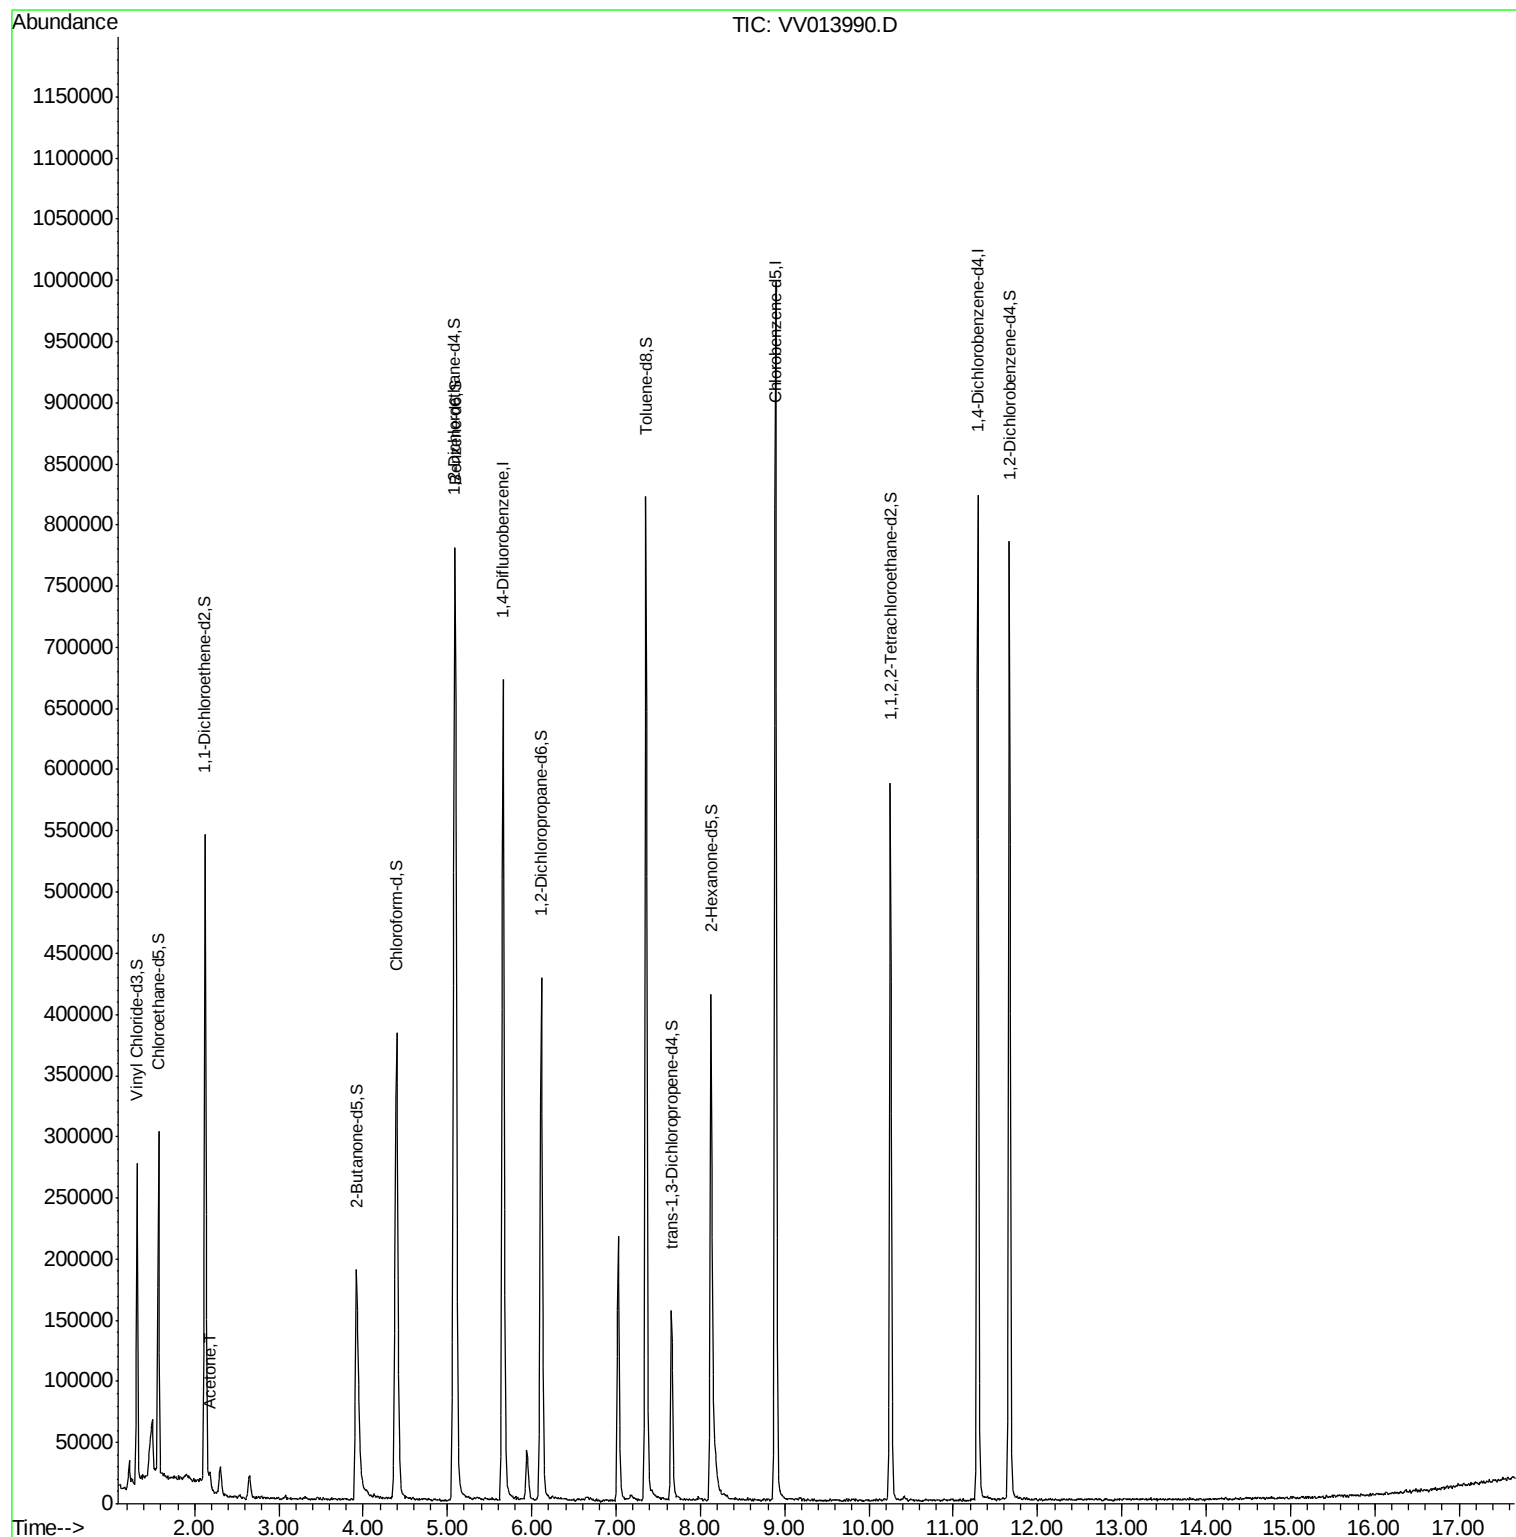

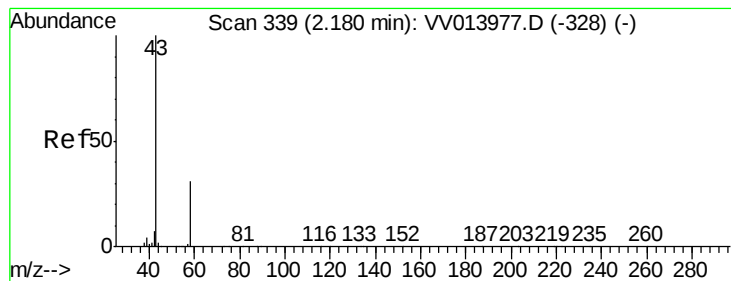

#13
 Acetone
 Concen: 2.079 ug/L
 RT: 2.18 min Scan# 340
 Delta R.T. 0.00 min
 Lab File: VV013990.D
 Acq: 10 Dec 2019 16:11

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C04

Tot Ion: 43 Resp: 7339
 Ion Ratio Lower Upper
 43 100
 58 34.8 0.0 60.8

