

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
 Data File : VV013987.D
 Acq On : 10 Dec 2019 14:58
 Operator : SY/MD
 Sample : K6202-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BZ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	83	rVB	261012	253581	13.55%	1.785%
2	1.573	144	150	165	rVB	272965	315433	16.86%	2.220%
3	2.126	314	322	333	rBV	512264	699203	37.37%	4.922%
4	2.631	476	479	481	rBV3	1923	1286	0.07%	0.009%
5	2.827	537	540	543	rBV2	930	743	0.04%	0.005%
6	2.878	551	556	559	rBV6	917	702	0.04%	0.005%
7	2.955	578	580	584	rVB3	932	485	0.03%	0.003%
8	2.994	589	592	595	rBV5	1667	1262	0.07%	0.009%
9	3.106	624	627	631	rVB3	1152	623	0.03%	0.004%
10	3.151	639	641	644	rBV4	1007	499	0.03%	0.004%
11	3.174	644	648	650	rBV4	713	548	0.03%	0.004%
12	3.235	662	667	671	rBV5	1164	1358	0.07%	0.010%
13	3.254	671	673	676	rBV3	1249	944	0.05%	0.007%
14	3.322	689	694	699	rBV6	1283	1361	0.07%	0.010%
15	3.344	699	701	705	rBV3	1153	883	0.05%	0.006%
16	3.409	719	721	723	rBV3	809	531	0.03%	0.004%
17	3.499	745	749	750	rBV3	1493	726	0.04%	0.005%
18	3.586	774	776	778	rBV2	1473	599	0.03%	0.004%
19	3.608	778	783	787	rVV6	1285	1332	0.07%	0.009%
20	3.643	791	794	797	rBV5	1345	872	0.05%	0.006%
21	3.672	801	803	805	rBV	1036	483	0.03%	0.003%
22	3.721	815	818	821	rVB5	1432	940	0.05%	0.007%
23	3.762	828	831	832	rBV2	773	471	0.03%	0.003%
24	3.791	837	840	845	rVV5	1343	1062	0.06%	0.007%
25	3.856	857	860	863	rVB2	869	473	0.03%	0.003%
26	3.920	870	880	909	rBV	148768	391158	20.91%	2.753%
27	4.396	1010	1028	1054	rBV2	327468	789281	42.19%	5.556%
28	4.569	1079	1082	1083	rBV3	1034	608	0.03%	0.004%
29	4.634	1100	1102	1104	rBV	959	499	0.03%	0.004%
30	4.872	1174	1176	1180	rBV3	815	566	0.03%	0.004%
31	4.984	1208	1211	1213	rBV2	1115	679	0.04%	0.005%
32	5.026	1220	1224	1226	rBV3	784	639	0.03%	0.004%
33	5.090	1227	1244	1271	rBV2	741798	1870861	100.00%	13.169%
34	5.338	1317	1321	1323	rBV4	1647	1296	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
 Data File : VV013987.D
 Acq On : 10 Dec 2019 14:58
 Operator : SY/MD
 Sample : K6202-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BZ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	5.582	1395	1397	1399	rBV4	1080	543	0.03%	0.004%
36	5.659	1408	1421	1444	rBV	688917	1347004	72.00%	9.481%
37	6.113	1549	1562	1582	rBV	405221	817880	43.72%	5.757%
38	6.328	1626	1629	1632	rBV4	1768	1328	0.07%	0.009%
39	6.380	1642	1645	1646	rBV3	1426	920	0.05%	0.006%
40	6.550	1696	1698	1701	rBV4	2053	1484	0.08%	0.010%
41	6.605	1712	1715	1719	rBV4	1026	831	0.04%	0.006%
42	6.788	1768	1772	1776	rBV5	1422	1385	0.07%	0.010%
43	6.827	1782	1784	1787	rVB3	1625	805	0.04%	0.006%
44	6.846	1787	1790	1791	rBV3	1302	865	0.05%	0.006%
45	6.910	1808	1810	1813	rBV3	1126	673	0.04%	0.005%
46	6.952	1818	1823	1826	rBV6	781	929	0.05%	0.007%
47	7.026	1835	1846	1861	rBV	206007	366752	19.60%	2.581%
48	7.357	1935	1949	1965	rBV	790945	1364599	72.94%	9.605%
49	7.659	2033	2043	2071	rVB	151631	262966	14.06%	1.851%
50	7.756	2071	2073	2076	rBV2	1219	750	0.04%	0.005%
51	7.945	2130	2132	2135	rBV3	1281	825	0.04%	0.006%
52	8.084	2173	2175	2177	rBV3	967	516	0.03%	0.004%
53	8.126	2178	2188	2222	rVV2	393536	829562	44.34%	5.839%
54	8.531	2312	2314	2316	rBV3	1147	599	0.03%	0.004%
55	8.585	2327	2331	2332	rBV3	951	670	0.04%	0.005%
56	8.769	2384	2388	2392	rVB3	1323	929	0.05%	0.007%
57	8.794	2392	2396	2397	rBV3	827	468	0.03%	0.003%
58	8.807	2397	2400	2403	rVB3	1001	630	0.03%	0.004%
59	8.891	2411	2426	2447	rBV	961978	1550258	82.86%	10.912%
60	9.122	2496	2498	2501	rVB4	1822	798	0.04%	0.006%
61	9.280	2542	2547	2548	rBV3	1561	1139	0.06%	0.008%
62	9.367	2572	2574	2580	rVB7	919	759	0.04%	0.005%
63	9.508	2613	2618	2620	rBV4	1438	961	0.05%	0.007%
64	9.582	2637	2641	2643	rBV3	1414	1212	0.06%	0.009%
65	9.656	2661	2664	2665	rBV2	1047	545	0.03%	0.004%
66	9.762	2694	2697	2699	rBV2	1116	785	0.04%	0.006%
67	9.804	2706	2710	2712	rBV4	1116	1084	0.06%	0.008%
68	9.859	2724	2727	2730	rBV5	1338	1144	0.06%	0.008%
69	9.987	2762	2767	2769	rBV4	1494	1127	0.06%	0.008%
70	9.997	2769	2770	2773	rVB3	1278	597	0.03%	0.004%
71	10.064	2784	2791	2793	rBV7	1282	1409	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
 Data File : VV013987.D
 Acq On : 10 Dec 2019 14:58
 Operator : SY/MD
 Sample : K6202-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BZ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	10.116	2804	2807	2811	rBV5	1552	906	0.05%	0.006%
73	10.257	2838	2851	2866	rBV	544222	858429	45.88%	6.042%
74	10.601	2953	2958	2961	rBV4	935	909	0.05%	0.006%
75	10.659	2974	2976	2978	rBV2	1006	529	0.03%	0.004%
76	10.826	3025	3028	3031	rBV5	1348	968	0.05%	0.007%
77	10.945	3062	3065	3067	rVV4	767	534	0.03%	0.004%
78	11.035	3090	3093	3096	rBV3	677	629	0.03%	0.004%
79	11.113	3114	3117	3118	rBV2	947	562	0.03%	0.004%
80	11.190	3136	3141	3142	rBV3	1532	1233	0.07%	0.009%
81	11.289	3159	3172	3189	rBV	788218	1232360	65.87%	8.674%
82	11.579	3259	3262	3265	rBV4	1986	1128	0.06%	0.008%
83	11.666	3276	3289	3307	rBV	744403	1187297	63.46%	8.357%
84	11.990	3388	3390	3392	rBV3	933	509	0.03%	0.004%
85	12.350	3500	3502	3505	rBV2	1020	729	0.04%	0.005%
86	12.389	3512	3514	3516	rBV3	836	449	0.02%	0.003%
87	12.424	3523	3525	3527	rVB3	1331	456	0.02%	0.003%
88	12.447	3530	3532	3535	rBV3	948	662	0.04%	0.005%
89	12.482	3539	3543	3545	rBV3	1306	887	0.05%	0.006%
90	12.531	3556	3558	3561	rBV2	1174	834	0.04%	0.006%
91	12.669	3598	3601	3605	rBV4	1304	1240	0.07%	0.009%
92	12.743	3619	3624	3627	rBV6	1633	1849	0.10%	0.013%
93	12.778	3633	3635	3637	rBV2	854	437	0.02%	0.003%
94	12.862	3658	3661	3665	rVB5	1727	1201	0.06%	0.008%
95	12.884	3665	3668	3670	rBV2	1079	633	0.03%	0.004%
96	13.000	3702	3704	3707	rVB3	1060	500	0.03%	0.004%
97	13.157	3751	3753	3757	rBV4	1101	1061	0.06%	0.007%
98	13.730	3929	3931	3932	rBV2	1248	566	0.03%	0.004%
99	13.903	3982	3985	3987	rBV4	1496	1014	0.05%	0.007%
100	13.958	3999	4002	4003	rBV2	1108	726	0.04%	0.005%


Sum of corrected areas: 14206955

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121019\
Data File : VV013987.D
Acq On : 10 Dec 2019 14:58
Operator : SY/MD
Sample : K6202-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

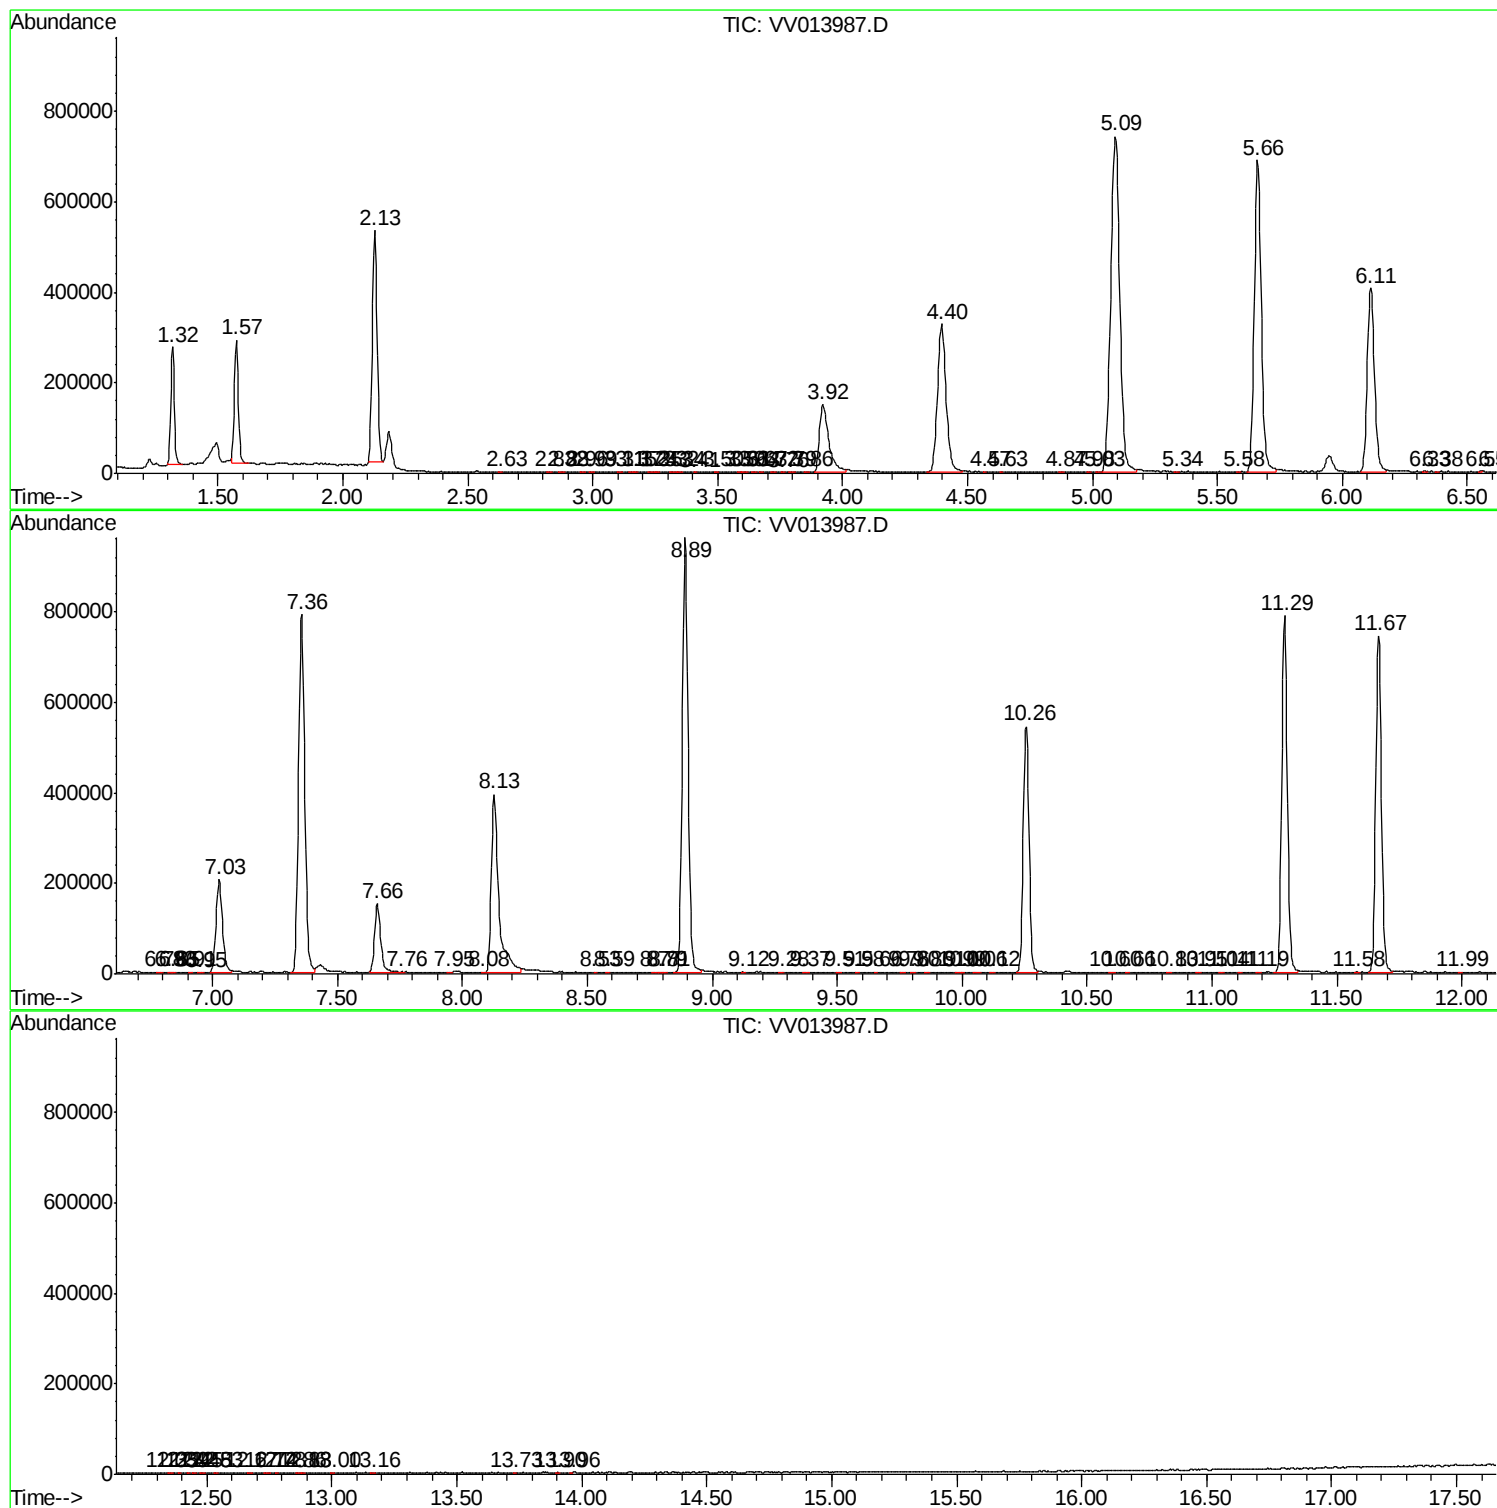

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121019\
Data File : VV013987.D
Acq On : 10 Dec 2019 14:58
Operator : SY/MD
Sample : K6202-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121019\
Data File : VV013987.D
Acq On : 10 Dec 2019 14:58
Operator : SY/MD
Sample : K6202-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BZ6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc