

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
 Data File : VV013989.D
 Acq On : 10 Dec 2019 15:47
 Operator : SY/MD
 Sample : K6202-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	82	rVB	258202	250794	13.27%	1.715%
2	1.566	142	148	160	rVB	270987	314474	16.64%	2.150%
3	2.126	313	322	334	rVB	494809	703797	37.24%	4.812%
4	2.624	470	477	478	rBV5	1815	1875	0.10%	0.013%
5	2.852	543	548	551	rBV5	1154	999	0.05%	0.007%
6	2.971	583	585	587	rBV3	1015	416	0.02%	0.003%
7	3.058	604	612	613	rBV5	2666	2703	0.14%	0.018%
8	3.122	630	632	633	rBV2	861	362	0.02%	0.002%
9	3.171	644	647	650	rBV4	1287	821	0.04%	0.006%
10	3.206	655	658	660	rBV3	892	503	0.03%	0.003%
11	3.264	673	676	677	rBV2	604	301	0.02%	0.002%
12	3.296	684	686	690	rVB3	1043	697	0.04%	0.005%
13	3.360	704	706	711	rBV4	1337	1351	0.07%	0.009%
14	3.441	729	731	733	rVB3	1139	472	0.02%	0.003%
15	3.460	733	737	742	rVB5	1203	1015	0.05%	0.007%
16	3.483	742	744	745	rBV2	1083	402	0.02%	0.003%
17	3.521	754	756	760	rVB5	677	375	0.02%	0.003%
18	3.537	760	761	763	rVB2	616	160	0.01%	0.001%
19	3.550	763	765	766	rVB3	588	179	0.01%	0.001%
20	3.560	766	768	770	rVB	746	224	0.01%	0.002%
21	3.576	770	773	775	rBV2	679	450	0.02%	0.003%
22	3.614	782	785	786	rBV4	919	477	0.03%	0.003%
23	3.663	799	800	803	rVB2	970	377	0.02%	0.003%
24	3.782	834	837	838	rBV3	1052	604	0.03%	0.004%
25	3.794	839	841	846	rVV3	1727	1159	0.06%	0.008%
26	3.814	846	847	849	rVV2	334	126	0.01%	0.001%
27	3.833	849	853	859	rVV8	1138	1195	0.06%	0.008%
28	3.920	869	880	902	rBV	150833	386061	20.43%	2.640%
29	4.171	956	958	960	rVB2	1423	579	0.03%	0.004%
30	4.296	995	997	998	rBV2	1013	398	0.02%	0.003%
31	4.396	1009	1028	1054	rBV	315380	797080	42.17%	5.450%
32	4.698	1119	1122	1123	rBV3	986	447	0.02%	0.003%
33	4.785	1146	1149	1151	rBV2	1157	757	0.04%	0.005%
34	4.798	1151	1153	1158	rVB3	1341	1070	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
 Data File : VV013989.D
 Acq On : 10 Dec 2019 15:47
 Operator : SY/MD
 Sample : K6202-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	4.836	1163	1165	1166	rBV3	900	426	0.02%	0.003%
36	4.846	1166	1168	1170	rVB3	1033	257	0.01%	0.002%
37	4.856	1170	1171	1173	rBV2	686	245	0.01%	0.002%
38	4.907	1185	1187	1188	rBV2	1066	415	0.02%	0.003%
39	4.997	1208	1215	1219	rBV7	1434	1615	0.09%	0.011%
40	5.019	1219	1222	1223	rBV3	1250	775	0.04%	0.005%
41	5.090	1226	1244	1274	rBV2	743943	1889943	100.00%	12.922%
42	5.560	1388	1390	1392	rBV3	1897	846	0.04%	0.006%
43	5.659	1407	1421	1447	rBV	684103	1356697	71.79%	9.276%
44	6.113	1549	1562	1585	rVB2	410403	831263	43.98%	5.684%
45	6.486	1676	1678	1685	rBV4	1891	1589	0.08%	0.011%
46	6.762	1762	1764	1765	rBV2	1179	429	0.02%	0.003%
47	6.878	1798	1800	1801	rBV	1225	436	0.02%	0.003%
48	6.923	1812	1814	1815	rBV2	957	403	0.02%	0.003%
49	6.958	1820	1825	1826	rBV3	804	539	0.03%	0.004%
50	7.026	1830	1846	1861	rBV	208699	381976	20.21%	2.612%
51	7.357	1936	1949	1962	rBV	821618	1404904	74.34%	9.606%
52	7.659	2034	2043	2061	rVB	155817	253485	13.41%	1.733%
53	7.836	2095	2098	2100	rBV3	1681	1224	0.06%	0.008%
54	8.061	2166	2168	2170	rVB3	1126	386	0.02%	0.003%
55	8.125	2178	2188	2218	rBV2	426860	869785	46.02%	5.947%
56	8.637	2345	2347	2348	rBV2	1180	496	0.03%	0.003%
57	8.666	2354	2356	2358	rBV3	874	542	0.03%	0.004%
58	8.746	2377	2381	2383	rBV5	1614	893	0.05%	0.006%
59	8.820	2400	2404	2406	rBV4	1083	896	0.05%	0.006%
60	8.833	2406	2408	2410	rBV3	868	342	0.02%	0.002%
61	8.891	2414	2426	2445	rVV	999450	1593580	84.32%	10.896%
62	9.286	2547	2549	2551	rBV2	1219	476	0.03%	0.003%
63	9.354	2569	2570	2575	rVB2	1617	913	0.05%	0.006%
64	9.386	2575	2580	2583	rBV4	1774	1479	0.08%	0.010%
65	9.540	2626	2628	2630	rBV2	805	296	0.02%	0.002%
66	9.553	2630	2632	2634	rVB2	1424	517	0.03%	0.004%
67	9.569	2634	2637	2638	rBV2	876	493	0.03%	0.003%
68	9.633	2655	2657	2658	rBV2	980	500	0.03%	0.003%
69	9.656	2662	2664	2667	rBV4	1409	900	0.05%	0.006%
70	10.010	2771	2774	2775	rBV2	980	600	0.03%	0.004%
71	10.051	2786	2787	2790	rBV3	1246	770	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
 Data File : VV013989.D
 Acq On : 10 Dec 2019 15:47
 Operator : SY/MD
 Sample : K6202-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	10.068	2790	2792	2793	rVV2	923	269	0.01%	0.002%
73	10.113	2802	2806	2807	rBV3	891	539	0.03%	0.004%
74	10.193	2828	2831	2834	rBV3	1353	801	0.04%	0.005%
75	10.254	2834	2850	2872	rBV	602950	941485	49.82%	6.437%
76	10.585	2951	2953	2959	rBV5	1520	1482	0.08%	0.010%
77	10.678	2979	2982	2983	rBV2	517	317	0.02%	0.002%
78	10.691	2984	2986	2992	rVB7	1431	1003	0.05%	0.007%
79	10.807	3020	3022	3025	rBV3	981	524	0.03%	0.004%
80	10.839	3030	3032	3034	rBV2	850	321	0.02%	0.002%
81	10.932	3059	3061	3062	rBV2	1088	396	0.02%	0.003%
82	11.119	3116	3119	3124	rBV5	1668	1646	0.09%	0.011%
83	11.289	3160	3172	3192	rBV	831209	1306899	69.15%	8.936%
84	11.534	3246	3248	3252	rBV3	1181	812	0.04%	0.006%
85	11.559	3253	3256	3263	rVV9	2144	2818	0.15%	0.019%
86	11.666	3277	3289	3313	rBV	817221	1285857	68.04%	8.792%
87	12.209	3456	3458	3461	rBV4	1131	644	0.03%	0.004%
88	12.267	3474	3476	3478	rBV3	1390	589	0.03%	0.004%
89	12.286	3478	3482	3484	rVV3	2156	1412	0.07%	0.010%
90	12.318	3488	3492	3493	rBV2	1834	1056	0.06%	0.007%
91	12.929	3680	3682	3683	rBV2	1225	470	0.02%	0.003%
92	12.987	3698	3700	3702	rBV2	1310	635	0.03%	0.004%
93	13.251	3778	3782	3787	rVB7	1991	1647	0.09%	0.011%


Sum of corrected areas: 14625653

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121019\
Data File : VV013989.D
Acq On : 10 Dec 2019 15:47
Operator : SY/MD
Sample : K6202-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0C02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

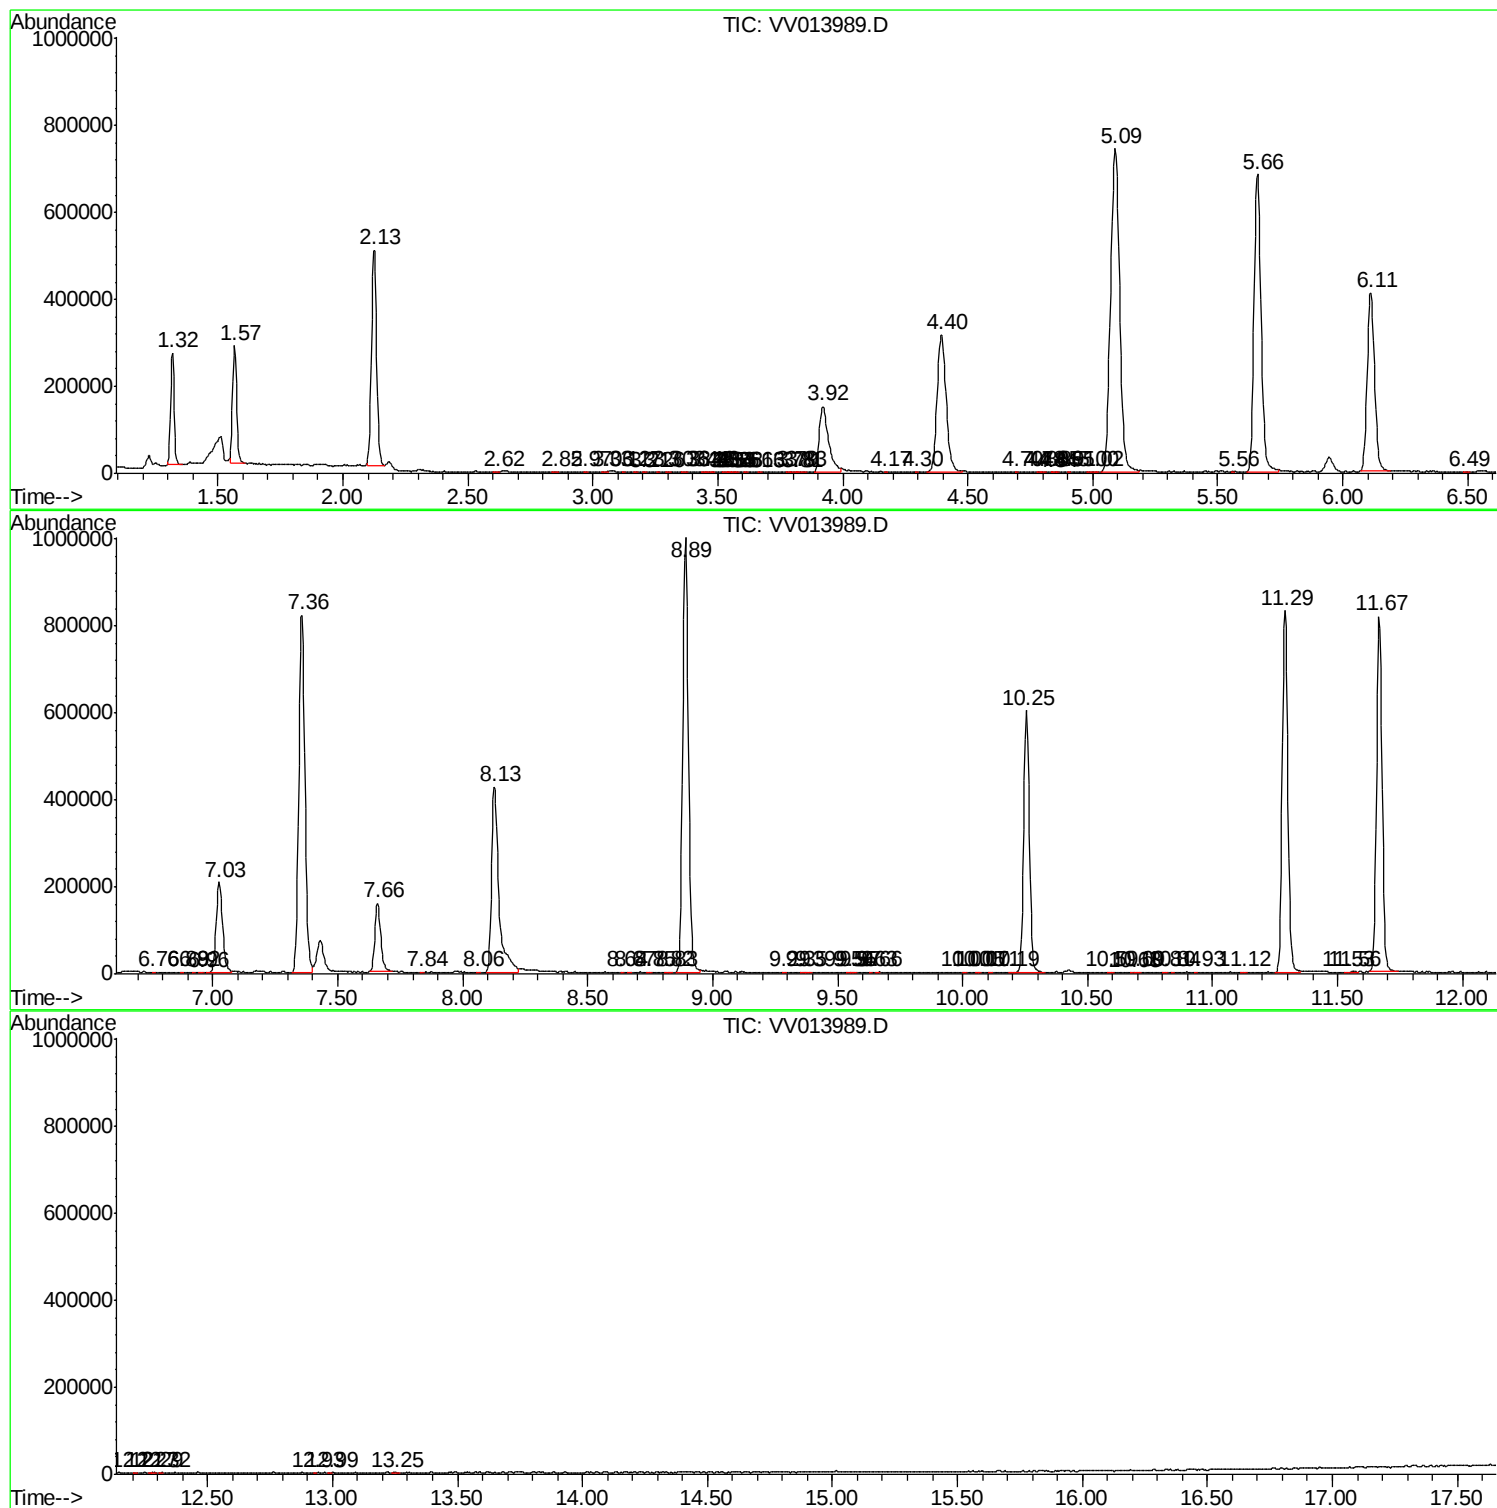

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121019\
Data File : VV013989.D
Acq On : 10 Dec 2019 15:47
Operator : SY/MD
Sample : K6202-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121019\
Data File : VV013989.D
Acq On : 10 Dec 2019 15:47
Operator : SY/MD
Sample : K6202-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C02

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc