

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
 Data File : VV013998.D
 Acq On : 10 Dec 2019 19:50
 Operator : SY/MD
 Sample : K6200-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	80	rVB	236902	225303	12.53%	1.597%
2	1.573	144	150	160	rVB	250639	288859	16.06%	2.047%
3	2.126	314	322	336	rVB	485039	673580	37.46%	4.773%
4	2.508	439	441	444	rBV3	1438	848	0.05%	0.006%
5	2.579	462	463	465	rBV2	751	396	0.02%	0.003%
6	2.901	559	563	566	rVB4	1667	1380	0.08%	0.010%
7	2.920	566	569	572	rBV3	1302	1136	0.06%	0.008%
8	2.981	585	588	591	rVB5	1615	1029	0.06%	0.007%
9	2.997	591	593	596	rBV3	598	411	0.02%	0.003%
10	3.016	596	599	601	rVB4	1145	658	0.04%	0.005%
11	3.081	615	619	620	rBV3	1040	757	0.04%	0.005%
12	3.148	638	640	642	rBV2	798	447	0.02%	0.003%
13	3.200	654	656	662	rBV6	901	840	0.05%	0.006%
14	3.261	673	675	676	rVB2	629	177	0.01%	0.001%
15	3.277	676	680	681	rBV4	1235	849	0.05%	0.006%
16	3.348	696	702	706	rBV8	1406	1538	0.09%	0.011%
17	3.412	718	722	723	rBV4	1153	637	0.04%	0.005%
18	3.431	725	728	732	rVV4	1220	1065	0.06%	0.008%
19	3.470	737	740	744	rBV3	1212	1053	0.06%	0.007%
20	3.518	753	755	759	rBV3	947	717	0.04%	0.005%
21	3.537	759	761	764	rBV2	1182	666	0.04%	0.005%
22	3.557	764	767	768	rBV2	612	295	0.02%	0.002%
23	3.585	774	776	780	rVB4	1536	1006	0.06%	0.007%
24	3.608	780	783	784	rBV2	777	415	0.02%	0.003%
25	3.627	786	789	791	rBV2	1289	819	0.05%	0.006%
26	3.659	796	799	800	rBV2	739	416	0.02%	0.003%
27	3.692	808	809	810	rBV	989	202	0.01%	0.001%
28	3.772	832	834	835	rBV2	1094	287	0.02%	0.002%
29	3.827	845	851	854	rVB8	1699	1725	0.10%	0.012%
30	3.846	854	857	859	rBV3	1027	545	0.03%	0.004%
31	3.923	869	881	902	rBV	156550	401594	22.33%	2.846%
32	4.283	991	993	995	rBV3	1168	593	0.03%	0.004%
33	4.338	1004	1010	1011	rBV5	2315	2047	0.11%	0.015%
34	4.396	1013	1028	1056	rVB2	310941	748527	41.62%	5.304%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
 Data File : VV013998.D
 Acq On : 10 Dec 2019 19:50
 Operator : SY/MD
 Sample : K6200-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	4.601	1088	1092	1094	rBV2	1526	1107	0.06%	0.008%
36	4.727	1129	1131	1134	rBV4	1387	760	0.04%	0.005%
37	4.753	1137	1139	1141	rVV3	1092	463	0.03%	0.003%
38	4.888	1176	1181	1185	rBV6	1574	1187	0.07%	0.008%
39	4.910	1185	1188	1190	rBV2	1096	764	0.04%	0.005%
40	4.978	1207	1209	1211	rBV	989	471	0.03%	0.003%
41	5.000	1214	1216	1219	rBV2	677	438	0.02%	0.003%
42	5.090	1226	1244	1275	rBV2	703544	1798356	100.00%	12.744%
43	5.659	1408	1421	1450	rBV	667615	1314231	73.08%	9.313%
44	6.113	1548	1562	1589	rBV	383799	784835	43.64%	5.562%
45	6.482	1675	1677	1680	rVB4	1049	517	0.03%	0.004%
46	6.592	1705	1711	1714	rBV6	1211	1695	0.09%	0.012%
47	6.650	1725	1729	1736	rBV9	3840	4534	0.25%	0.032%
48	6.814	1778	1780	1783	rBV2	1473	865	0.05%	0.006%
49	6.852	1790	1792	1795	rBV2	927	438	0.02%	0.003%
50	6.881	1799	1801	1803	rBV2	759	277	0.02%	0.002%
51	6.942	1818	1820	1821	rBV2	1014	450	0.03%	0.003%
52	7.026	1835	1846	1860	rBV	199665	348131	19.36%	2.467%
53	7.254	1914	1917	1921	rBV5	1250	839	0.05%	0.006%
54	7.357	1937	1949	1970	rBV	757078	1307468	72.70%	9.265%
55	7.659	2033	2043	2061	rBV	141911	241746	13.44%	1.713%
56	7.775	2077	2079	2082	rBV3	1067	865	0.05%	0.006%
57	8.125	2178	2188	2220	rBV2	426553	884059	49.16%	6.265%
58	8.576	2325	2328	2329	rBV2	961	551	0.03%	0.004%
59	8.891	2414	2426	2446	rBV	1005106	1611212	89.59%	11.418%
60	9.138	2499	2503	2505	rBV5	1655	1300	0.07%	0.009%
61	9.296	2550	2552	2554	rBV3	1247	556	0.03%	0.004%
62	9.373	2573	2576	2578	rBV3	794	535	0.03%	0.004%
63	9.408	2584	2587	2589	rBV4	996	431	0.02%	0.003%
64	9.444	2594	2598	2601	rBV4	1412	1152	0.06%	0.008%
65	9.514	2617	2620	2621	rBV2	757	476	0.03%	0.003%
66	9.540	2625	2628	2630	rBV2	1052	759	0.04%	0.005%
67	9.566	2633	2636	2637	rBV3	1040	541	0.03%	0.004%
68	9.614	2648	2651	2654	rVB3	1733	1035	0.06%	0.007%
69	9.630	2654	2656	2660	rBV4	1271	895	0.05%	0.006%
70	9.669	2663	2668	2673	rBV5	1236	1081	0.06%	0.008%
71	9.691	2673	2675	2678	rBV4	1289	1078	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
 Data File : VV013998.D
 Acq On : 10 Dec 2019 19:50
 Operator : SY/MD
 Sample : K6200-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF24

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	9.778	2697	2702	2704	rBV6	1905	1725	0.10%	0.012%
73	9.830	2715	2718	2719	rBV3	1282	616	0.03%	0.004%
74	10.058	2784	2789	2793	rBV5	1947	2303	0.13%	0.016%
75	10.080	2793	2796	2798	rBV2	1102	670	0.04%	0.005%
76	10.113	2805	2806	2809	rBV3	882	456	0.03%	0.003%
77	10.254	2839	2850	2869	rBV	568295	888012	49.38%	6.293%
78	10.492	2921	2924	2926	rVB4	1093	555	0.03%	0.004%
79	10.505	2926	2928	2930	rBV3	965	596	0.03%	0.004%
80	10.582	2950	2952	2953	rBV2	1060	433	0.02%	0.003%
81	10.627	2959	2966	2967	rBV6	1146	1096	0.06%	0.008%
82	10.897	3048	3050	3054	rBV4	936	575	0.03%	0.004%
83	11.032	3089	3092	3095	rVB4	1347	863	0.05%	0.006%
84	11.051	3095	3098	3099	rBV3	865	429	0.02%	0.003%
85	11.138	3122	3125	3126	rBV3	956	518	0.03%	0.004%
86	11.289	3160	3172	3190	rBV	846099	1325868	73.73%	9.396%
87	11.614	3269	3273	3277	rVB5	1649	1237	0.07%	0.009%
88	11.666	3277	3289	3308	rBV	750149	1205049	67.01%	8.540%
89	12.566	3567	3569	3571	rBV2	1372	624	0.03%	0.004%
90	13.389	3822	3825	3828	rBV4	1287	948	0.05%	0.007%
91	14.640	4212	4214	4218	rBV5	2286	1721	0.10%	0.012%


Sum of corrected areas: 14111209

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121019\
Data File : VV013998.D
Acq On : 10 Dec 2019 19:50
Operator : SY/MD
Sample : K6200-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF24

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

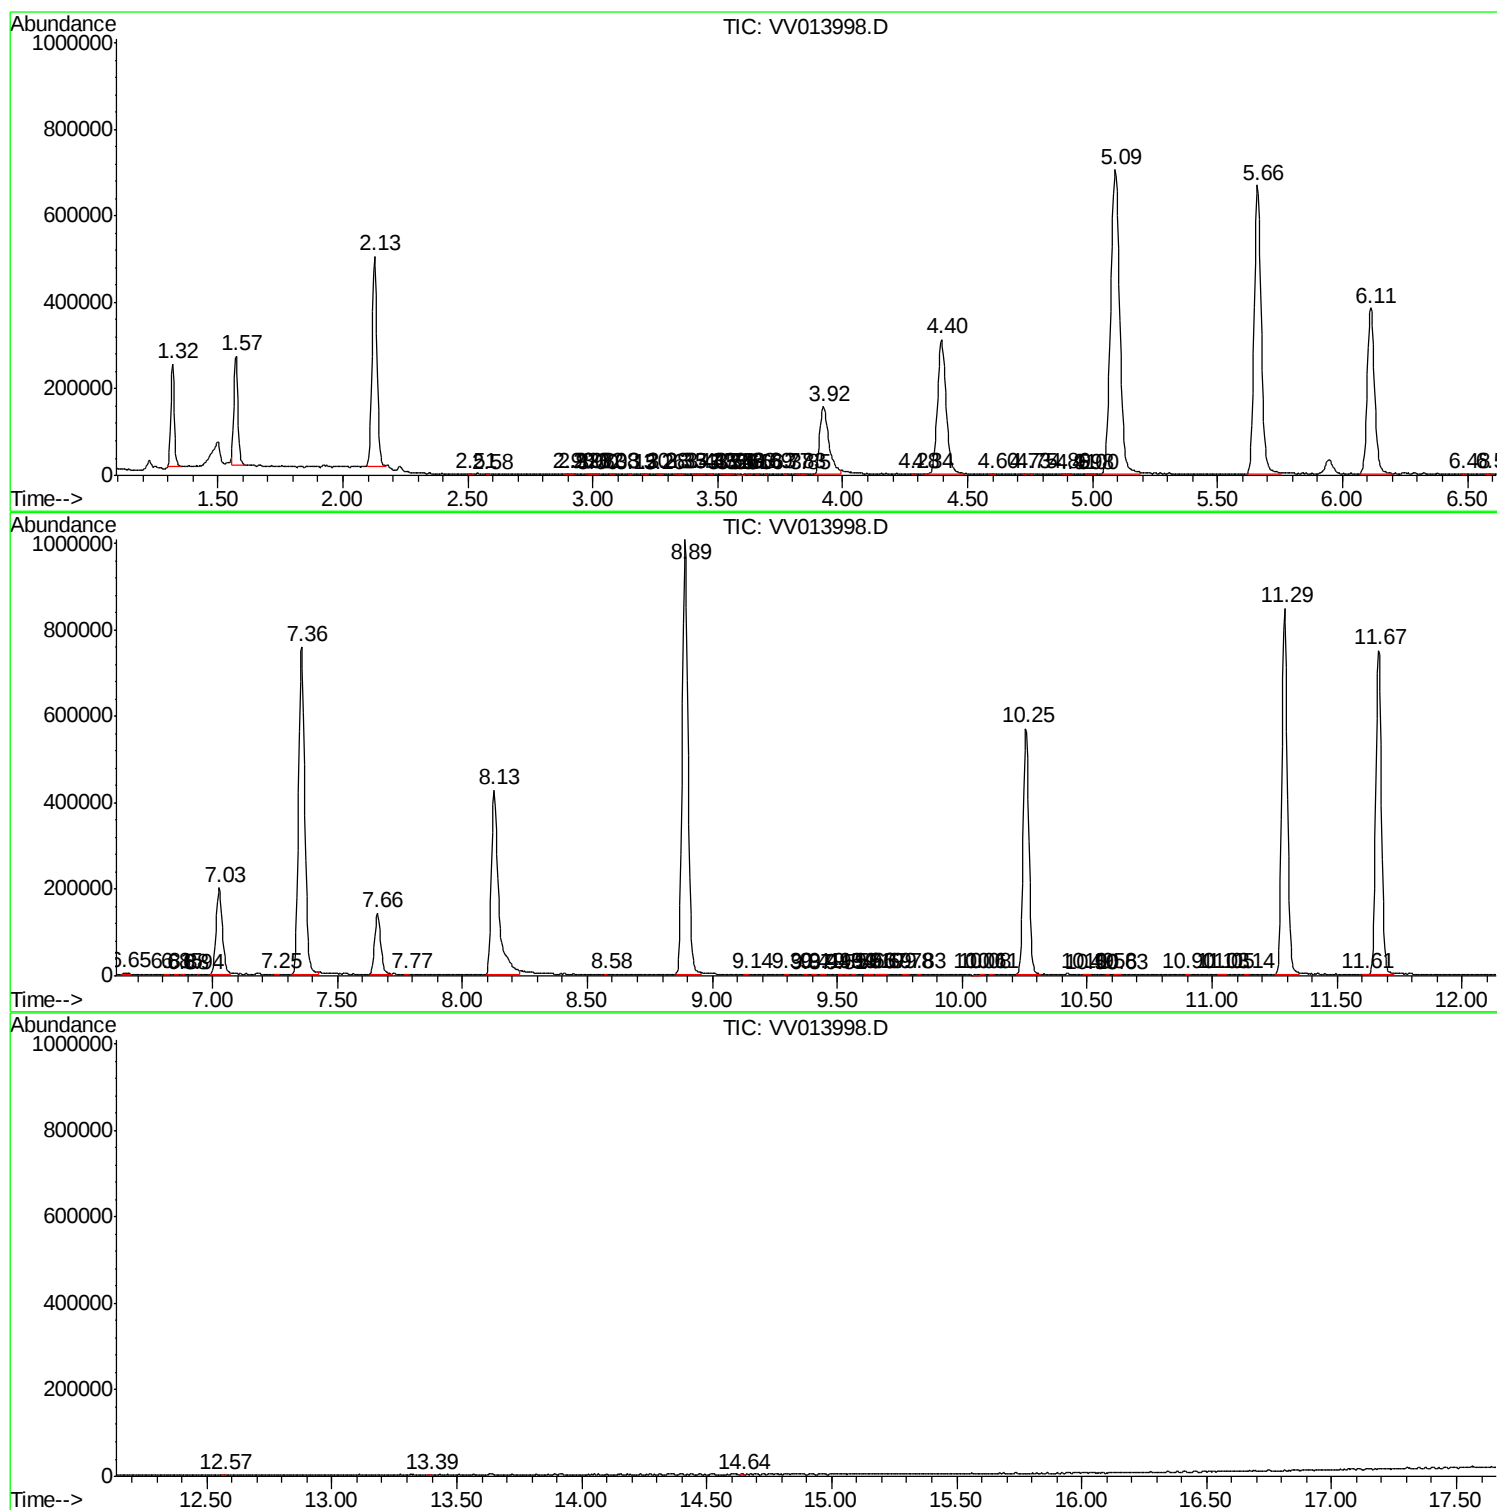

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121019\
Data File : VV013998.D
Acq On : 10 Dec 2019 19:50
Operator : SY/MD
Sample : K6200-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF24

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121019\
Data File : VV013998.D
Acq On : 10 Dec 2019 19:50
Operator : SY/MD
Sample : K6200-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF24

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc