

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
 Data File : VV013999.D
 Acq On : 10 Dec 2019 20:15
 Operator : SY/MD
 Sample : K6200-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	83	rVB	249261	240605	10.57%	1.526%
2	1.576	144	151	161	rVB	271988	303597	13.34%	1.925%
3	2.129	314	323	334	rVB	499140	705512	31.00%	4.474%
4	2.405	407	409	411	rBV3	2142	934	0.04%	0.006%
5	2.949	574	578	580	rBV4	1789	1205	0.05%	0.008%
6	3.248	667	671	675	rVB7	1702	1316	0.06%	0.008%
7	3.737	821	823	825	rVB3	1440	603	0.03%	0.004%
8	3.865	861	863	868	rBV5	1074	898	0.04%	0.006%
9	3.920	870	880	909	rBV	181288	478883	21.04%	3.037%
10	4.396	1014	1028	1052	rVB2	365942	883028	38.80%	5.599%
11	5.090	1224	1244	1275	rBV2	885218	2275605	100.00%	14.430%
12	5.659	1408	1421	1446	rBV	836855	1631610	71.70%	10.346%
13	6.113	1550	1562	1582	rBV	492507	974940	42.84%	6.182%
14	6.383	1643	1646	1650	rBV4	3591	3383	0.15%	0.021%
15	7.026	1836	1846	1868	rVB	243985	427647	18.79%	2.712%
16	7.357	1936	1949	1967	rBV	925358	1604335	70.50%	10.173%
17	7.659	2034	2043	2060	rVB	169246	281252	12.36%	1.783%
18	8.058	2164	2167	2169	rBV4	1124	873	0.04%	0.006%
19	8.126	2178	2188	2227	rBV2	416661	883613	38.83%	5.603%
20	8.473	2293	2296	2302	rVV7	1720	1703	0.07%	0.011%
21	8.511	2305	2308	2311	rVB4	1612	849	0.04%	0.005%
22	8.595	2331	2334	2337	rBV3	1336	1126	0.05%	0.007%
23	8.621	2340	2342	2344	rBV2	1144	644	0.03%	0.004%
24	8.634	2344	2346	2347	rBV2	1027	441	0.02%	0.003%
25	8.730	2373	2376	2379	rVB5	729	487	0.02%	0.003%
26	8.749	2379	2382	2385	rBV5	1622	903	0.04%	0.006%
27	8.801	2392	2398	2400	rVB5	1464	1183	0.05%	0.008%
28	8.820	2400	2404	2406	rBV4	1080	821	0.04%	0.005%
29	8.833	2406	2408	2410	rBV3	845	390	0.02%	0.002%
30	8.891	2413	2426	2450	rBV	1001743	1624569	71.39%	10.301%
31	9.048	2472	2475	2477	rBV3	1372	966	0.04%	0.006%
32	9.103	2489	2492	2495	rBV4	1309	778	0.03%	0.005%
33	9.283	2546	2548	2551	rBV4	898	479	0.02%	0.003%
34	9.373	2572	2576	2578	rBV4	1705	1232	0.05%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
 Data File : VV013999.D
 Acq On : 10 Dec 2019 20:15
 Operator : SY/MD
 Sample : K6200-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	9.434	2592	2595	2597	rVB3	764	373	0.02%	0.002%
36	9.473	2605	2607	2609	rVB3	1166	461	0.02%	0.003%
37	9.492	2609	2613	2618	rBV4	996	1133	0.05%	0.007%
38	9.531	2623	2625	2631	rVB5	1179	732	0.03%	0.005%
39	9.614	2649	2651	2653	rBV2	774	411	0.02%	0.003%
40	9.688	2671	2674	2677	rVB5	1009	681	0.03%	0.004%
41	9.707	2677	2680	2683	rBV3	1043	712	0.03%	0.005%
42	9.765	2695	2698	2700	rBV4	1735	1132	0.05%	0.007%
43	9.807	2708	2711	2713	rBV2	898	620	0.03%	0.004%
44	9.839	2718	2721	2725	rVV4	1131	894	0.04%	0.006%
45	9.891	2733	2737	2741	rBV5	829	696	0.03%	0.004%
46	9.910	2741	2743	2745	rBV3	755	408	0.02%	0.003%
47	9.942	2751	2753	2755	rBV2	673	371	0.02%	0.002%
48	10.003	2768	2772	2774	rBV4	668	444	0.02%	0.003%
49	10.023	2776	2778	2780	rVV3	921	424	0.02%	0.003%
50	10.039	2780	2783	2785	rVB3	1059	628	0.03%	0.004%
51	10.051	2785	2787	2789	rBV2	706	370	0.02%	0.002%
52	10.158	2816	2820	2824	rVB3	864	773	0.03%	0.005%
53	10.180	2824	2827	2831	rBV3	830	666	0.03%	0.004%
54	10.254	2837	2850	2870	rBV	556745	877112	38.54%	5.562%
55	10.399	2892	2895	2898	rBV5	766	648	0.03%	0.004%
56	10.424	2900	2903	2908	rVV6	2148	1804	0.08%	0.011%
57	10.447	2908	2910	2916	rVB5	1654	1465	0.06%	0.009%
58	10.482	2920	2921	2923	rBV2	873	399	0.02%	0.003%
59	10.518	2929	2932	2933	rBV2	881	404	0.02%	0.003%
60	10.543	2938	2940	2943	rVB4	1207	641	0.03%	0.004%
61	10.569	2943	2948	2951	rBV4	1394	1216	0.05%	0.008%
62	10.598	2955	2957	2961	rVB3	1552	1048	0.05%	0.007%
63	10.704	2988	2990	2996	rVB4	1342	1121	0.05%	0.007%
64	10.730	2996	2998	3003	rBV3	707	458	0.02%	0.003%
65	10.759	3003	3007	3008	rBV2	1019	637	0.03%	0.004%
66	10.842	3029	3033	3038	rVB8	1177	1253	0.06%	0.008%
67	10.875	3038	3043	3047	rBV5	1170	1379	0.06%	0.009%
68	10.939	3059	3063	3068	rBV5	1212	1295	0.06%	0.008%
69	11.010	3082	3085	3090	rBV6	1250	1217	0.05%	0.008%
70	11.206	3143	3146	3151	rBV7	1600	1386	0.06%	0.009%
71	11.289	3160	3172	3189	rBV	819727	1290488	56.71%	8.183%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121019\
 Data File : VV013999.D
 Acq On : 10 Dec 2019 20:15
 Operator : SY/MD
 Sample : K6200-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	11.579	3260	3262	3264	rBV3	1244	465	0.02%	0.003%
73	11.666	3276	3289	3311	rBV	774704	1216158	53.44%	7.712%
74	11.865	3349	3351	3353	rBV3	1321	672	0.03%	0.004%
75	12.010	3393	3396	3399	rBV3	1641	1268	0.06%	0.008%
76	12.067	3413	3414	3417	rVB3	990	449	0.02%	0.003%
77	12.084	3417	3419	3424	rBV3	885	709	0.03%	0.004%
78	12.106	3424	3426	3431	rBV5	1568	1246	0.05%	0.008%
79	12.270	3472	3477	3479	rBV4	1547	1285	0.06%	0.008%
80	12.344	3498	3500	3502	rBV	822	474	0.02%	0.003%
81	12.392	3512	3515	3517	rBV3	1810	1302	0.06%	0.008%
82	12.434	3526	3528	3531	rBV2	1335	530	0.02%	0.003%
83	12.511	3551	3552	3554	rBV2	716	389	0.02%	0.002%
84	12.601	3577	3580	3581	rBV3	844	408	0.02%	0.003%
85	12.633	3586	3590	3591	rBV4	1117	686	0.03%	0.004%
86	12.685	3601	3606	3607	rBV3	1415	968	0.04%	0.006%
87	12.849	3654	3657	3659	rVB4	1624	792	0.03%	0.005%
88	12.913	3672	3677	3678	rBV3	1252	851	0.04%	0.005%
89	12.987	3696	3700	3704	rBV6	817	915	0.04%	0.006%
90	13.116	3737	3740	3741	rBV2	900	621	0.03%	0.004%
91	13.148	3748	3750	3752	rBV3	1194	658	0.03%	0.004%
92	13.180	3758	3760	3762	rBV2	943	411	0.02%	0.003%
93	13.575	3881	3883	3889	rVB6	1672	977	0.04%	0.006%
94	13.698	3919	3921	3922	rBV2	996	422	0.02%	0.003%
95	13.788	3947	3949	3951	rBV3	1290	699	0.03%	0.004%
96	13.903	3981	3985	3988	rBV3	1295	1245	0.05%	0.008%
97	13.955	3999	4001	4005	rBV4	1018	708	0.03%	0.004%
98	14.157	4062	4064	4070	rVB4	1484	935	0.04%	0.006%
99	14.334	4117	4119	4122	rVB3	1691	661	0.03%	0.004%
100	14.579	4193	4195	4198	rBV3	1539	1128	0.05%	0.007%


Sum of corrected areas: 15770342

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121019\
Data File : VV013999.D
Acq On : 10 Dec 2019 20:15
Operator : SY/MD
Sample : K6200-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF25

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

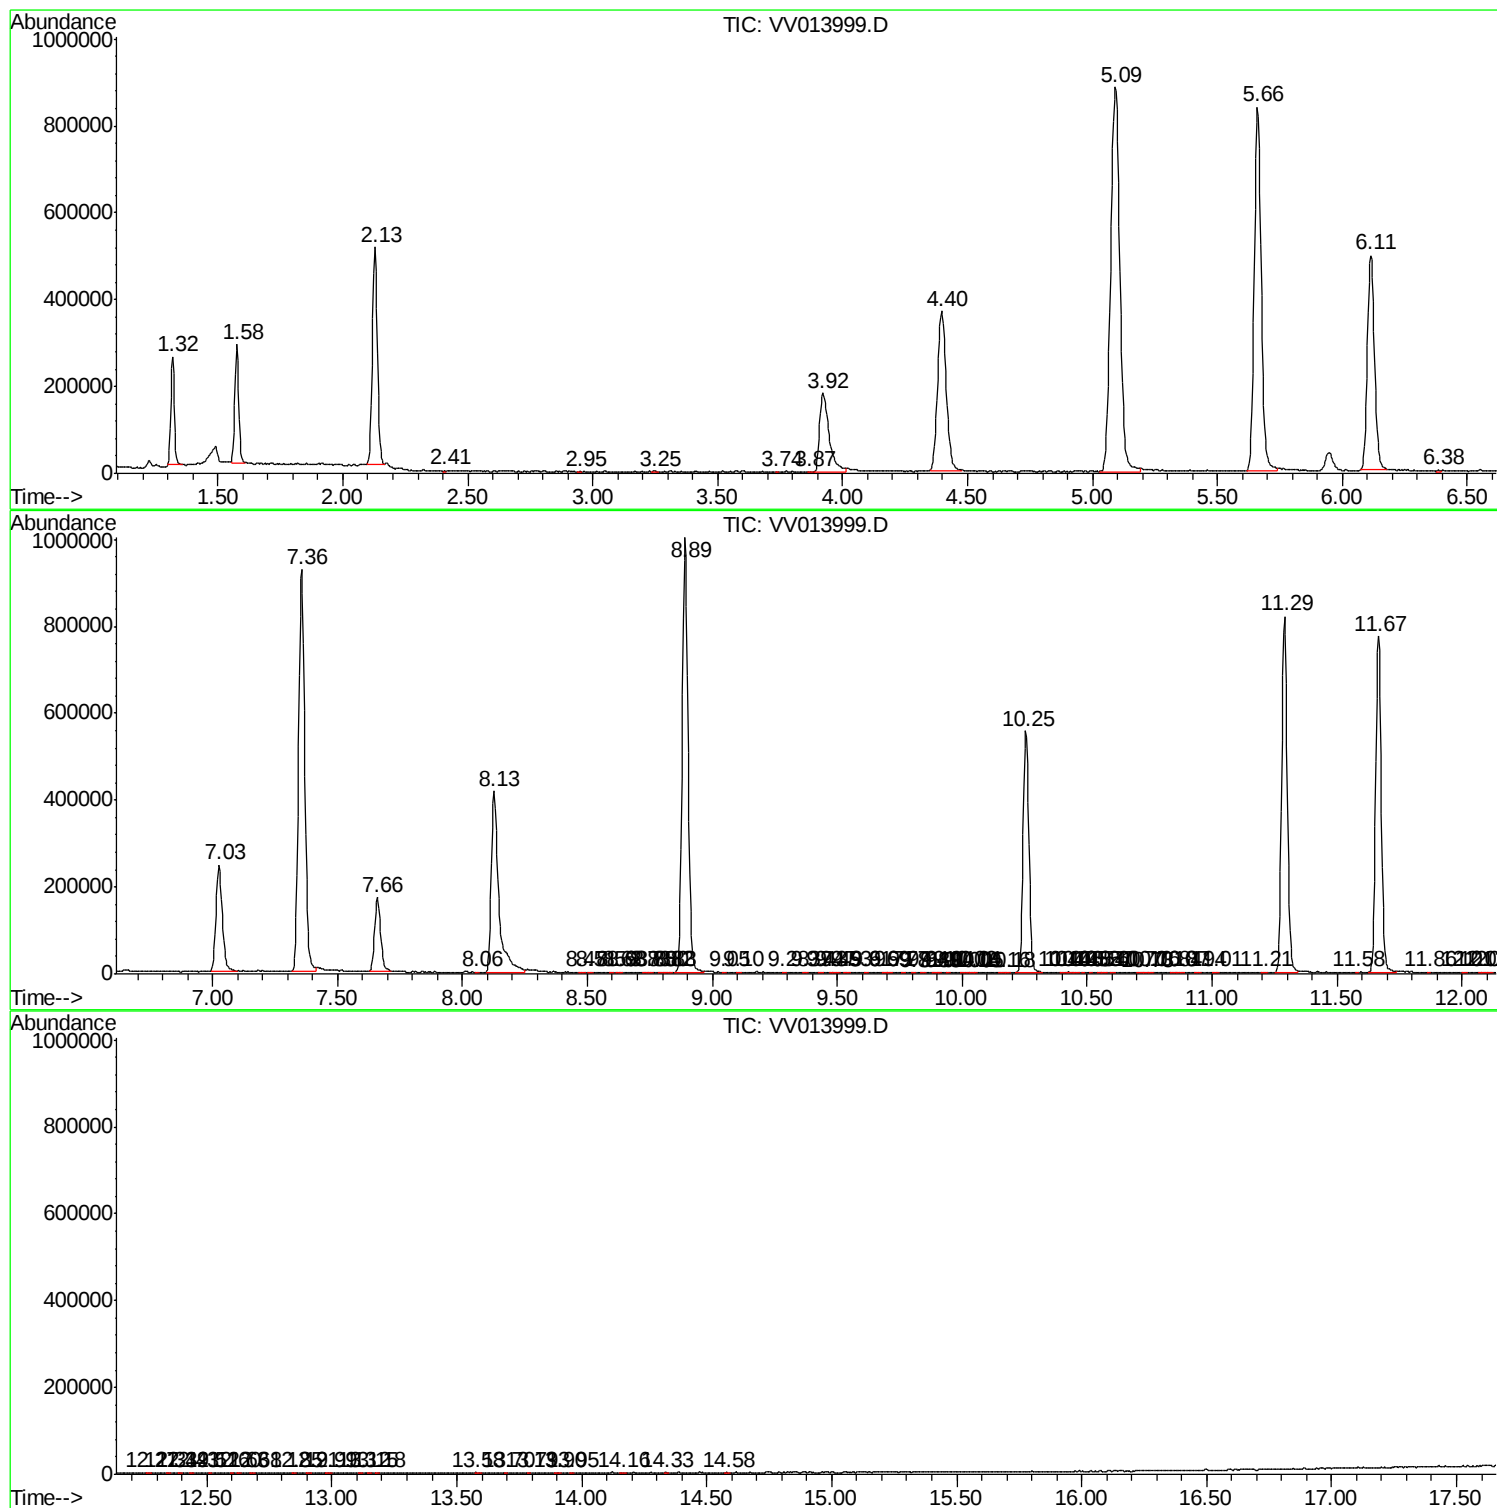

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121019\
Data File : VV013999.D
Acq On : 10 Dec 2019 20:15
Operator : SY/MD
Sample : K6200-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF25

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121019\
Data File : VV013999.D
Acq On : 10 Dec 2019 20:15
Operator : SY/MD
Sample : K6200-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF25

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc