


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121019\
 Data File : VV013976.D
 Acq On : 10 Dec 2019 09:46
 Operator : SY/MD
 Sample : BFB79
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB79

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis
 Last Update : Wed Dec 11 00:25:42 2019

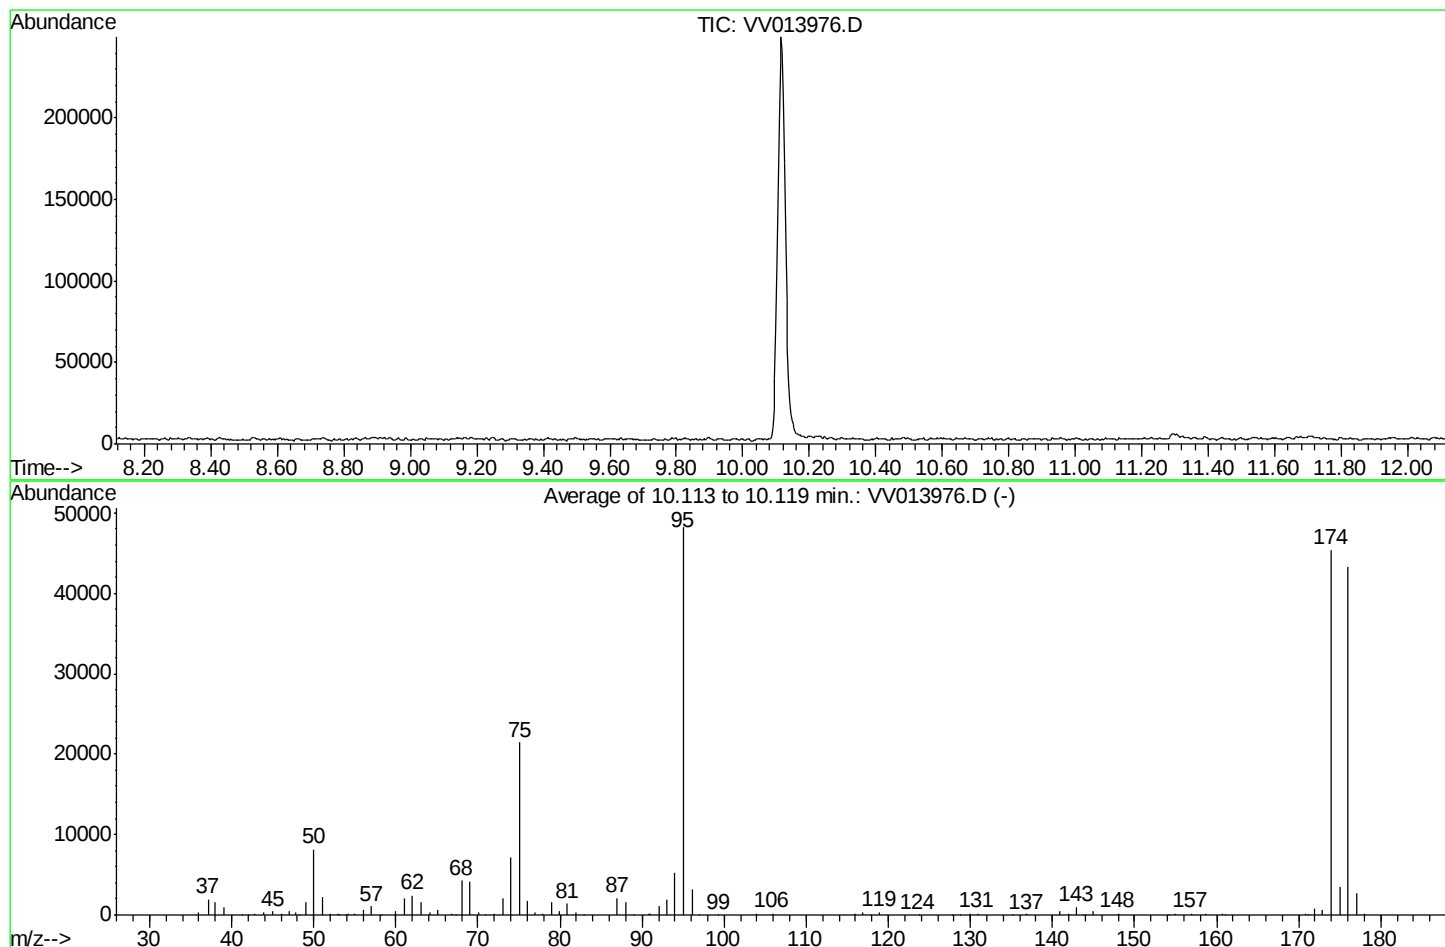

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	8131	PASS
75	95	30	80	44.5	21469	PASS
95	95	100	100	100.0	48197	PASS
96	95	5	9	6.5	3121	PASS
173	174	0.00	2	1.6	719	PASS
174	95	50	120	94.3	45429	PASS
175	174	5	9	7.8	3536	PASS
176	174	95	101	95.3	43312	PASS
177	176	5	9	6.4	2752	PASS

m/z	Abundance
35.90	413.0
37.10	1990.0
38.00	1655.0
39.00	880.0
40.00	641.0
41.20	107.0
42.00	114.0
42.90	193.0
44.00	922.0
45.00	450.0
46.10	179.0
47.00	458.0
47.80	325.0
48.20	192.0
49.00	1679.0
50.00	8178.0
51.00	2124.0
52.00	168.0
52.80	159.0
53.80	115.0
54.10	116.0
54.90	170.0
56.00	782.0
57.00	1086.0
58.20	112.0
60.10	456.0
61.00	2069.0
62.00	2121.0
63.00	1691.0
64.20	372.0
65.10	627.0
66.70	145.0
68.00	4211.0
69.00	4141.0
70.10	437.0
72.00	146.0
73.00	1881.0
74.10	6880.0
75.10	21352.0
76.00	1693.0
77.00	415.0
77.80	171.0
79.00	1561.0
80.00	493.0
80.90	1432.0
82.00	315.0
87.00	1889.0
88.10	1682.0
88.90	118.0
90.80	248.0
92.00	1012.0
93.00	1854.0
94.00	4780.0
95.00	47016.0
96.10	3014.0
97.00	110.0
99.30	105.0
104.00	165.0
106.00	208.0
116.00	213.0
116.90	421.0
118.90	402.0
127.80	156.0
130.00	153.0
130.90	136.0
140.90	420.0
142.90	936.0
143.70	137.0
144.00	125.0
144.90	464.0
148.00	169.0
154.80	131.0
156.90	160.0
160.70	144.0
170.80	260.0
171.90	743.0
172.90	692.0
174.00	42944.0
175.00	3506.0
176.00	41224.0
177.00	2838.0
178.00	186.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
35.90	436.0
37.10	2123.0
38.00	1727.0
39.00	988.0
40.00	617.0
42.70	161.0
42.90	164.0
43.90	904.0
45.00	444.0
46.00	189.0
47.00	466.0
47.80	316.0
49.00	1697.0
50.00	8583.0
51.00	2186.0
51.90	219.0
52.90	173.0
54.10	112.0
55.00	230.0
56.00	718.0
57.00	1067.0
58.30	103.0
60.00	514.0
61.00	2075.0
62.10	2531.0
63.00	1692.0
64.10	386.0
65.00	643.0
66.80	129.0
67.20	124.0
68.00	4492.0
69.00	4135.0
70.10	371.0
72.00	186.0
73.00	2120.0
74.10	7439.0
75.10	22160.0
76.00	1845.0
77.00	406.0
77.80	174.0
78.90	1600.0
79.90	455.0
80.90	1427.0
82.00	298.0
86.90	2166.0
88.00	1632.0
90.80	243.0
92.00	1151.0
93.00	1979.0
94.00	5314.0
95.00	50096.0
96.10	3283.0
96.80	120.0
104.00	231.0
105.90	218.0
116.00	224.0
116.90	353.0
119.00	412.0
130.00	150.0
130.80	190.0
135.10	101.0
136.80	128.0
140.90	443.0
142.00	123.0
143.00	1016.0
144.90	528.0
148.00	184.0
154.90	162.0
156.90	199.0
158.70	133.0
160.80	127.0
170.90	250.0
171.90	801.0
172.90	724.0
174.00	47048.0
175.00	3663.0
176.00	44624.0
177.00	2817.0
178.00	188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
36.00	409.0
37.10	2007.0
38.00	1717.0
39.00	952.0
39.90	684.0
42.70	139.0
43.90	943.0
45.00	445.0
46.00	168.0
47.00	518.0
47.80	301.0
49.10	1615.0
50.00	8069.0
51.00	2257.0
51.90	242.0
53.10	188.0
54.10	126.0
55.00	286.0
56.00	646.0
57.00	1079.0
59.90	577.0
61.00	1913.0
62.10	2583.0
63.00	1577.0
64.10	374.0
65.00	563.0
66.90	164.0
68.00	4147.0
69.00	3949.0
70.00	282.0
70.90	116.0
71.90	216.0
73.00	2050.0
74.00	7148.0
75.10	20896.0
76.00	1746.0
76.90	372.0
77.90	151.0
78.90	1490.0
79.90	381.0
80.90	1340.0
82.00	249.0
82.80	114.0
86.90	2228.0
87.90	1695.0
91.00	260.0
92.00	1185.0
93.10	1948.0
94.00	5473.0
95.00	47480.0
96.10	3066.0
103.90	243.0
105.80	231.0
116.00	271.0
117.00	256.0
117.80	114.0
118.90	343.0
123.70	111.0
128.80	150.0
130.00	163.0
130.80	176.0
135.10	110.0
136.90	158.0
141.00	437.0
141.90	173.0
143.00	928.0
144.90	554.0
148.00	169.0
154.10	104.0
155.00	155.0
156.90	185.0
158.70	150.0
161.00	146.0
171.10	228.0
171.90	766.0
172.90	743.0
174.00	46296.0
175.00	3440.0
176.00	44088.0
177.00	2601.0
178.00	234.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
36.00	126.0
37.10	119.0
38.20	108.0
40.00	667.0
40.80	111.0
42.30	159.0
43.10	152.0
44.00	581.0
47.30	115.0
50.10	145.0
55.10	103.0
60.30	171.0
93.30	102.0
207.10	117.0
207.60	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79