

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019522.D
 Acq On : 10 Dec 2020 20:16
 Operator : SY/MD
 Sample : L4997-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ4

Quant Time: Dec 11 02:39:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 11 02:38:22 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 12/14/2020 9:11:38 AM

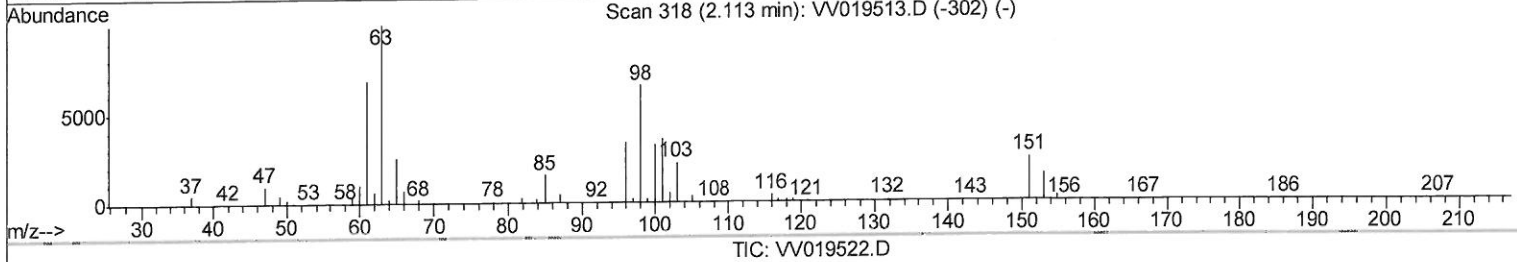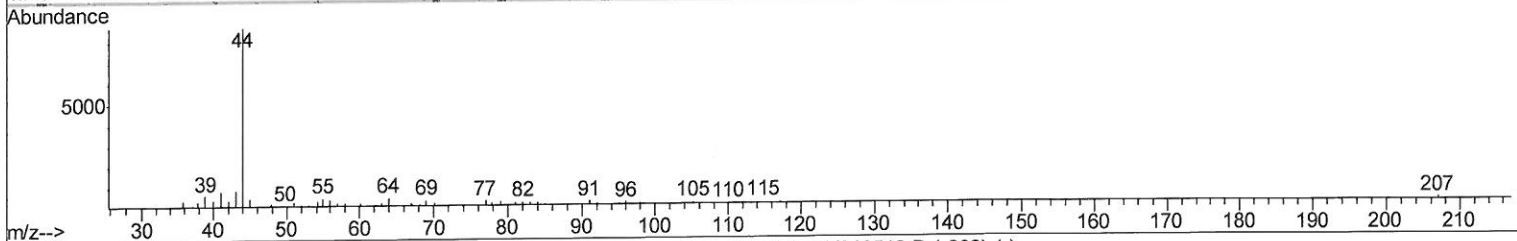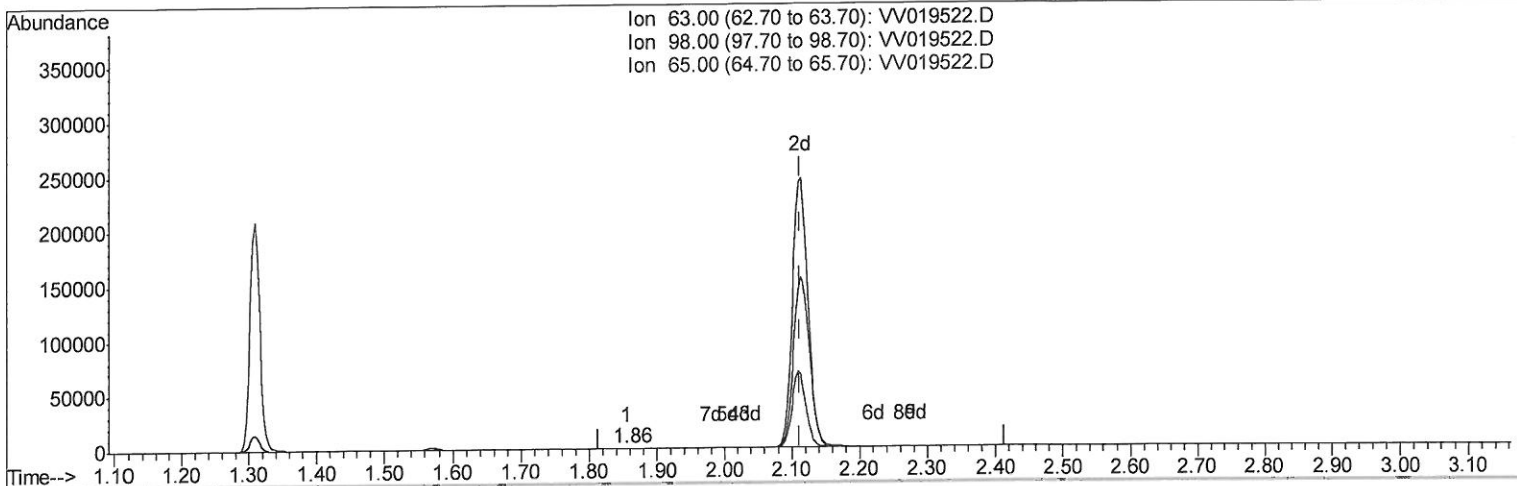

(11) 1,1-Dichloroethene-d2 (S)

1.856min (-0.257) 0.01ug/L

response 128

Ion	Exp%	Act%
63.00	100	100
98.00	79.80	103.13
65.00	19.20	15.63
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019522.D
 Acq On : 10 Dec 2020 20:16
 Operator : SY/MD
 Sample : L4997-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ4

Quant Time: Dec 11 02:39:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 11 02:38:22 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 12/14/2020 9:11:38 AM

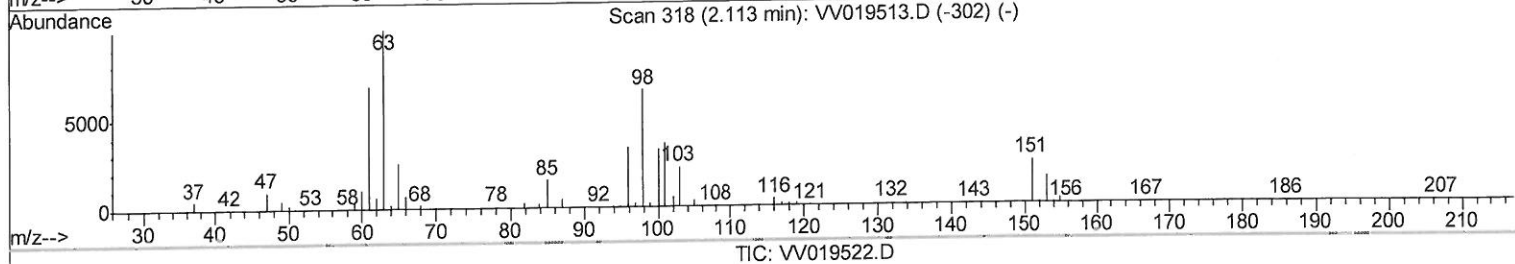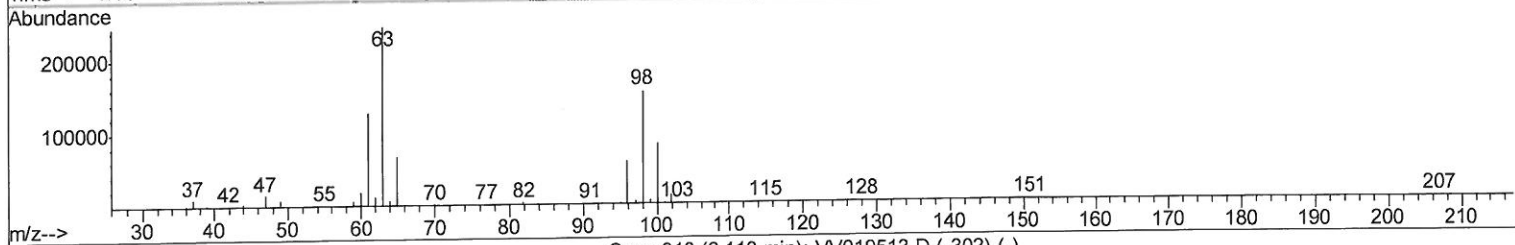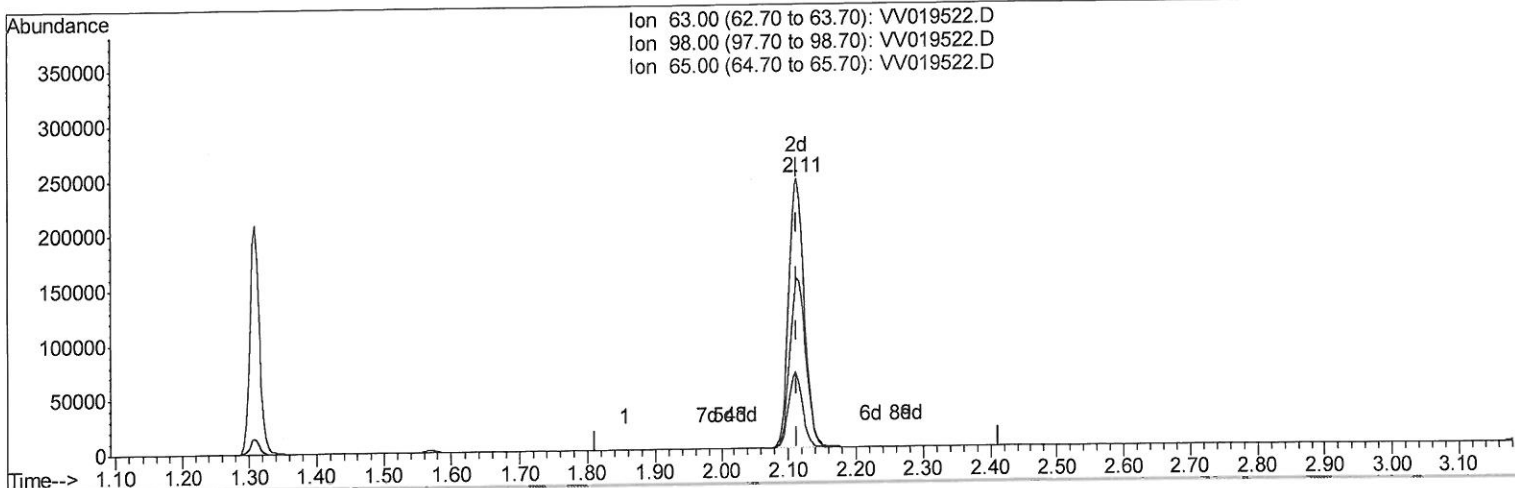

(11) 1,1-Dichloroethene-d2 (S)

2.113min (-0.000) 41.82ug/L m

>1210872087

response 391691

Ion	Exp%	Act%
63.00	100	100
98.00	79.80	0.03#
65.00	19.20	0.01#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019522.D
 Acq On : 10 Dec 2020 20:16
 Operator : SY/MD
 Sample : L4997-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sample ID :
 C0AQ4

Quant Time: Dec 11 03:47:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 11 02:38:22 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 12/14/2020 9:11:38 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.62	114	703776	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.86	117	651175	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.25	152	302258	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	205881	40.80	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.60%		
7) Chloroethane-d5	1.57	69	172395	43.31	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.62%		
11) 1,1-Dichloroethene-d2	2.11	63	391691m	41.82	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.64%		
21) 2-Butanone-d5	3.89	46	272456	99.33	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	99.33%		
24) Chloroform-d	4.35	84	409214	44.99	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.98%		
26) 1,2-Dichloroethane-d4	5.04	65	285818	48.09	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.18%		
32) Benzene-d6	5.05	84	812579	46.79	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.58%		
36) 1,2-Dichloropropane-d6	6.07	67	254861	46.85	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.70%		
41) Toluene-d8	7.32	98	733653	46.92	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.84%		
43) trans-1,3-Dichloropropene-	7.62	79	144719	46.77	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.54%		
47) 2-Hexanone-d5	8.09	63	205838	96.40	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	96.40%		
57) 1,1,2,2-Tetrachloroethane-	10.22	84	341997	46.48	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.96%		
64) 1,2-Dichlorobenzene-d4	11.63	152	271305	48.02	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.04%		

Target Compounds

					Ovalue
12) 1,1-Dichloroethene	2.12	96	136083	32.457 ug/L	# 70
19) 1,1-Dichloroethane	3.20	63	11720	1.315 ug/L	100
20) cis-1,2-Dichloroethene	3.92	96	163909	32.446 ug/L	# 97
30) 1,1,1-Trichloroethane	4.61	97	237891	29.136 ug/L	99
34) Trichloroethene	5.92	95	2399678	477.330 ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019522.D
 Acq On : 10 Dec 2020 20:16
 Operator : SY/MD
 Sample : L4997-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 C0AQ4

Quant Time: Dec 11 03:47:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 11 02:38:22 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 12/14/2020 9:11:38 AM

