

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019523.D
 Acq On : 10 Dec 2020 20:40
 Operator : SY/MD
 Sample : L4997-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ5

Manual Integrations
 APPROVED

MMDadoda
 12/14/2020 9:11:40 AM

Quant Time: Dec 11 03:51:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 11 02:38:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.62	114	688365	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.86	117	648883	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.25	152	299325	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	202793	41.08	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.16%
7) Chloroethane-d5	1.57	69	172534	44.32	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	88.64%
11) 1,1-Dichloroethene-d2	2.11	63	313385m	34.21	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.42%
21) 2-Butanone-d5	3.89	46	256520	95.61	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.61%
24) Chloroform-d	4.35	84	405234	45.55	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.10%
26) 1,2-Dichloroethane-d4	5.04	65	285356	49.08	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.16%
32) Benzene-d6	5.05	84	811304	46.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.76%
36) 1,2-Dichloropropane-d6	6.07	67	259093	47.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.58%
41) Toluene-d8	7.32	98	731708	46.96	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.92%
43) trans-1,3-Dichloropropene-	7.62	79	138579	44.94	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.88%
47) 2-Hexanone-d5	8.09	63	202269	95.07	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.07%
57) 1,1,2,2-Tetrachloroethane-	10.22	84	340004	46.37	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.74%
64) 1,2-Dichlorobenzene-d4	11.63	152	268854	48.05	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.10%

Target Compounds					Ovalue
34) Trichloroethene	5.93	95	5404	1.079 ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121020\
Data File : VV019523.D
Acq On : 10 Dec 2020 20:40
Operator : SY/MD
Sample : L4997-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1




Instrument :
MSVOA_V
ClientSampleId :
C0AQ5

Manual Integrations
APPROVED

MMDadoda
12/14/2020 9:11:40 AM

Quant Time: Dec 11 03:51:13 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 11 02:38:22 2020
Response via : Initial Calibration

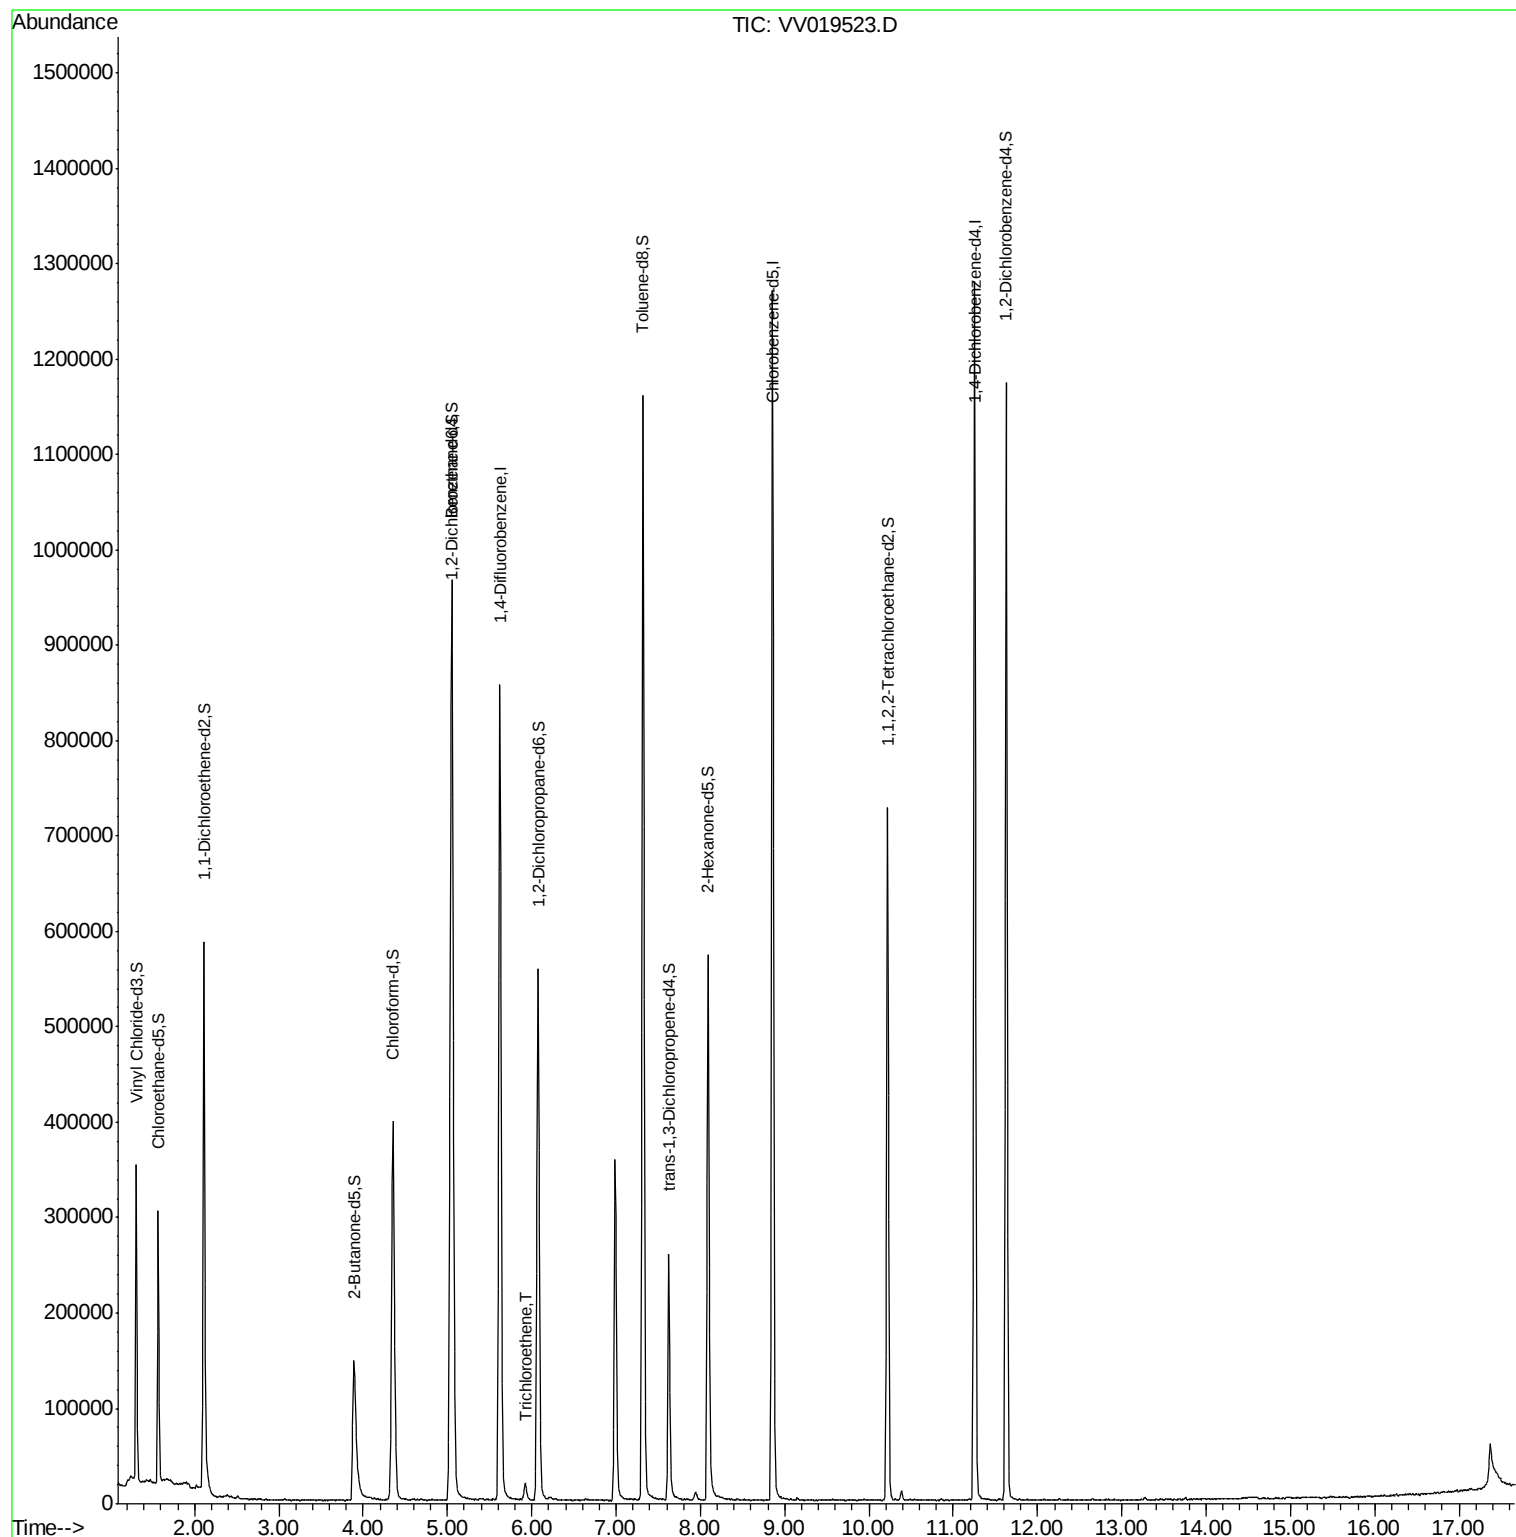

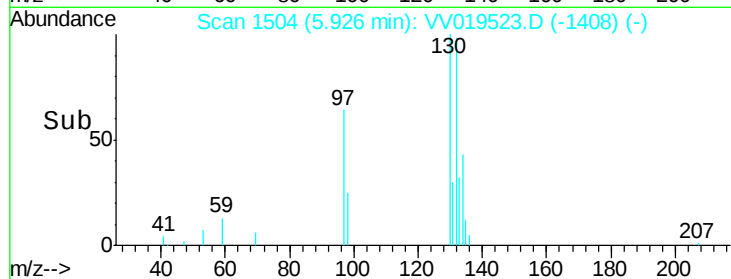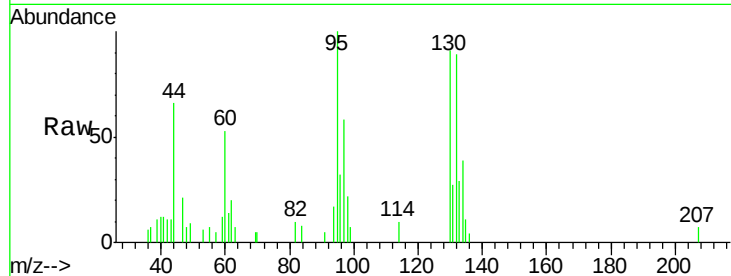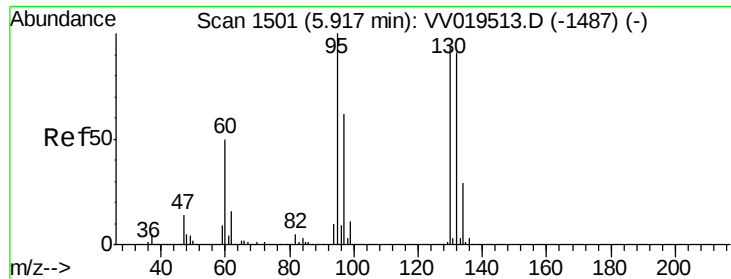

#34

Trichloroethene

Concen: 1.079 ug/L


RT: 5.93 min Scan# 1504

Delta R.T. 0.01 min

Lab File: VV019523.D

Acq: 10 Dec 2020 20:40

Tot Ion	Ion	Ratio	Resp: Lower	Upper
95	100			
97	58.4	44.4	82.4	
132	88.7	64.3	119.3	
130	90.5	67.8	125.8	

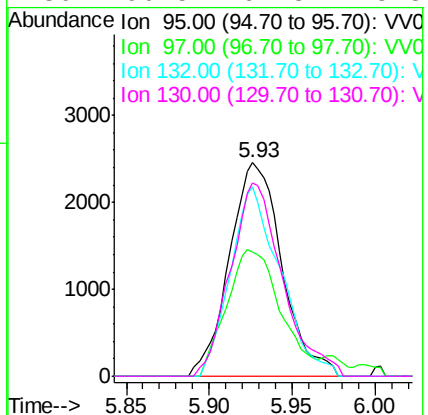

Instrument :

MSVOA_V

ClientSampleId :

C0AQ5

Manual Integrations
APPROVED

MMDadoda
12/14/2020 9:11:40 AM