

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019519.D
 Acq On : 10 Dec 2020 19:04
 Operator : SY/MD
 Sample : L4997-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	79	rVB	340162	333879	13.65%	1.711%
2	1.570	142	149	163	rBV	277526	312173	12.76%	1.600%
3	2.110	308	317	344	rVB	588756	917831	37.52%	4.704%
4	2.611	470	473	477	rBV5	1374	843	0.03%	0.004%
5	2.737	509	512	515	rBV2	1122	998	0.04%	0.005%
6	2.891	557	560	565	rVB7	808	650	0.03%	0.003%
7	2.917	565	568	573	rVB6	932	788	0.03%	0.004%
8	2.978	585	587	592	rBV7	1041	856	0.03%	0.004%
9	3.042	603	607	611	rBV5	1341	988	0.04%	0.005%
10	3.193	650	654	657	rBV4	1641	1209	0.05%	0.006%
11	3.296	682	686	690	rBV5	779	680	0.03%	0.003%
12	3.396	714	717	720	rVB5	1300	855	0.03%	0.004%
13	3.467	737	739	742	rBV3	779	594	0.02%	0.003%
14	3.582	772	775	782	rBV6	1108	1118	0.05%	0.006%
15	3.669	796	802	807	rBV7	783	1157	0.05%	0.006%
16	3.814	843	847	849	rBV5	906	820	0.03%	0.004%
17	3.897	860	873	910	rBV	156790	527678	21.57%	2.704%
18	4.354	996	1015	1038	rBV	390943	964261	39.42%	4.942%
19	4.602	1080	1092	1094	rBV10	5197	6528	0.27%	0.033%
20	4.746	1134	1137	1141	rVB5	938	983	0.04%	0.005%
21	4.833	1160	1164	1168	rBV6	1057	878	0.04%	0.004%
22	4.875	1173	1177	1180	rBV5	882	888	0.04%	0.005%
23	4.936	1192	1196	1199	rVB5	844	657	0.03%	0.003%
24	4.955	1199	1202	1206	rBV5	1182	985	0.04%	0.005%
25	5.052	1214	1232	1263	rBV2	960715	2446081	100.00%	12.535%
26	5.348	1322	1324	1328	rVB4	1292	727	0.03%	0.004%
27	5.373	1328	1332	1338	rBV6	1033	1164	0.05%	0.006%
28	5.405	1338	1342	1352	rVB10	1840	2681	0.11%	0.014%
29	5.518	1373	1377	1381	rBV6	1557	1098	0.04%	0.006%
30	5.563	1389	1391	1396	rBV4	780	912	0.04%	0.005%
31	5.621	1396	1409	1434	rBV	860193	1706118	69.75%	8.743%
32	5.923	1488	1503	1516	rBV7	21052	49283	2.01%	0.253%
33	6.074	1534	1550	1578	rBV	546692	1115113	45.59%	5.715%
34	6.483	1674	1677	1679	rBV4	1239	896	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019519.D
 Acq On : 10 Dec 2020 19:04
 Operator : SY/MD
 Sample : L4997-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.553	1696	1699	1702	rBV4	1129	973	0.04%	0.005%
36	6.630	1713	1723	1724	rBV8	1388	1569	0.06%	0.008%
37	6.762	1762	1764	1770	rVB5	737	653	0.03%	0.003%
38	6.804	1772	1777	1779	rBV5	790	690	0.03%	0.004%
39	6.865	1794	1796	1800	rVB3	1104	710	0.03%	0.004%
40	6.894	1800	1805	1807	rBV4	899	802	0.03%	0.004%
41	6.991	1822	1835	1854	rBV	353668	636547	26.02%	3.262%
42	7.151	1881	1885	1887	rBV4	1243	867	0.04%	0.004%
43	7.319	1924	1937	1978	rBV	1145943	1989133	81.32%	10.194%
44	7.624	2022	2032	2051	rBV	252920	432827	17.69%	2.218%
45	7.942	2122	2131	2141	rBV2	4510	8654	0.35%	0.044%
46	7.984	2141	2144	2145	rBV2	1091	654	0.03%	0.003%
47	8.090	2167	2177	2204	rBV	585977	994637	40.66%	5.097%
48	8.245	2223	2225	2230	rVB6	1657	1166	0.05%	0.006%
49	8.437	2282	2285	2288	rVV4	1315	1152	0.05%	0.006%
50	8.534	2311	2315	2319	rVB7	1216	1001	0.04%	0.005%
51	8.650	2347	2351	2353	rVV4	994	835	0.03%	0.004%
52	8.663	2353	2355	2360	rVB4	1415	1015	0.04%	0.005%
53	8.746	2379	2381	2384	rVB4	1175	700	0.03%	0.004%
54	8.855	2402	2415	2445	rBV	1271270	2063576	84.36%	10.575%
55	9.138	2499	2503	2504	rBV4	1531	990	0.04%	0.005%
56	9.206	2522	2524	2529	rVB4	1211	737	0.03%	0.004%
57	9.328	2558	2562	2565	rBV5	1154	947	0.04%	0.005%
58	9.380	2570	2578	2580	rBV7	1062	1328	0.05%	0.007%
59	9.418	2588	2590	2596	rVB4	1057	980	0.04%	0.005%
60	9.470	2602	2606	2609	rVB6	835	837	0.03%	0.004%
61	9.489	2609	2612	2613	rBV2	1613	901	0.04%	0.005%
62	9.900	2736	2740	2744	rVB6	1030	961	0.04%	0.005%
63	9.926	2744	2748	2749	rBV3	1236	824	0.03%	0.004%
64	10.222	2823	2840	2859	rBV	725582	1135595	46.43%	5.820%
65	10.389	2884	2892	2900	rVB4	4043	6758	0.28%	0.035%
66	10.444	2906	2909	2912	rVB2	1160	708	0.03%	0.004%
67	10.463	2912	2915	2918	rBV4	1225	852	0.03%	0.004%
68	10.550	2940	2942	2946	rVB4	1134	811	0.03%	0.004%
69	10.627	2962	2966	2973	rBV8	1180	1437	0.06%	0.007%
70	10.855	3033	3037	3038	rBV3	1191	636	0.03%	0.003%
71	10.868	3039	3041	3046	rVB4	1002	828	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019519.D
 Acq On : 10 Dec 2020 19:04
 Operator : SY/MD
 Sample : L4997-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.971	3069	3073	3080	rVB7	1197	1270	0.05%	0.007%
73	11.103	3111	3114	3116	rVB3	1190	791	0.03%	0.004%
74	11.122	3116	3120	3121	rBV3	946	708	0.03%	0.004%
75	11.254	3149	3161	3183	rBV	1316557	2014046	82.34%	10.321%
76	11.460	3222	3225	3228	rBV4	1066	791	0.03%	0.004%
77	11.630	3265	3278	3299	rBV	1128835	1777181	72.65%	9.107%
78	11.772	3318	3322	3324	rBV4	840	641	0.03%	0.003%
79	11.875	3351	3354	3357	rBV5	992	619	0.03%	0.003%
80	11.907	3361	3364	3367	rVV3	973	728	0.03%	0.004%
81	12.032	3399	3403	3405	rBV4	719	627	0.03%	0.003%
82	12.257	3468	3473	3474	rBV4	1468	1191	0.05%	0.006%
83	12.334	3493	3497	3502	rBV7	1075	1199	0.05%	0.006%
84	12.424	3523	3525	3528	rBV4	927	629	0.03%	0.003%
85	12.604	3578	3581	3585	rBV3	1067	823	0.03%	0.004%
86	12.653	3590	3596	3601	rBV5	2439	3224	0.13%	0.017%
87	12.704	3610	3612	3615	rBV2	874	587	0.02%	0.003%
88	12.723	3615	3618	3621	rVV3	1196	858	0.04%	0.004%
89	12.743	3621	3624	3626	rVB3	1235	725	0.03%	0.004%
90	12.990	3698	3701	3704	rVB3	838	584	0.02%	0.003%
91	13.061	3720	3723	3729	rVB6	767	776	0.03%	0.004%
92	13.116	3737	3740	3745	rBV3	1062	861	0.04%	0.004%
93	13.389	3822	3825	3831	rVV7	1059	900	0.04%	0.005%
94	13.514	3860	3864	3867	rVV5	1839	1668	0.07%	0.009%
95	13.649	3903	3906	3908	rBV3	879	600	0.02%	0.003%
96	14.048	4026	4030	4033	rBV3	974	1031	0.04%	0.005%
97	14.106	4046	4048	4051	rVB2	1267	731	0.03%	0.004%
98	14.276	4098	4101	4104	rBV5	1428	994	0.04%	0.005%
99	14.460	4155	4158	4161	rVB4	1408	986	0.04%	0.005%
100	14.479	4161	4164	4166	rBV3	1627	1079	0.04%	0.006%


Sum of corrected areas: 19513509

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121020\
Data File : VV019519.D
Acq On : 10 Dec 2020 19:04
Operator : SY/MD
Sample : L4997-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

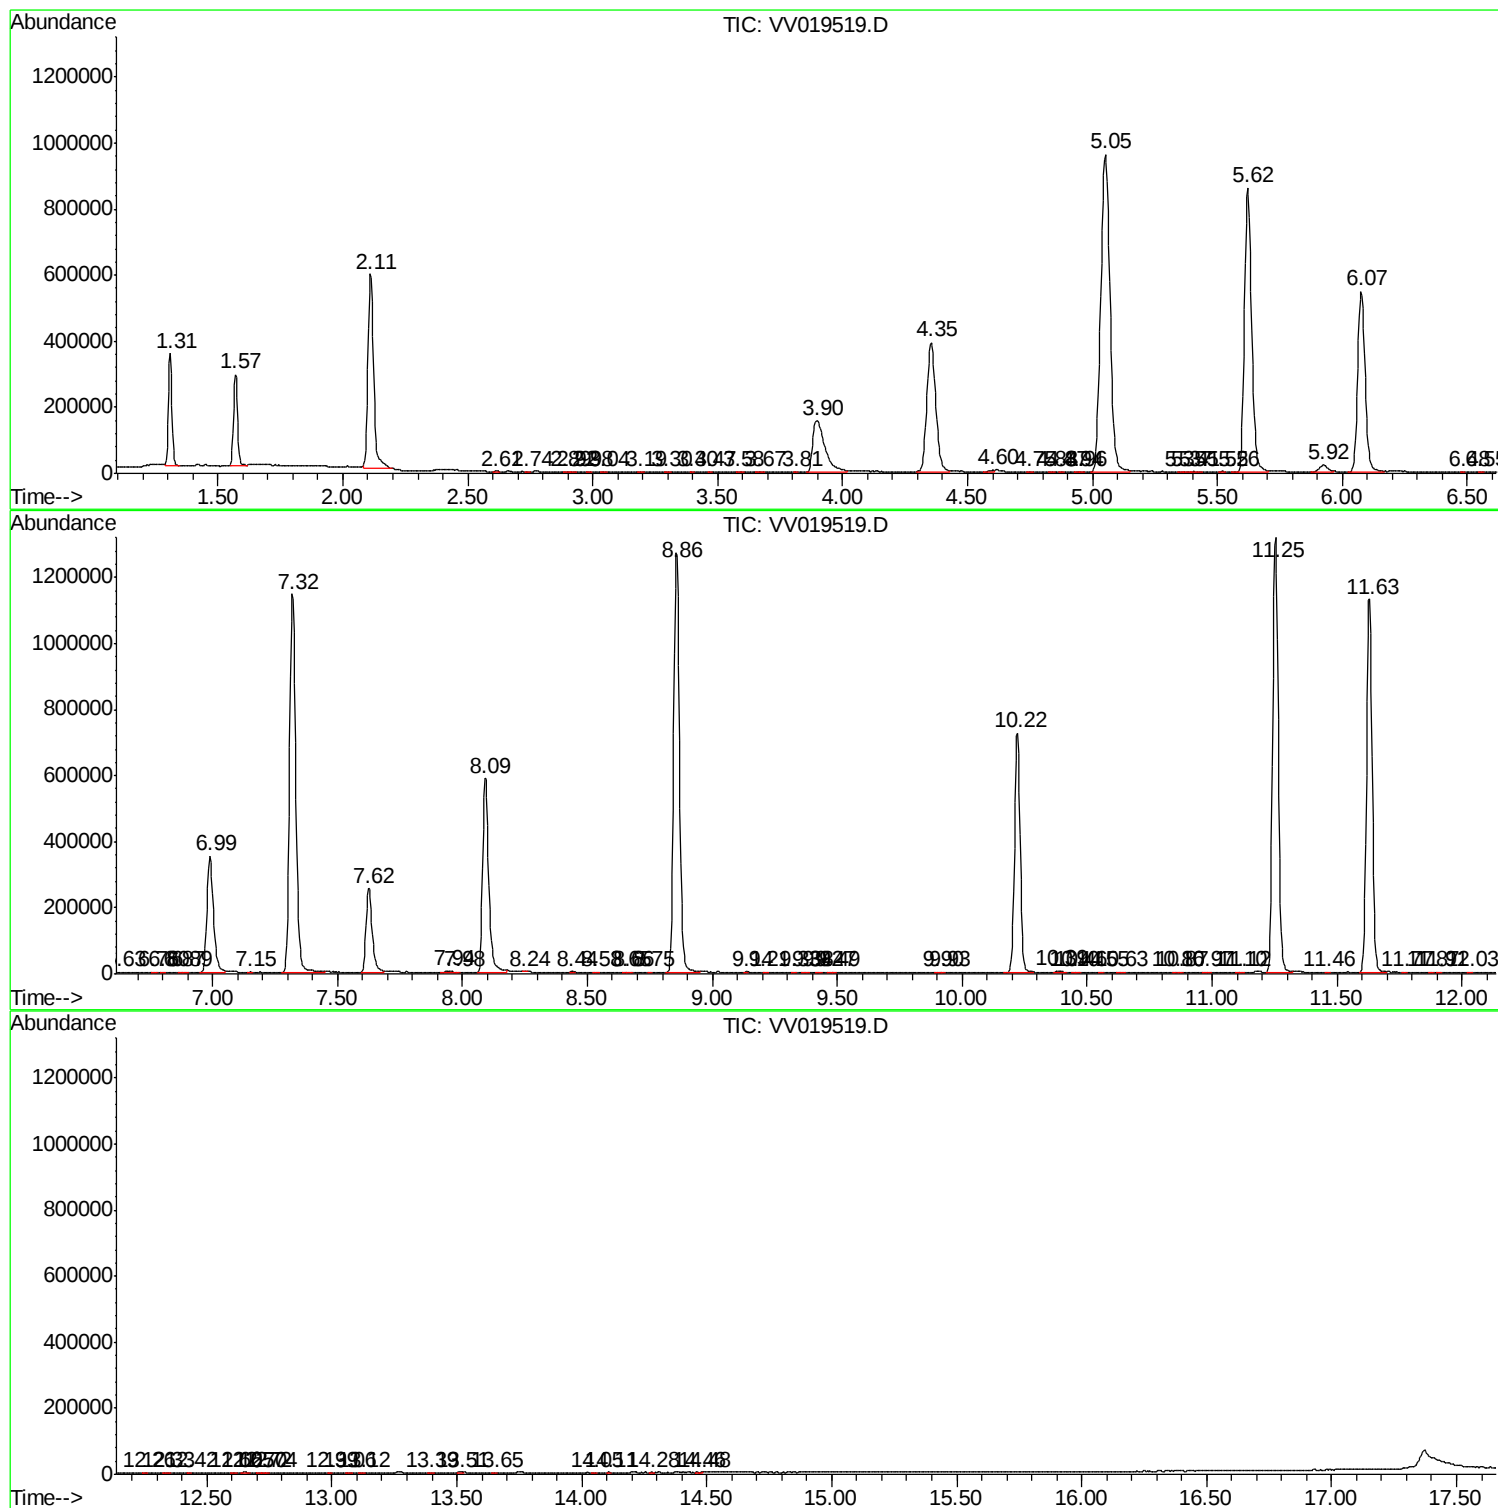

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121020\
Data File : VV019519.D
Acq On : 10 Dec 2020 19:04
Operator : SY/MD
Sample : L4997-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121020\
Data File : VV019519.D
Acq On : 10 Dec 2020 19:04
Operator : SY/MD
Sample : L4997-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc