

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019521.D
 Acq On : 10 Dec 2020 19:52
 Operator : SY/MD
 Sample : L4997-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	83	rVB	345171	333861	13.54%	1.716%
2	1.569	142	149	164	rBV	284837	318879	12.94%	1.639%
3	2.110	308	317	351	rVB	570784	905380	36.73%	4.653%
4	2.357	391	394	396	rBV4	1394	873	0.04%	0.004%
5	2.605	468	471	473	rVB4	1422	833	0.03%	0.004%
6	2.621	473	476	479	rBV4	1127	978	0.04%	0.005%
7	2.872	552	554	559	rBV5	1192	1192	0.05%	0.006%
8	3.087	612	621	624	rBV8	1152	1437	0.06%	0.007%
9	3.126	629	633	637	rVB7	1365	1116	0.05%	0.006%
10	3.248	666	671	673	rBV3	962	760	0.03%	0.004%
11	3.370	707	709	715	rVB5	1372	691	0.03%	0.004%
12	3.476	737	742	747	rVB6	641	756	0.03%	0.004%
13	3.502	747	750	752	rBV3	1081	775	0.03%	0.004%
14	3.579	770	774	779	rBV6	1053	987	0.04%	0.005%
15	3.897	862	873	916	rVV	140167	472482	19.17%	2.428%
16	4.354	996	1015	1039	rBV	397969	977523	39.66%	5.024%
17	4.547	1072	1075	1077	rBV4	1091	718	0.03%	0.004%
18	4.666	1109	1112	1115	rBV4	859	733	0.03%	0.004%
19	4.698	1119	1122	1130	rVB6	1436	1443	0.06%	0.007%
20	4.756	1138	1140	1144	rVB4	918	639	0.03%	0.003%
21	4.836	1163	1165	1169	rVV5	701	625	0.03%	0.003%
22	5.052	1213	1232	1258	rBV2	964870	2464971	100.00%	12.668%
23	5.415	1341	1345	1349	rVB6	1191	865	0.04%	0.004%
24	5.434	1349	1351	1356	rVB7	1277	842	0.03%	0.004%
25	5.540	1381	1384	1391	rVB6	1114	1427	0.06%	0.007%
26	5.621	1395	1409	1437	rBV	852476	1705284	69.18%	8.764%
27	5.833	1473	1475	1480	rBV5	1154	1108	0.04%	0.006%
28	5.917	1494	1501	1514	rVB5	5451	12280	0.50%	0.063%
29	6.003	1524	1528	1532	rVB6	1224	1011	0.04%	0.005%
30	6.074	1532	1550	1583	rBV	558500	1139698	46.24%	5.857%
31	6.280	1612	1614	1621	rVB6	1968	1723	0.07%	0.009%
32	6.312	1621	1624	1628	rBV4	1283	1236	0.05%	0.006%
33	6.383	1644	1646	1649	rBV5	861	748	0.03%	0.004%
34	6.508	1681	1685	1691	rVB8	1424	1723	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019521.D
 Acq On : 10 Dec 2020 19:52
 Operator : SY/MD
 Sample : L4997-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.630	1719	1723	1724	rBV4	1484	1011	0.04%	0.005%
36	6.691	1737	1742	1745	rVB7	927	836	0.03%	0.004%
37	6.724	1748	1752	1753	rBV3	975	646	0.03%	0.003%
38	6.759	1761	1763	1768	rVB6	785	623	0.03%	0.003%
39	6.788	1768	1772	1775	rBV6	745	628	0.03%	0.003%
40	6.849	1788	1791	1798	rVB7	1128	1089	0.04%	0.006%
41	6.910	1805	1810	1812	rBV5	1474	1125	0.05%	0.006%
42	6.990	1823	1835	1863	rBV	355004	644342	26.14%	3.311%
43	7.318	1924	1937	1960	rBV	1144052	1990631	80.76%	10.230%
44	7.556	2007	2011	2015	rBV5	1292	1323	0.05%	0.007%
45	7.624	2022	2032	2053	rBV	249770	435052	17.65%	2.236%
46	7.942	2123	2131	2141	rBV3	3096	5473	0.22%	0.028%
47	7.981	2141	2143	2148	rBV4	1168	673	0.03%	0.003%
48	8.093	2167	2178	2200	rBV	580415	996593	40.43%	5.122%
49	8.553	2318	2321	2328	rVB7	1516	1487	0.06%	0.008%
50	8.588	2328	2332	2336	rVB5	944	772	0.03%	0.004%
51	8.614	2336	2340	2343	rBV5	1180	968	0.04%	0.005%
52	8.630	2343	2345	2352	rVB6	1059	840	0.03%	0.004%
53	8.707	2367	2369	2375	rBV5	675	749	0.03%	0.004%
54	8.855	2401	2415	2437	rBV	1268627	2060127	83.58%	10.587%
55	9.113	2486	2495	2496	rBV7	1087	1625	0.07%	0.008%
56	9.338	2558	2565	2567	rBV5	837	940	0.04%	0.005%
57	9.444	2595	2598	2600	rBV2	912	625	0.03%	0.003%
58	9.547	2623	2630	2638	rVV10	1321	2296	0.09%	0.012%
59	9.707	2675	2680	2685	rBV8	1239	1524	0.06%	0.008%
60	9.775	2698	2701	2702	rBV3	1115	675	0.03%	0.003%
61	9.955	2754	2757	2760	rVB2	1349	967	0.04%	0.005%
62	10.013	2771	2775	2782	rVB5	1185	1305	0.05%	0.007%
63	10.132	2807	2812	2816	rBV6	1037	1051	0.04%	0.005%
64	10.222	2827	2840	2861	rBV	725178	1143728	46.40%	5.878%
65	10.341	2874	2877	2879	rBV3	1232	824	0.03%	0.004%
66	10.386	2884	2891	2898	rVB6	4485	6961	0.28%	0.036%
67	10.431	2903	2905	2909	rVB4	1058	782	0.03%	0.004%
68	10.460	2909	2914	2916	rBV4	873	789	0.03%	0.004%
69	10.543	2935	2940	2945	rBV8	1753	1995	0.08%	0.010%
70	10.730	2995	2998	3002	rBV4	1000	640	0.03%	0.003%
71	10.862	3034	3039	3044	rVB7	1877	1545	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019521.D
 Acq On : 10 Dec 2020 19:52
 Operator : SY/MD
 Sample : L4997-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.913	3051	3055	3056	rBV2	1340	916	0.04%	0.005%
73	11.119	3114	3119	3121	rBV4	789	659	0.03%	0.003%
74	11.148	3121	3128	3129	rBV6	679	669	0.03%	0.003%
75	11.177	3132	3137	3138	rBV4	1534	1018	0.04%	0.005%
76	11.254	3148	3161	3183	rBV	1281149	1986218	80.58%	10.207%
77	11.476	3225	3230	3235	rBV7	1310	1360	0.06%	0.007%
78	11.540	3244	3250	3252	rBV4	1765	1815	0.07%	0.009%
79	11.627	3265	3277	3300	rVV	1140395	1773806	71.96%	9.116%
80	11.820	3333	3337	3340	rBV4	1143	827	0.03%	0.004%
81	11.929	3368	3371	3374	rBV4	901	686	0.03%	0.004%
82	11.971	3382	3384	3388	rVB4	984	723	0.03%	0.004%
83	12.112	3423	3428	3431	rBV5	1270	1112	0.05%	0.006%
84	12.173	3442	3447	3448	rBV4	1122	934	0.04%	0.005%
85	12.318	3490	3492	3497	rVB4	1378	948	0.04%	0.005%
86	12.350	3497	3502	3505	rBV7	1268	1333	0.05%	0.007%
87	12.534	3556	3559	3564	rVV7	1017	1023	0.04%	0.005%
88	12.649	3591	3595	3598	rBV3	2556	2381	0.10%	0.012%
89	12.778	3629	3635	3638	rVB7	1560	1441	0.06%	0.007%
90	12.952	3686	3689	3696	rVB6	716	691	0.03%	0.004%
91	13.276	3782	3790	3797	rVB10	2134	3392	0.14%	0.017%
92	13.344	3807	3811	3814	rBV4	819	715	0.03%	0.004%
93	13.360	3814	3816	3822	rVB4	935	623	0.03%	0.003%
94	13.514	3858	3864	3870	rVB8	1193	1656	0.07%	0.009%
95	13.598	3886	3890	3893	rBV4	900	767	0.03%	0.004%
96	14.022	4018	4022	4025	rBV4	1192	1121	0.05%	0.006%
97	14.193	4072	4075	4078	rBV4	1148	733	0.03%	0.004%
98	14.633	4210	4212	4216	rVB4	1360	798	0.03%	0.004%
99	14.881	4285	4289	4291	rBV4	1045	822	0.03%	0.004%
100	15.704	4543	4545	4547	rBV2	1310	772	0.03%	0.004%


Sum of corrected areas: 19458816

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121020\
Data File : VV019521.D
Acq On : 10 Dec 2020 19:52
Operator : SY/MD
Sample : L4997-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

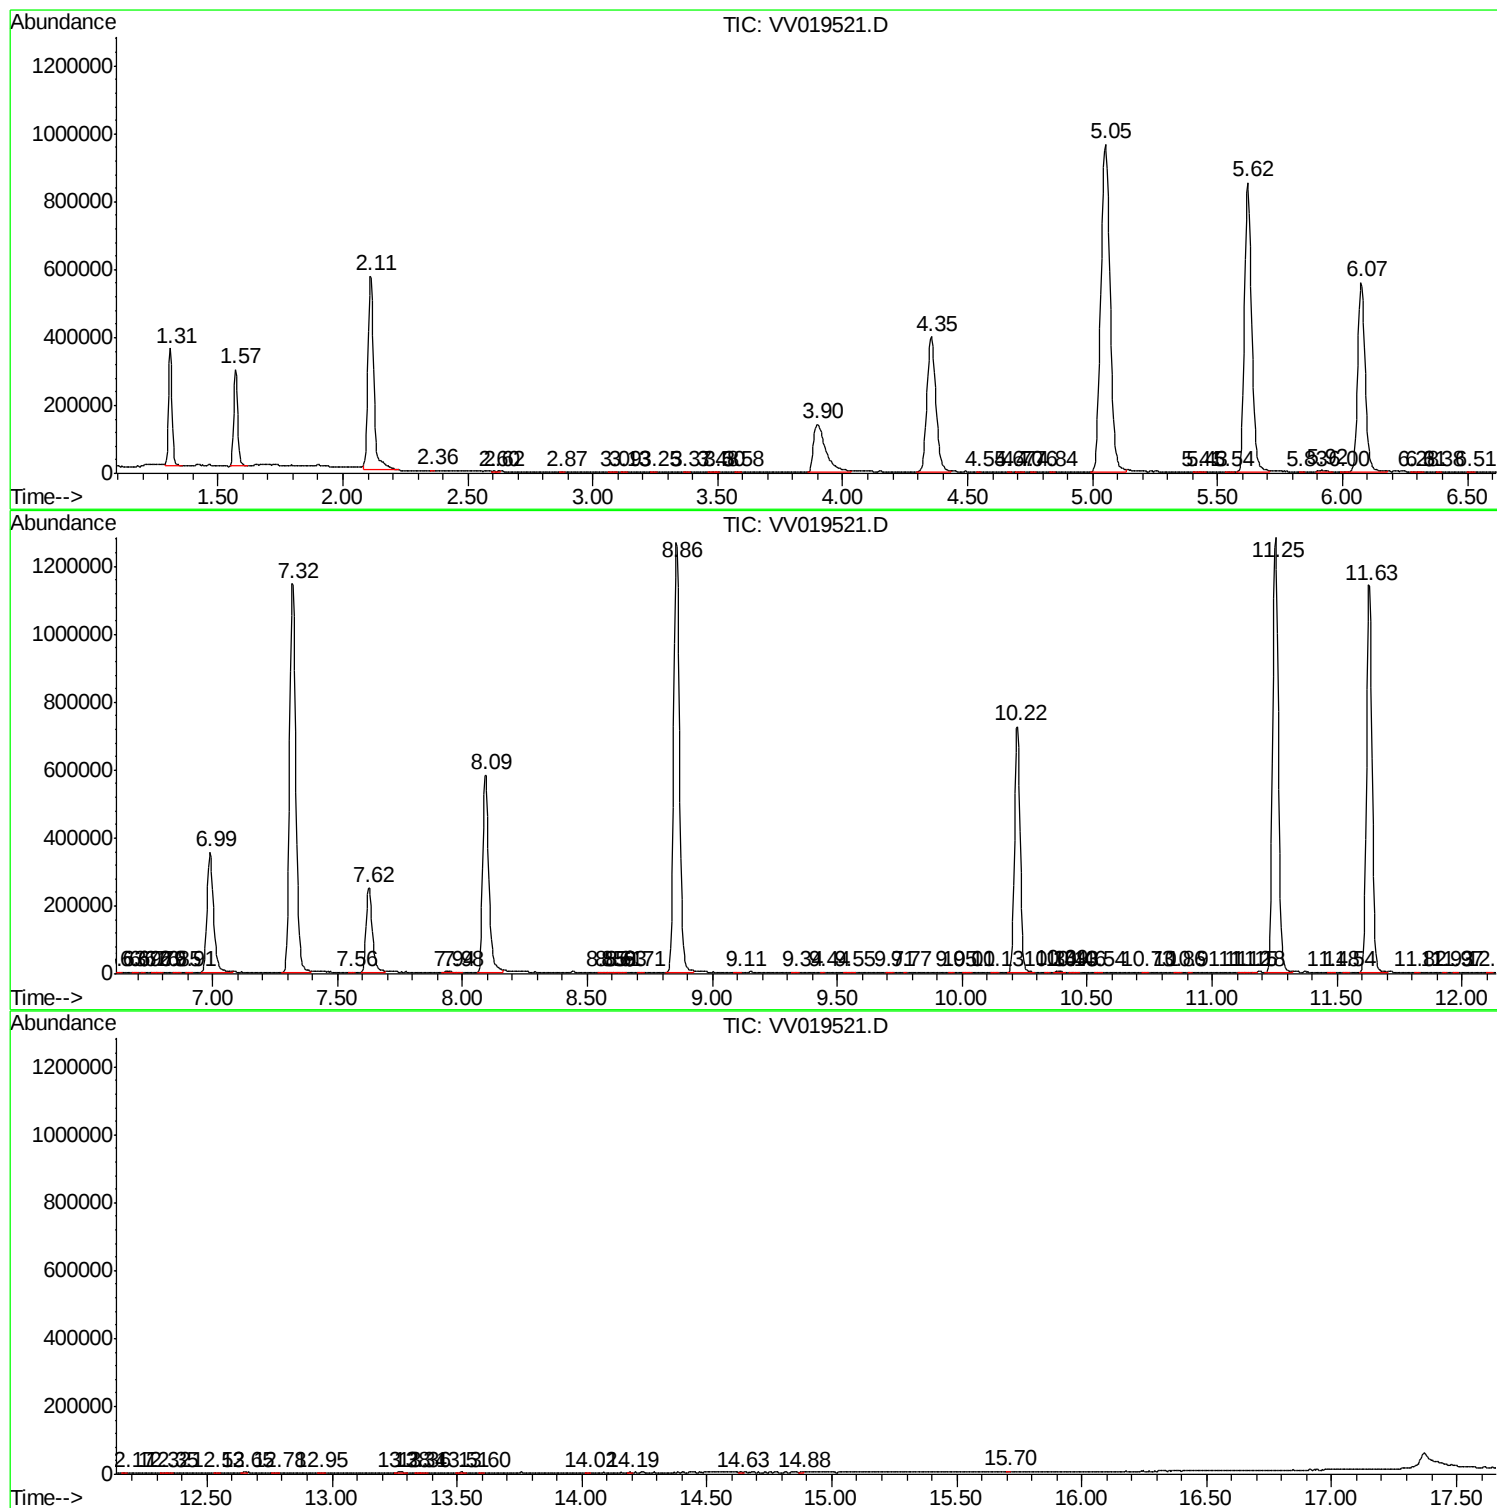

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121020\
Data File : VV019521.D
Acq On : 10 Dec 2020 19:52
Operator : SY/MD
Sample : L4997-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121020\
Data File : VV019521.D
Acq On : 10 Dec 2020 19:52
Operator : SY/MD
Sample : L4997-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc