

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019529.D
 Acq On : 10 Dec 2020 23:03
 Operator : SY/MD
 Sample : L4997-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	77	rVB	339042	324579	13.04%	1.653%
2	1.569	143	149	162	rVB	283692	312827	12.57%	1.593%
3	2.113	309	318	358	rVB2	608115	1007125	40.46%	5.128%
4	2.965	581	583	586	rBV3	825	475	0.02%	0.002%
5	3.341	697	700	703	rBV4	518	471	0.02%	0.002%
6	3.399	716	718	721	rBV3	691	311	0.01%	0.002%
7	3.495	745	748	750	rBV3	627	449	0.02%	0.002%
8	3.553	762	766	768	rBV4	497	449	0.02%	0.002%
9	3.579	771	774	776	rBV2	912	458	0.02%	0.002%
10	3.595	776	779	781	rBV3	950	689	0.03%	0.004%
11	3.611	782	784	789	rVB4	927	440	0.02%	0.002%
12	3.714	813	816	819	rVB5	579	397	0.02%	0.002%
13	3.730	819	821	824	rBV3	975	535	0.02%	0.003%
14	3.791	837	840	842	rBV3	435	223	0.01%	0.001%
15	3.817	842	848	850	rBV5	984	1000	0.04%	0.005%
16	3.852	857	859	861	rBV2	722	412	0.02%	0.002%
17	3.907	862	876	918	rVV2	174838	627618	25.22%	3.195%
18	4.354	998	1015	1049	rBV	400481	998124	40.10%	5.082%
19	4.785	1147	1149	1151	rBV3	720	471	0.02%	0.002%
20	4.862	1171	1173	1175	rBV3	562	281	0.01%	0.001%
21	4.917	1186	1190	1193	rVB5	811	519	0.02%	0.003%
22	4.942	1193	1198	1200	rBV4	877	683	0.03%	0.003%
23	4.958	1201	1203	1208	rVB4	784	592	0.02%	0.003%
24	5.052	1214	1232	1265	rBV2	966898	2488985	100.00%	12.672%
25	5.537	1380	1383	1384	rBV	698	381	0.02%	0.002%
26	5.621	1396	1409	1442	rBV	852556	1708351	68.64%	8.698%
27	5.923	1491	1503	1519	rBV8	13456	32283	1.30%	0.164%
28	6.074	1537	1550	1575	rBV	552671	1119664	44.98%	5.701%
29	6.553	1696	1699	1700	rBV3	394	236	0.01%	0.001%
30	6.608	1714	1716	1718	rBV3	815	462	0.02%	0.002%
31	6.720	1747	1751	1755	rBV4	1011	821	0.03%	0.004%
32	6.810	1775	1779	1781	rBV3	591	424	0.02%	0.002%
33	6.826	1781	1784	1787	rBV4	867	534	0.02%	0.003%
34	6.875	1796	1799	1802	rBV3	1121	693	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019529.D
 Acq On : 10 Dec 2020 23:03
 Operator : SY/MD
 Sample : L4997-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.891	1802	1804	1808	rVV5	815	481	0.02%	0.002%
36	6.910	1808	1810	1813	rVB4	579	330	0.01%	0.002%
37	6.929	1813	1816	1818	rBV3	977	604	0.02%	0.003%
38	6.990	1823	1835	1864	rBV	352569	639533	25.69%	3.256%
39	7.318	1925	1937	1957	rBV	1162649	1998214	80.28%	10.173%
40	7.624	2022	2032	2054	rBV	248155	430142	17.28%	2.190%
41	8.032	2157	2159	2160	rBV2	451	248	0.01%	0.001%
42	8.093	2167	2178	2208	rBV	558031	974780	39.16%	4.963%
43	8.431	2281	2283	2287	rBV4	575	322	0.01%	0.002%
44	8.521	2308	2311	2312	rBV3	691	442	0.02%	0.002%
45	8.640	2347	2348	2350	rVB2	479	115	0.00%	0.001%
46	8.656	2350	2353	2354	rBV2	563	296	0.01%	0.002%
47	8.704	2365	2368	2371	rVB4	517	303	0.01%	0.002%
48	8.720	2371	2373	2374	rBV2	727	293	0.01%	0.001%
49	8.736	2377	2378	2380	rBV3	467	176	0.01%	0.001%
50	8.778	2387	2391	2393	rVB3	869	576	0.02%	0.003%
51	8.794	2393	2396	2398	rBV2	897	573	0.02%	0.003%
52	8.855	2404	2415	2437	rBV	1301237	2043803	82.11%	10.406%
53	9.203	2520	2523	2526	rVB5	1001	595	0.02%	0.003%
54	9.228	2529	2531	2533	rBV3	792	343	0.01%	0.002%
55	9.328	2559	2562	2564	rBV3	749	296	0.01%	0.002%
56	9.376	2574	2577	2578	rBV3	196	101	0.00%	0.001%
57	9.386	2578	2580	2582	rBV2	413	183	0.01%	0.001%
58	9.399	2582	2584	2585	rBV2	391	136	0.01%	0.001%
59	9.450	2598	2600	2601	rBV3	450	160	0.01%	0.001%
60	9.482	2606	2610	2614	rVV6	941	798	0.03%	0.004%
61	9.537	2624	2627	2628	rVB3	419	166	0.01%	0.001%
62	9.624	2651	2654	2655	rBV3	621	373	0.01%	0.002%
63	9.646	2660	2661	2663	rVV2	932	309	0.01%	0.002%
64	9.659	2663	2665	2666	rVB	381	121	0.00%	0.001%
65	9.701	2676	2678	2680	rBV3	769	500	0.02%	0.003%
66	9.743	2685	2691	2694	rVB4	927	1036	0.04%	0.005%
67	9.772	2694	2700	2702	rBV4	789	696	0.03%	0.004%
68	9.785	2702	2704	2706	rBV	734	331	0.01%	0.002%
69	9.797	2706	2708	2713	rBV3	849	593	0.02%	0.003%
70	9.830	2713	2718	2723	rVB6	682	838	0.03%	0.004%
71	9.855	2723	2726	2728	rBV5	507	412	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019529.D
 Acq On : 10 Dec 2020 23:03
 Operator : SY/MD
 Sample : L4997-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	9.916	2743	2745	2747	rBV2	901	590	0.02%	0.003%
73	9.994	2763	2769	2773	rVB6	748	910	0.04%	0.005%
74	10.026	2773	2779	2781	rBV5	1622	1495	0.06%	0.008%
75	10.135	2810	2813	2815	rBV3	544	339	0.01%	0.002%
76	10.219	2825	2839	2860	rBV	727449	1129349	45.37%	5.750%
77	10.331	2871	2874	2877	rBV5	910	563	0.02%	0.003%
78	10.482	2917	2921	2926	rBV7	831	956	0.04%	0.005%
79	10.749	3002	3004	3010	rVB3	706	575	0.02%	0.003%
80	10.810	3020	3023	3024	rBV3	595	371	0.01%	0.002%
81	10.887	3045	3047	3048	rBV2	487	167	0.01%	0.001%
82	10.939	3061	3063	3064	rBV2	389	128	0.01%	0.001%
83	11.058	3096	3100	3105	rVB8	1113	1052	0.04%	0.005%
84	11.087	3105	3109	3111	rBV2	751	458	0.02%	0.002%
85	11.254	3149	3161	3183	rBV	1287857	1980119	79.56%	10.081%
86	11.630	3265	3278	3300	rBV	1131424	1787605	71.82%	9.101%
87	12.424	3523	3525	3527	rBV3	789	444	0.02%	0.002%
88	12.501	3547	3549	3553	rBV4	705	386	0.02%	0.002%
89	12.656	3593	3597	3601	rBV4	1006	1261	0.05%	0.006%
90	12.730	3617	3620	3622	rBV2	848	568	0.02%	0.003%
91	12.788	3635	3638	3639	rBV2	1030	602	0.02%	0.003%
92	13.325	3803	3805	3810	rBV3	678	599	0.02%	0.003%
93	13.408	3827	3831	3834	rBV4	848	875	0.04%	0.004%
94	13.444	3839	3842	3844	rBV4	762	490	0.02%	0.002%
95	13.479	3851	3853	3857	rVB2	821	399	0.02%	0.002%


Sum of corrected areas: 19641481

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121020\
Data File : VV019529.D
Acq On : 10 Dec 2020 23:03
Operator : SY/MD
Sample : L4997-15
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

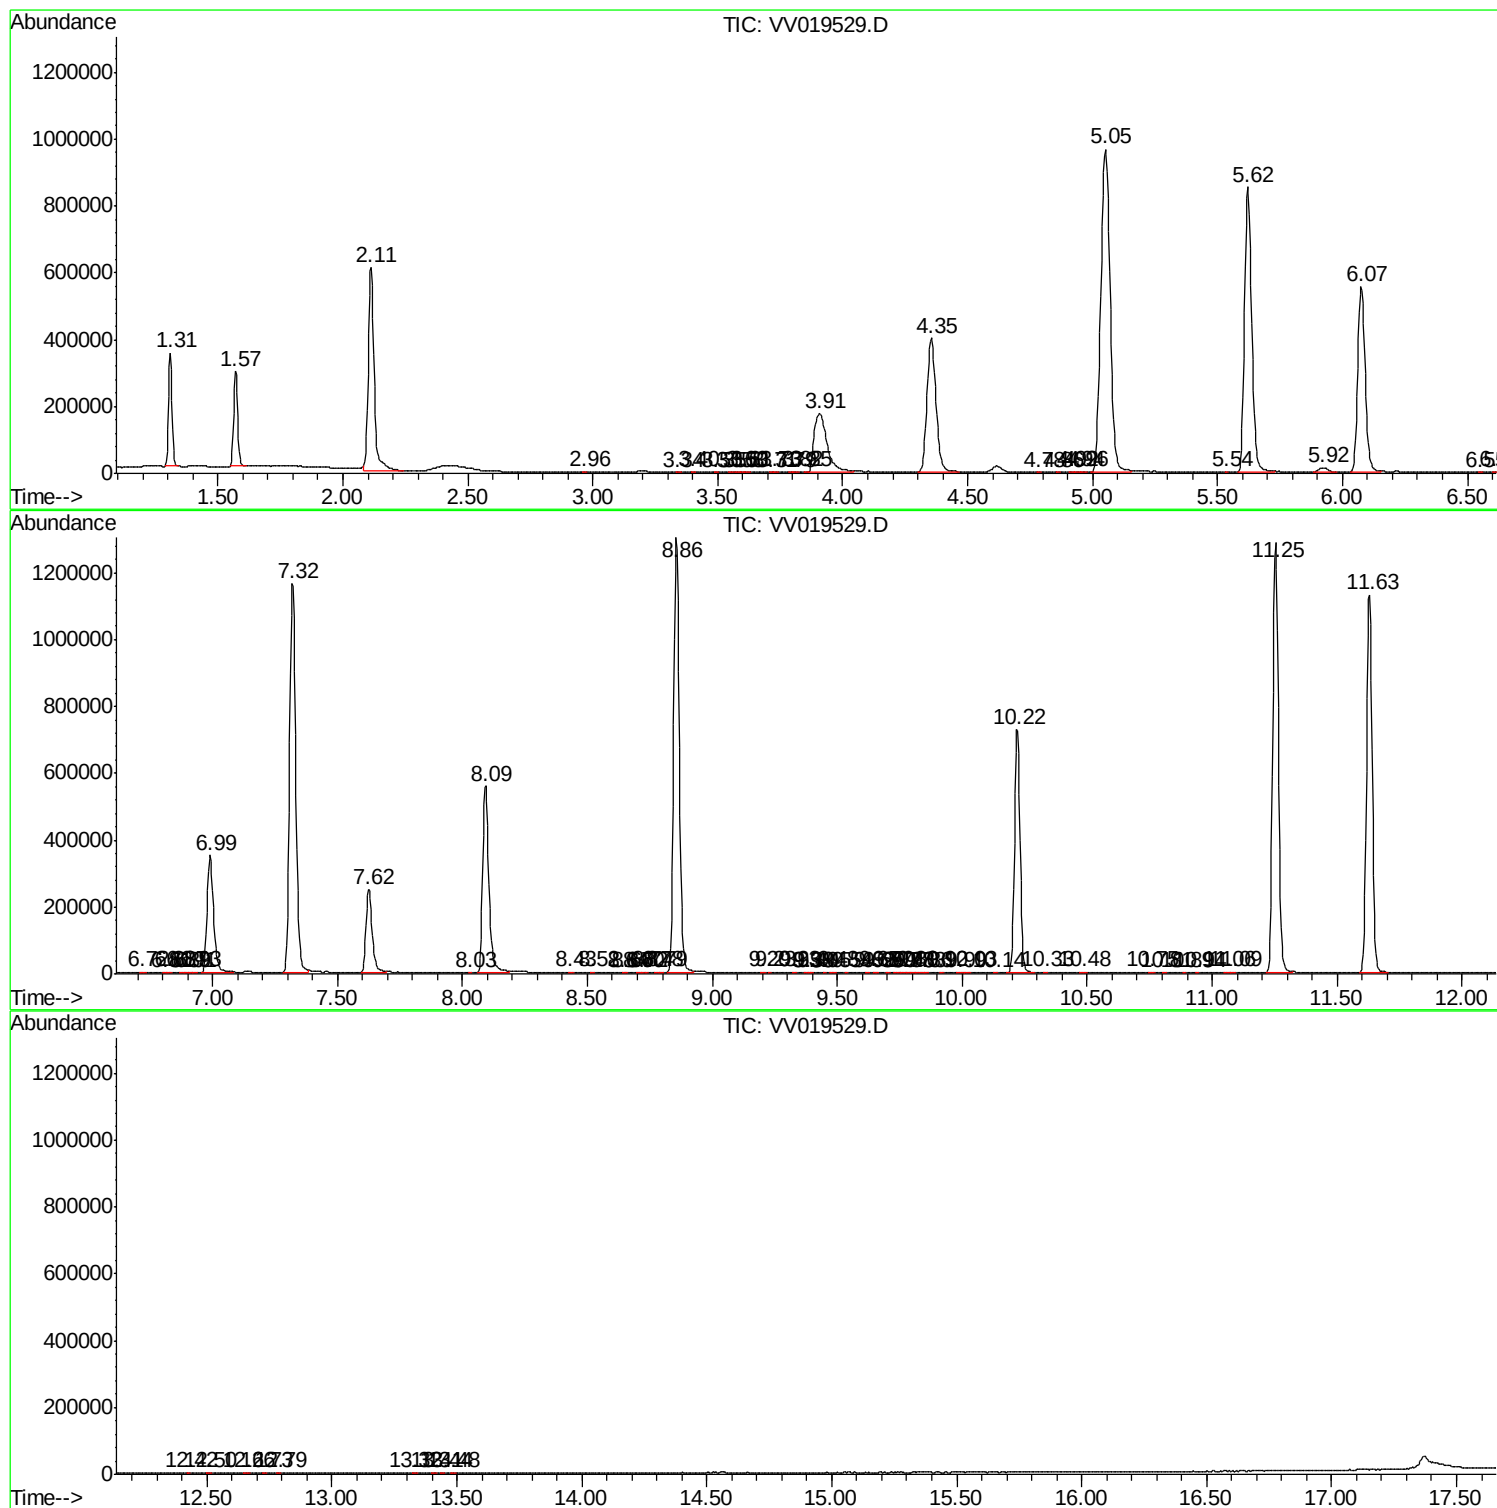

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121020\
Data File : VV019529.D
Acq On : 10 Dec 2020 23:03
Operator : SY/MD
Sample : L4997-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121020\
Data File : VV019529.D
Acq On : 10 Dec 2020 23:03
Operator : SY/MD
Sample : L4997-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc