

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019537.D
 Acq On : 11 Dec 2020 02:38
 Operator : SY/MD
 Sample : VV1210WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK99

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	83	rVB	382674	384007	14.69%	1.904%
2	1.569	143	149	164	rVB	313109	349104	13.36%	1.731%
3	2.113	309	318	362	rVB	626856	1004247	38.42%	4.981%
4	3.106	625	627	628	rBV2	557	172	0.01%	0.001%
5	3.302	684	688	689	rBV2	781	503	0.02%	0.002%
6	3.354	699	704	706	rBV4	692	650	0.02%	0.003%
7	3.482	742	744	748	rBV4	716	449	0.02%	0.002%
8	3.515	751	754	757	rVB5	674	536	0.02%	0.003%
9	3.534	757	760	762	rBV3	498	285	0.01%	0.001%
10	3.543	762	763	769	rBV3	391	379	0.01%	0.002%
11	3.608	778	783	788	rBV4	783	836	0.03%	0.004%
12	3.634	788	791	795	rVV4	609	541	0.02%	0.003%
13	3.656	795	798	800	rVV2	563	323	0.01%	0.002%
14	3.746	823	826	829	rBV5	698	549	0.02%	0.003%
15	3.862	860	862	863	rBV2	552	314	0.01%	0.002%
16	3.900	863	874	917	rVV2	147830	521450	19.95%	2.586%
17	4.354	999	1015	1048	rBV	416779	1030155	39.42%	5.109%
18	4.887	1179	1181	1182	rBV2	467	180	0.01%	0.001%
19	4.907	1184	1187	1190	rBV3	725	540	0.02%	0.003%
20	4.929	1192	1194	1199	rVB6	832	495	0.02%	0.002%
21	5.051	1213	1232	1270	rBV2	1015326	2613577	100.00%	12.962%
22	5.621	1396	1409	1441	rBV	827238	1659101	63.48%	8.228%
23	5.916	1488	1501	1513	rBV9	9652	22538	0.86%	0.112%
24	6.074	1536	1550	1580	rBV	584609	1187364	45.43%	5.889%
25	6.370	1637	1642	1644	rBV3	925	868	0.03%	0.004%
26	6.392	1647	1649	1653	rVB5	563	426	0.02%	0.002%
27	6.495	1679	1681	1683	rBV3	621	412	0.02%	0.002%
28	6.604	1713	1715	1717	rBV2	516	181	0.01%	0.001%
29	6.743	1756	1758	1760	rBV3	746	385	0.01%	0.002%
30	6.788	1769	1772	1774	rBV3	632	420	0.02%	0.002%
31	6.833	1782	1786	1789	rBV5	1047	772	0.03%	0.004%
32	6.913	1808	1811	1813	rBV2	722	498	0.02%	0.002%
33	6.990	1821	1835	1859	rBV	362742	652459	24.96%	3.236%
34	7.318	1925	1937	1960	rBV	1200203	2078898	79.54%	10.310%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019537.D
 Acq On : 11 Dec 2020 02:38
 Operator : SY/MD
 Sample : VV1210WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK99

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	7.624	2022	2032	2065	rBV	256532	447226	17.11%	2.218%
36	7.920	2121	2124	2127	rBV5	492	325	0.01%	0.002%
37	7.942	2127	2131	2133	rBV3	1063	910	0.03%	0.005%
38	8.090	2167	2177	2203	rBV	612131	1054232	40.34%	5.228%
39	8.424	2275	2281	2292	rVB4	4728	6895	0.26%	0.034%
40	8.723	2370	2374	2376	rBV4	762	547	0.02%	0.003%
41	8.855	2403	2415	2451	rBV	1233368	2008983	76.87%	9.964%
42	9.145	2500	2505	2514	rBV8	3126	4877	0.19%	0.024%
43	9.341	2562	2566	2567	rBV3	485	368	0.01%	0.002%
44	9.379	2574	2578	2579	rBV4	758	525	0.02%	0.003%
45	9.418	2586	2590	2592	rBV3	733	486	0.02%	0.002%
46	9.428	2592	2593	2596	rVB2	597	236	0.01%	0.001%
47	9.447	2596	2599	2601	rBV3	692	476	0.02%	0.002%
48	9.501	2613	2616	2618	rBV2	772	420	0.02%	0.002%
49	9.540	2626	2628	2629	rBV3	1054	431	0.02%	0.002%
50	9.704	2676	2679	2683	rBV4	1001	655	0.03%	0.003%
51	9.727	2683	2686	2690	rBV5	880	751	0.03%	0.004%
52	9.743	2690	2691	2694	rBV2	526	250	0.01%	0.001%
53	9.797	2704	2708	2710	rBV4	1080	772	0.03%	0.004%
54	9.845	2720	2723	2725	rBV	671	327	0.01%	0.002%
55	9.936	2744	2751	2755	rBV6	2935	4072	0.16%	0.020%
56	9.968	2760	2761	2763	rVB2	431	101	0.00%	0.001%
57	10.145	2815	2816	2817	rVB2	283	55	0.00%	0.000%
58	10.154	2817	2819	2822	rBV3	516	332	0.01%	0.002%
59	10.218	2827	2839	2857	rBV	761650	1189212	45.50%	5.898%
60	10.453	2909	2912	2914	rBV4	659	421	0.02%	0.002%
61	10.505	2926	2928	2933	rVB4	762	545	0.02%	0.003%
62	10.543	2933	2940	2949	rBV7	3769	5780	0.22%	0.029%
63	10.601	2956	2958	2965	rVB5	739	578	0.02%	0.003%
64	10.653	2971	2974	2979	rVB5	786	702	0.03%	0.003%
65	10.678	2979	2982	2986	rBV5	501	315	0.01%	0.002%
66	10.698	2986	2988	2989	rBV2	374	142	0.01%	0.001%
67	10.710	2990	2992	2993	rBV	365	97	0.00%	0.000%
68	10.720	2993	2995	2998	rBV2	682	405	0.02%	0.002%
69	10.755	3003	3006	3007	rBV2	478	211	0.01%	0.001%
70	10.784	3013	3015	3018	rBV2	419	218	0.01%	0.001%
71	10.855	3031	3037	3038	rBV3	711	606	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121020\
 Data File : VV019537.D
 Acq On : 11 Dec 2020 02:38
 Operator : SY/MD
 Sample : VV1210WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK99

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.878	3042	3044	3046	rVB3	723	264	0.01%	0.001%
73	10.926	3053	3059	3065	rVB5	3903	4537	0.17%	0.023%
74	10.948	3065	3066	3069	rVB3	666	282	0.01%	0.001%
75	11.016	3083	3087	3090	rBV5	631	577	0.02%	0.003%
76	11.074	3103	3105	3108	rVB4	545	201	0.01%	0.001%
77	11.189	3129	3141	3149	rBV10	5977	10800	0.41%	0.054%
78	11.254	3149	3161	3180	rBV	1245703	1936515	74.09%	9.604%
79	11.501	3237	3238	3242	rBV3	518	359	0.01%	0.002%
80	11.530	3245	3247	3249	rBV3	586	319	0.01%	0.002%
81	11.630	3264	3278	3299	rBV	1185326	1870391	71.56%	9.276%
82	11.861	3348	3350	3355	rBV4	666	642	0.02%	0.003%
83	11.955	3376	3379	3382	rVB4	810	501	0.02%	0.002%
84	12.228	3462	3464	3467	rBV2	659	471	0.02%	0.002%
85	12.244	3467	3469	3472	rVV2	1146	617	0.02%	0.003%
86	12.267	3474	3476	3479	rVB4	949	491	0.02%	0.002%
87	12.337	3494	3498	3503	rBV6	1022	1023	0.04%	0.005%
88	12.488	3539	3545	3547	rBV4	928	857	0.03%	0.004%
89	12.649	3588	3595	3605	rBV4	9388	14225	0.54%	0.071%
90	12.794	3637	3640	3643	rVB5	845	562	0.02%	0.003%
91	12.810	3643	3645	3647	rBV3	875	423	0.02%	0.002%
92	13.270	3779	3788	3799	rVB4	14063	22157	0.85%	0.110%
93	13.511	3856	3863	3874	rVB2	18109	27817	1.06%	0.138%
94	13.749	3929	3937	3948	rBV5	13839	22234	0.85%	0.110%


Sum of corrected areas: 20163363

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121020\
Data File : VV019537.D
Acq On : 11 Dec 2020 02:38
Operator : SY/MD
Sample : VV1210WBL02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK99

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

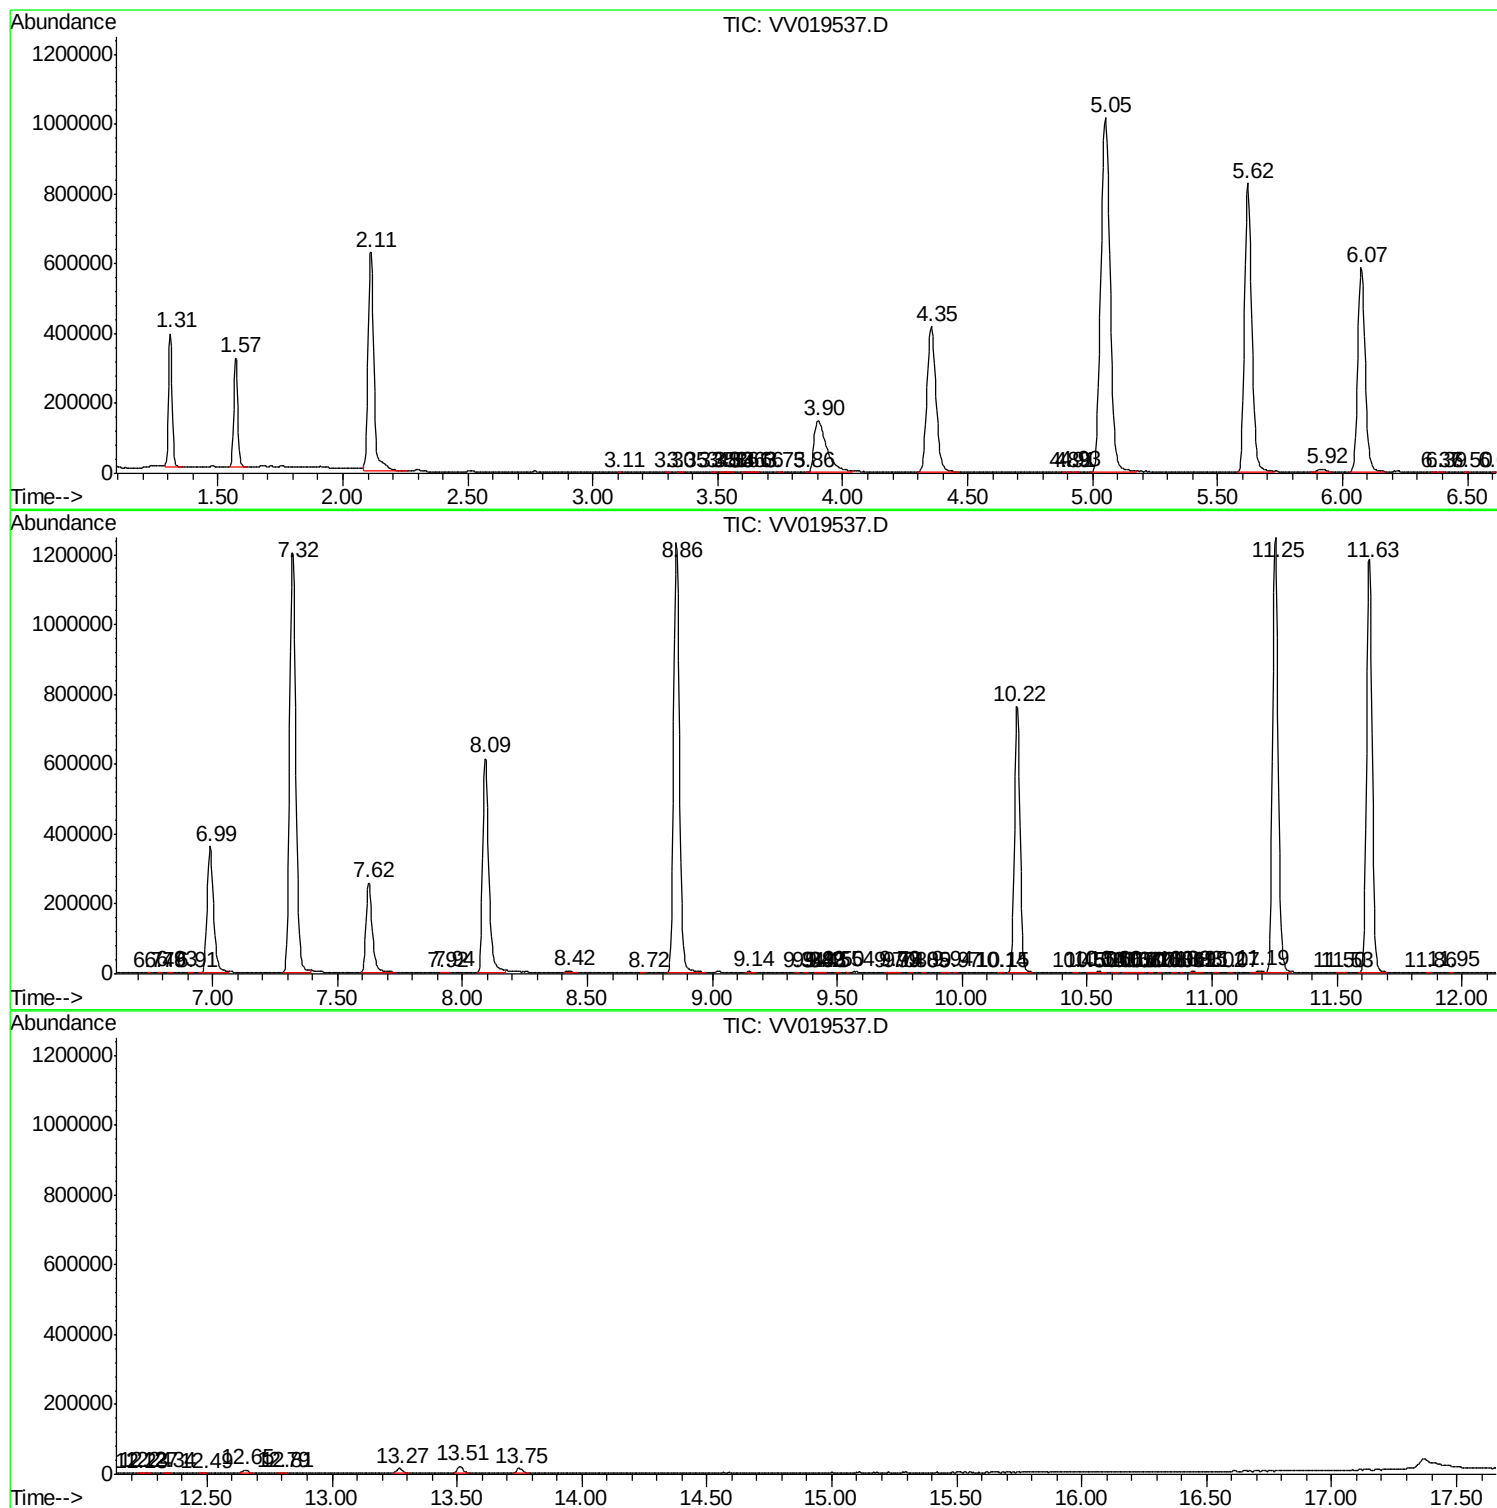

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121020\
Data File : VV019537.D
Acq On : 11 Dec 2020 02:38
Operator : SY/MD
Sample : VV1210WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK99

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121020\
Data File : VV019537.D
Acq On : 11 Dec 2020 02:38
Operator : SY/MD
Sample : VV1210WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK99

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc