


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121020\
 Data File : VV019505.D
 Acq On : 10 Dec 2020 09:38
 Operator : SY/MD
 Sample : BFB63
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB63

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR010220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jan 29 12:34:48 2020

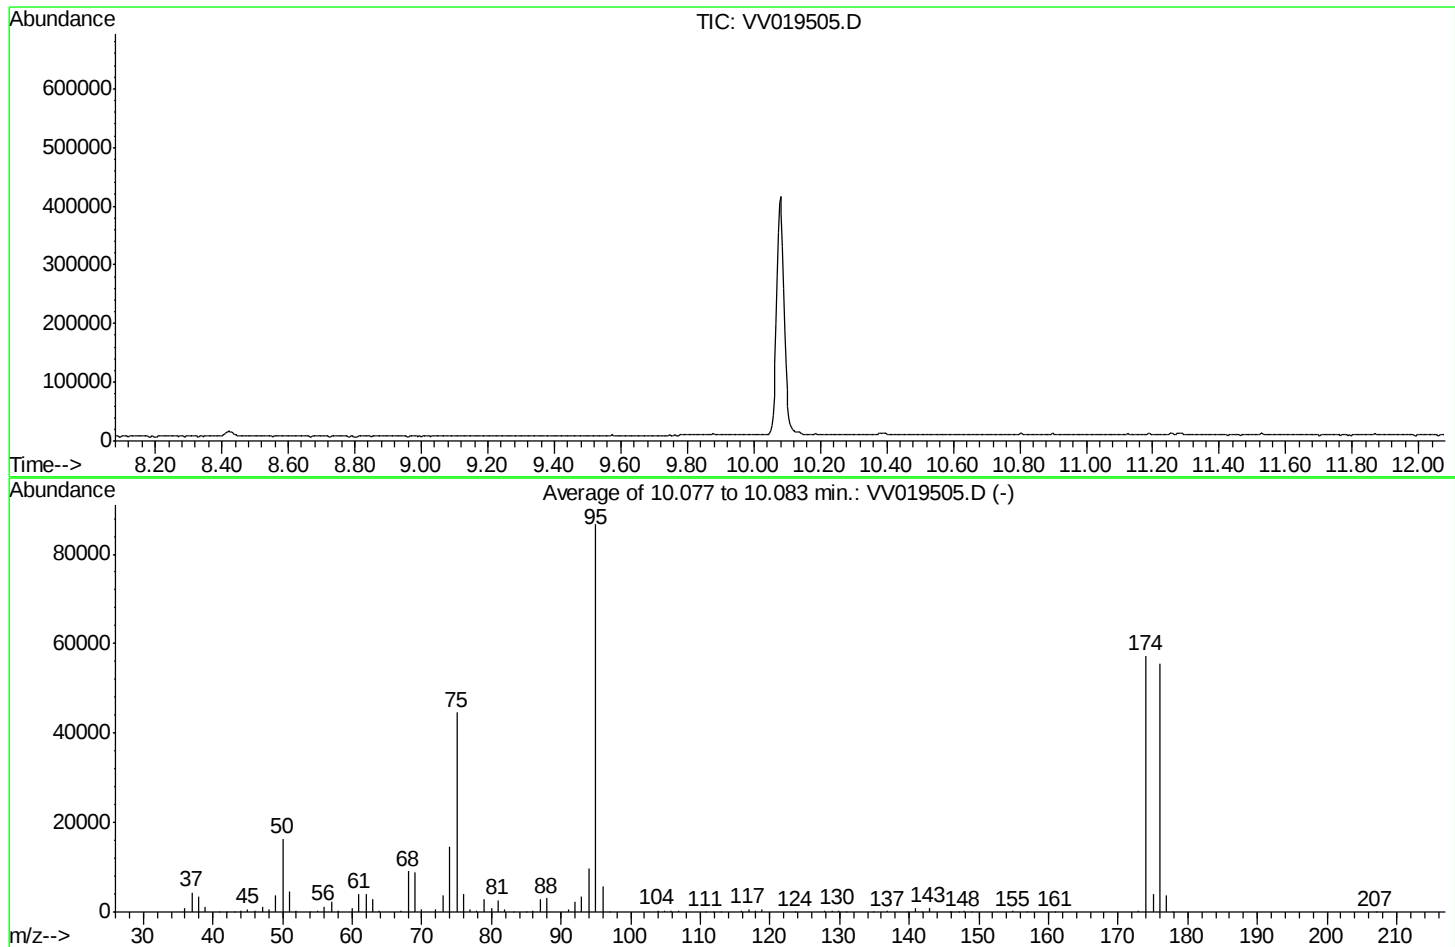

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2782

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	16433	PASS
75	95	30	80	51.4	44565	PASS
95	95	100	100	100.0	86685	PASS
96	95	5	9	6.7	5823	PASS
173	174	0.00	2	0.7	374	PASS
174	95	50	120	66.1	57256	PASS
175	174	5	9	7.2	4134	PASS
176	174	95	101	96.9	55456	PASS
177	176	5	9	6.8	3782	PASS

m/z	Abundance
36.00	2563.0
37.00	4769.0
38.00	4458.0
39.00	1822.0
39.90	415.0
41.00	538.0
42.00	278.0
43.00	776.0
44.00	2847.0
45.00	848.0
46.00	202.0
47.00	1086.0
48.00	618.0
49.00	3692.0
50.00	17304.0
51.10	4899.0
52.00	418.0
53.10	118.0
54.00	117.0
55.00	621.0
55.90	1528.0
57.00	2532.0
58.00	189.0
60.00	1002.0
61.00	4029.0
62.00	3951.0
63.00	3206.0
64.00	316.0
67.10	399.0
68.00	9384.0
69.00	9462.0
70.00	696.0
71.10	179.0
72.00	614.0
73.00	3866.0
74.00	15011.0
75.00	44968.0
76.00	3962.0
77.00	626.0
78.00	305.0
78.90	3066.0
80.00	921.0
80.90	2870.0
81.90	756.0
82.80	138.0
85.00	120.0
86.00	186.0
86.90	2824.0
87.90	3111.0
91.00	563.0
92.00	2254.0
93.00	3571.0
94.00	9656.0
95.00	86888.0
96.00	6171.0
97.10	233.0
98.20	113.0
103.90	372.0
104.90	170.0
106.00	373.0
106.90	141.0
110.80	134.0
115.90	348.0
116.90	688.0
117.90	392.0
118.90	573.0
123.70	124.0
127.80	281.0
128.90	220.0
129.90	357.0
131.10	142.0
135.00	128.0
137.00	156.0
139.90	117.0
140.90	859.0
141.80	111.0
142.90	1051.0
145.80	122.0
147.10	120.0
147.80	172.0
148.90	103.0
155.00	167.0
156.90	155.0
160.90	137.0
172.80	558.0
174.00	55976.0
175.00	4160.0
176.00	54256.0
177.00	3846.0
177.90	119.0
207.00	200.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	2582.0
37.00	4751.0
38.00	4329.0
39.00	1772.0
39.90	428.0
41.00	523.0
41.90	329.0
43.00	770.0
44.00	2939.0
45.00	964.0
46.10	186.0
47.10	1084.0
48.00	569.0
49.00	3714.0
50.10	17032.0
51.00	5012.0
52.00	376.0
52.90	129.0
55.00	568.0
56.00	1438.0
57.00	2656.0
58.00	197.0
60.00	1116.0
61.00	4175.0
62.00	3959.0
63.00	3079.0
64.00	355.0
65.10	106.0
67.00	398.0
68.00	9421.0
69.00	9246.0
70.00	726.0
71.10	138.0
72.00	660.0
73.00	3841.0
74.00	15089.0
75.00	46200.0
76.00	4053.0
77.00	616.0
77.90	293.0
78.90	3019.0
80.00	911.0
80.90	2994.0
81.90	757.0
83.10	177.0
85.10	119.0
86.00	179.0
87.00	2981.0
88.00	3209.0
91.00	563.0
91.90	2297.0
93.00	3622.0
94.00	10081.0
95.00	89776.0
96.00	6075.0
97.00	232.0
98.20	111.0
103.90	385.0
104.90	208.0
105.90	343.0
106.90	164.0
110.80	108.0
113.00	111.0
115.90	399.0
116.90	698.0
117.90	420.0
118.90	592.0
127.90	312.0
129.00	241.0
129.80	374.0
131.00	144.0
134.90	134.0
136.90	153.0
139.80	149.0
140.90	868.0
141.80	126.0
142.90	1012.0
146.00	121.0
147.00	125.0
147.90	192.0
155.00	165.0
156.90	136.0
160.90	163.0
172.80	566.0
174.00	59192.0
175.00	4296.0
176.00	57296.0
177.00	3899.0
177.80	129.0
207.00	190.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	2556.0
37.00	4382.0
38.00	3869.0
39.00	1556.0
39.90	441.0
41.00	496.0
42.00	360.0
43.00	676.0
44.00	3015.0
45.00	1021.0
46.10	145.0
47.10	973.0
48.00	475.0
49.00	3520.0
50.00	15337.0
51.00	4730.0
52.00	319.0
53.00	153.0
55.00	490.0
56.00	1371.0
57.00	2495.0
58.00	167.0
59.90	1043.0
61.00	3951.0
62.00	3835.0
63.00	2649.0
63.90	381.0
67.00	417.0
68.00	8528.0
69.00	8334.0
70.00	714.0
72.00	616.0
73.00	3443.0
74.00	13894.0
75.00	42528.0
76.00	3759.0
76.90	560.0
77.80	316.0
78.90	2662.0
80.00	813.0
80.90	2762.0
81.90	682.0
83.10	219.0
85.00	116.0
86.00	165.0
87.00	2883.0
88.00	3029.0
91.00	481.0
91.90	2179.0
93.00	3384.0
94.00	9323.0
95.00	83392.0
96.00	5630.0
97.10	245.0
98.10	122.0
103.80	391.0
104.90	209.0
105.80	309.0
107.00	166.0
111.90	115.0
113.00	124.0
115.90	381.0
116.90	572.0
117.90	360.0
118.90	512.0
127.90	308.0
129.00	206.0
129.80	332.0
131.00	148.0
134.80	144.0
136.80	165.0
139.70	136.0
140.90	836.0
141.70	101.0
142.90	936.0
146.00	136.0
147.00	107.0
147.90	200.0
154.90	175.0
156.90	110.0
161.00	120.0
174.00	56600.0
175.00	3946.0
176.00	54816.0
177.00	3602.0
178.00	102.0
207.10	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	1710.0
36.90	194.0
37.90	738.0
38.90	438.0
40.00	461.0
40.90	493.0
42.10	253.0
43.00	637.0
44.00	2603.0
44.90	278.0
50.00	124.0
51.10	152.0
53.00	145.0
55.10	373.0
55.90	256.0
57.20	279.0
60.00	170.0
65.00	170.0
65.90	140.0
66.90	158.0
69.10	265.0
71.00	138.0
79.10	127.0
81.10	148.0
82.00	208.0
82.90	117.0
84.00	111.0
95.80	135.0
96.90	141.0
98.00	152.0
105.80	103.0
207.00	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63