

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023890.D
 Acq On : 10 Dec 2021 16:42
 Operator : SY/MD
 Sample : M5003-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CX6




Manual IntegrationsAPPROVED

Quant Time: Dec 11 04:46:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

Reviewed By :Mahesh
 Dadoda

12/13/2021
 Supervised By :Semsettin
 Yesilyurt

12/13/2021

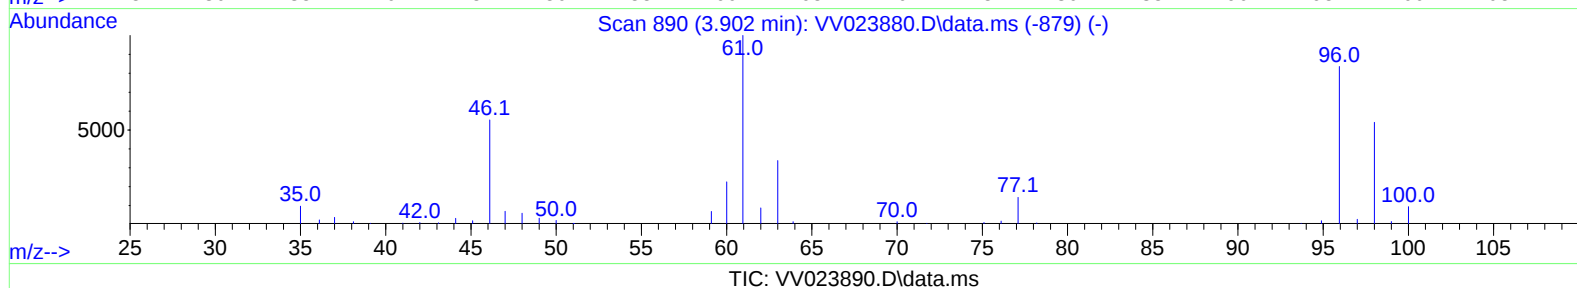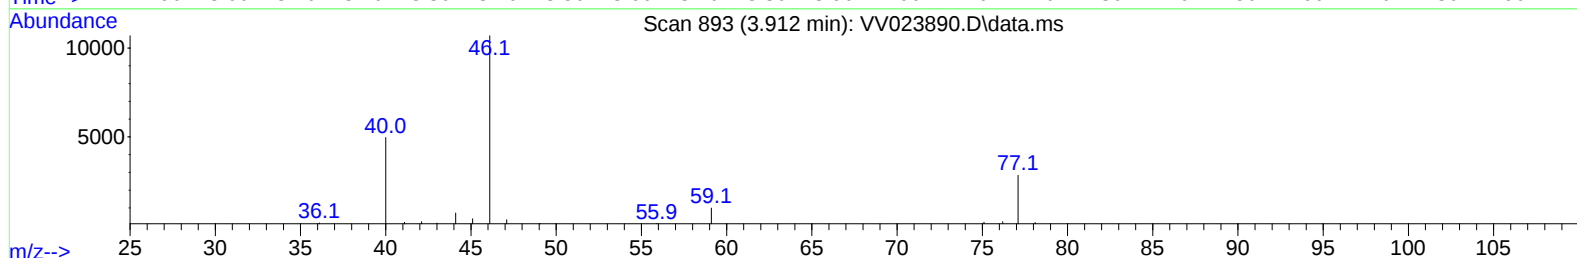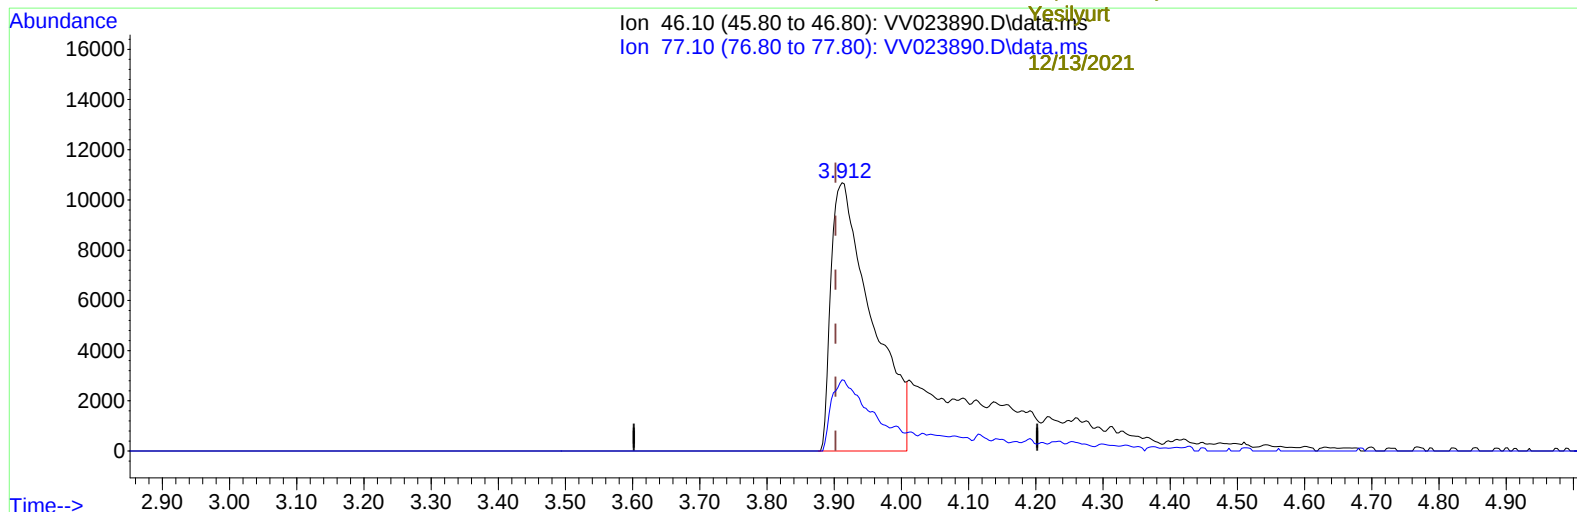

TIC: VV023890.D\data.ms

(20) 2-Butanone-d5 (S)

3.912min (+ 0.010) 37.15 ug/L

response 45120

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.40	24.01#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023890.D
Acq On : 10 Dec 2021 16:42
Operator : SY/MD
Sample : M5003-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CX6




Manual IntegrationsAPPROVED

Quant Time: Dec 11 04:46:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 11 04:33:17 2021
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

12/13/2021
Supervised By :Semsettin
Yesilyurt

12/13/2021

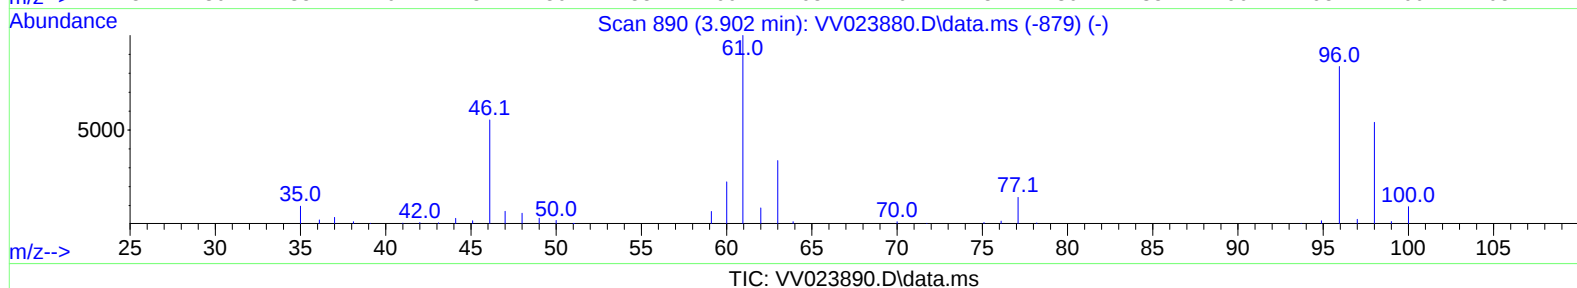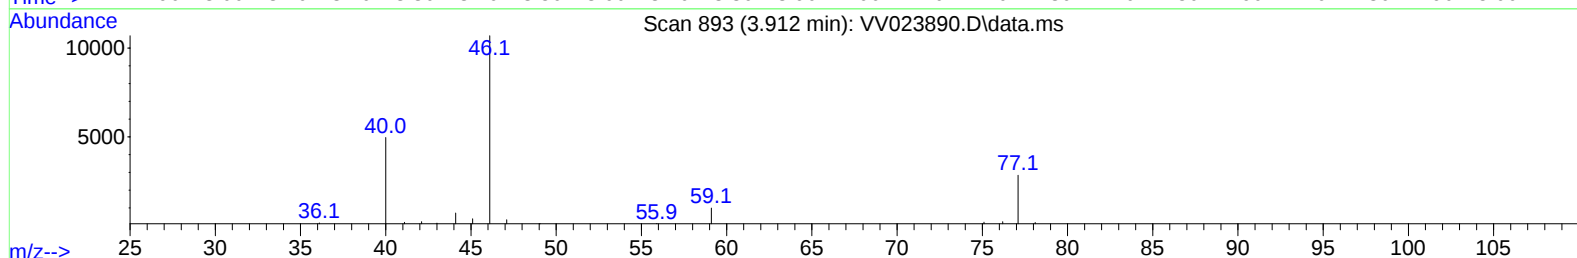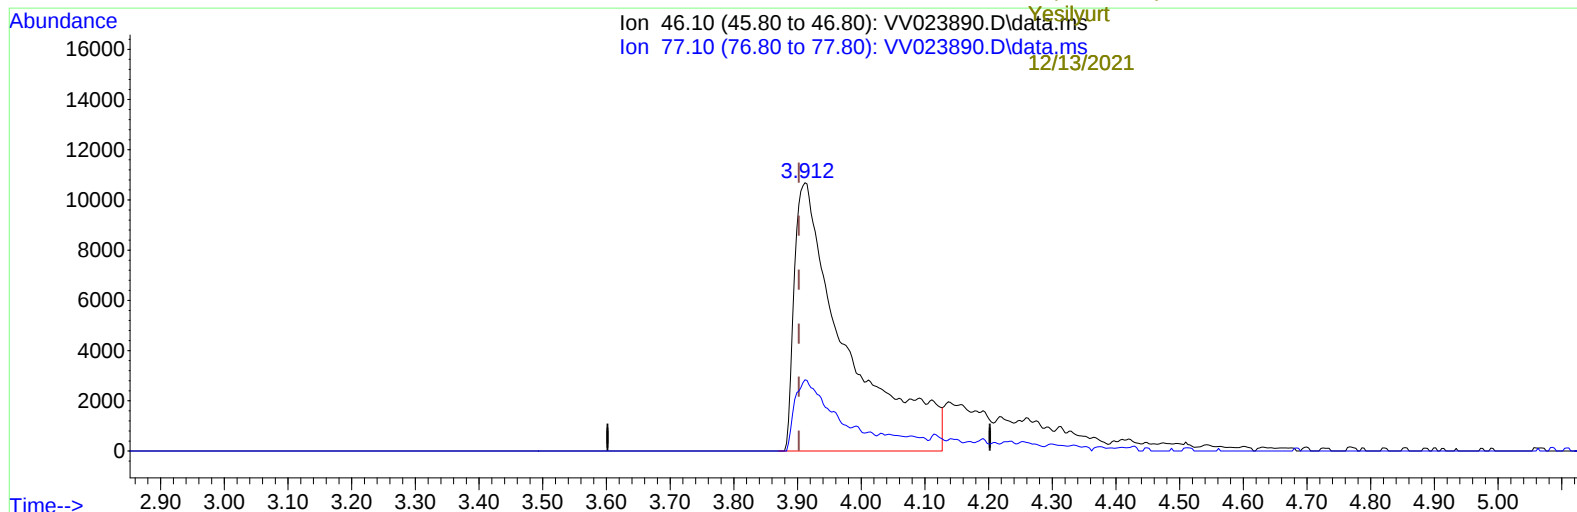

TIC: VV023890.D\data.ms

(20) 2-Butanone-d5 (S)

3.912min (+ 0.010) 49.78 ug/L m

response 60466

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.40	17.92#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121021\
 Data File : VW023890.D
 Acq On : 10 Dec 2021 16:42
 Operator : SY/MD
 Sample : M5003-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CX6

Manual IntegrationsAPPROVED

Quant Time: Dec 11 04:46:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

Reviewed By :Mahesh
 Dadoda

12/13/2021
 Supervised By :Semsettin
 Yesilyurt

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	115645	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	120283	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59775	5.000	ug/L	0.00

12/13/2021

System Monitoring Compounds

4) Vinyl Chloride-d3	1.307	65	27257	4.384	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	87.600%	
7) Chloroethane-d5	1.568	69	24687	4.759	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	95.200%	
11) 1,1-Dichloroethene-d2	2.108	63	37586	3.097	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	62.000%	
20) 2-Butanone-d5	3.912	46	60466m	49.782	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	99.560%	
24) Chloroform-d	4.352	84	64528	4.582	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.600%	
26) 1,2-Dichloroethane-d4	5.037	65	31441	4.795	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.000%	
32) Benzene-d6	5.050	84	111792	4.692	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.800%	
36) 1,2-Dichloropropane-d6	6.072	67	34888	4.854	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.000%	
41) Toluene-d8	7.317	98	90853	4.236	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.800%	
43) trans-1,3-Dichloroprop...	7.625	79	13986	4.690	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	93.800%	
46) 2-Hexanone-d5	8.092	63	62631	46.920	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	93.840%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	26968	4.523	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	90.400%	
66) 1,2-Dichlorobenzene-d4	11.625	152	41864	5.243	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	104.800%	

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023890.D
Acq On : 10 Dec 2021 16:42
Operator : SY/MD
Sample : M5003-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CX6

Manual IntegrationsAPPROVED

Quant Time: Dec 11 04:46:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 11 04:33:17 2021
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

12/13/2021
Supervised By :Semsettin
Yesilyurt

12/13/2021

