




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023917.D
 Acq On : 11 Dec 2021 03:50
 Operator : SY/MD
 Sample : M5025-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D09

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:06:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

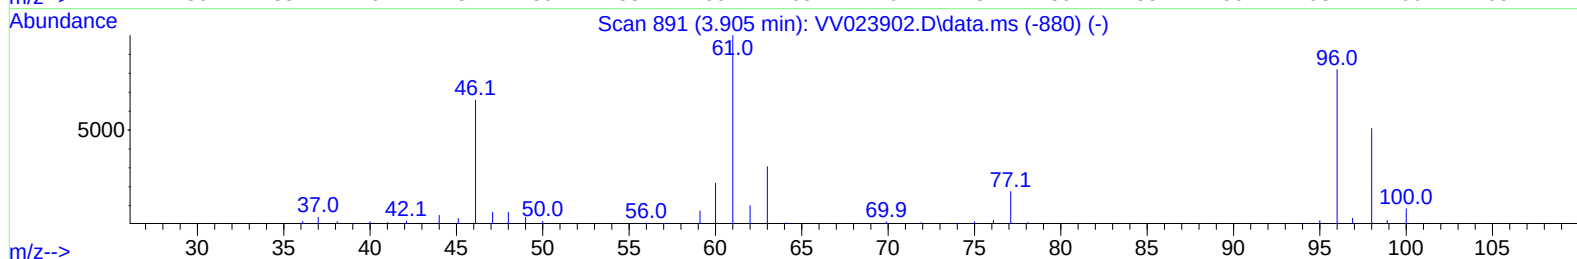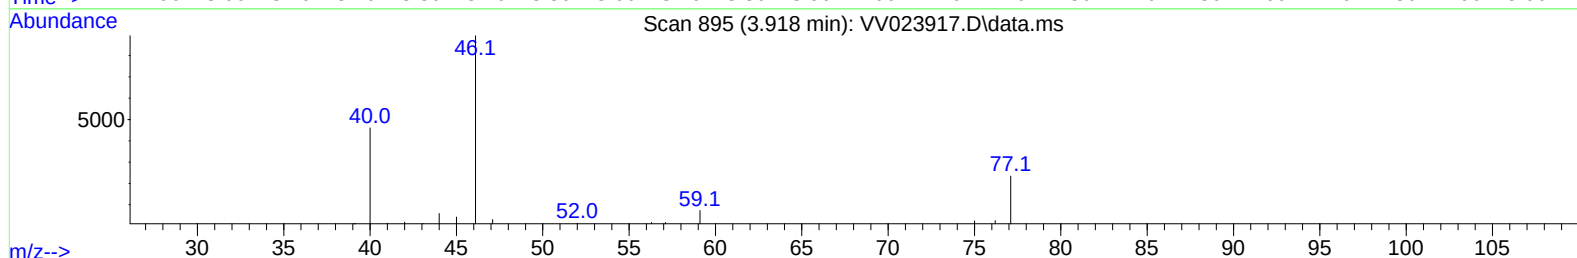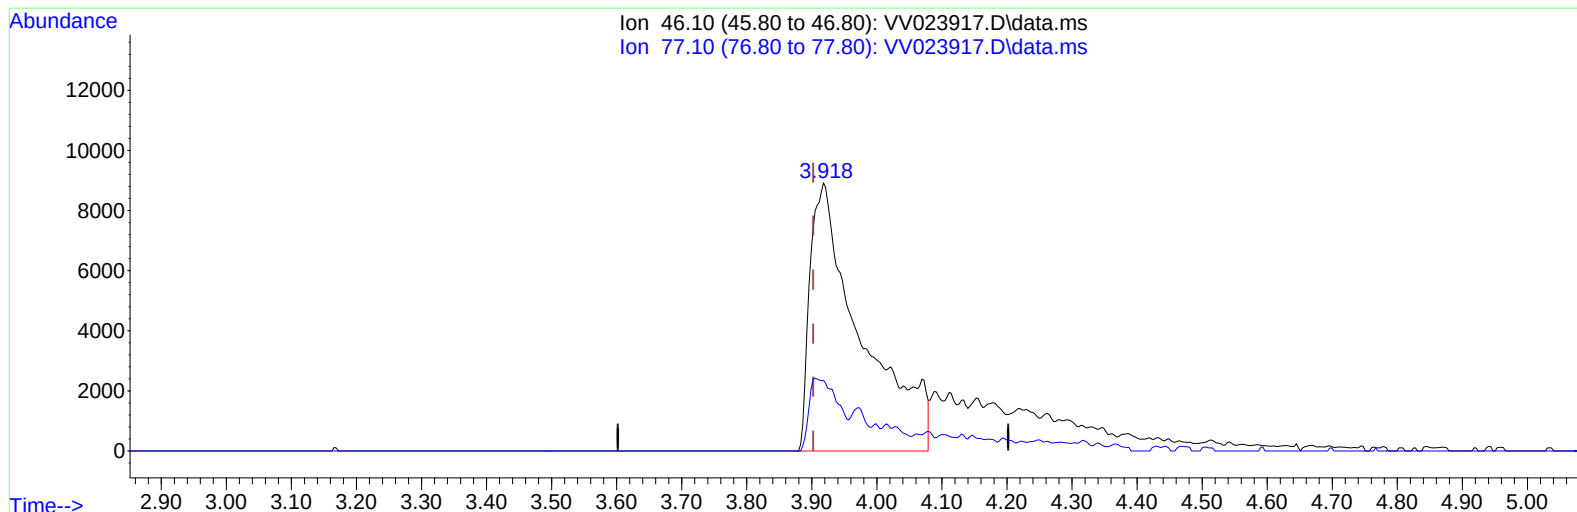

TIC: VV023917.D\data.ms

(20) 2-Butanone-d5 (S)

3.918min (+ 0.016) 44.62 ug/L m

response 48528

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.40	15.53#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023917.D
 Acq On : 11 Dec 2021 03:50
 Operator : SY/MD
 Sample : M5025-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D09

Manual IntegrationsAPPROVED

Quant Time: Dec 16 02:46:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

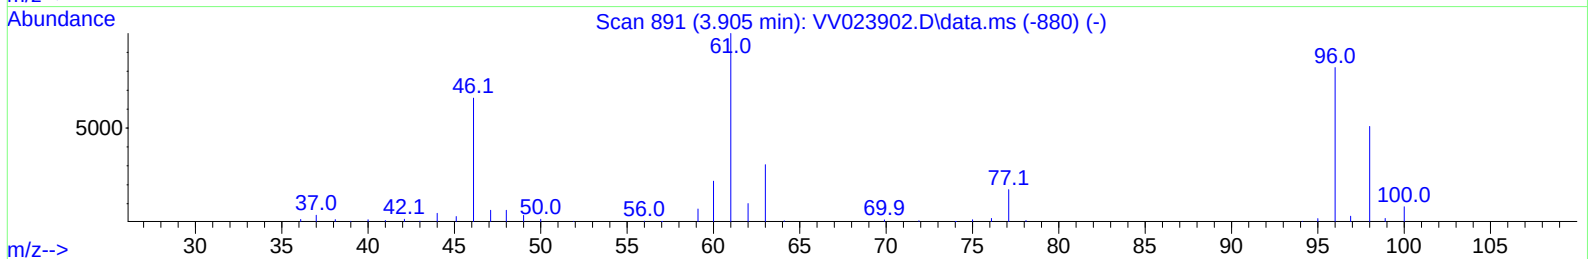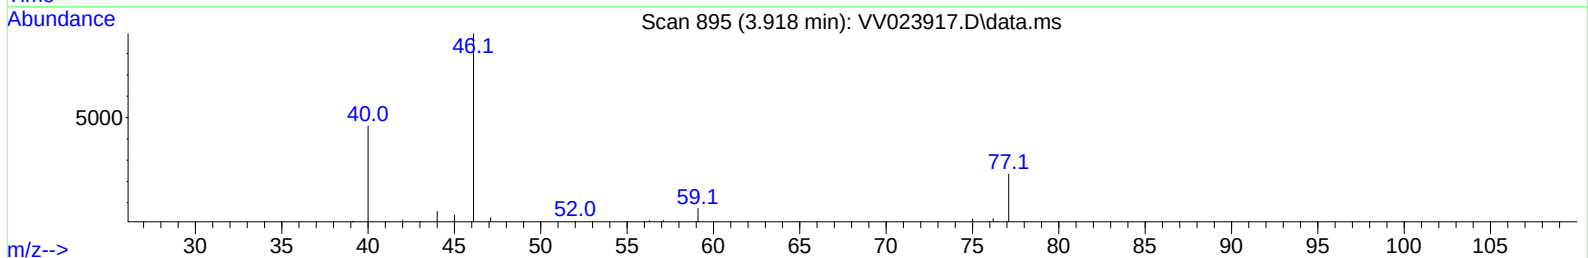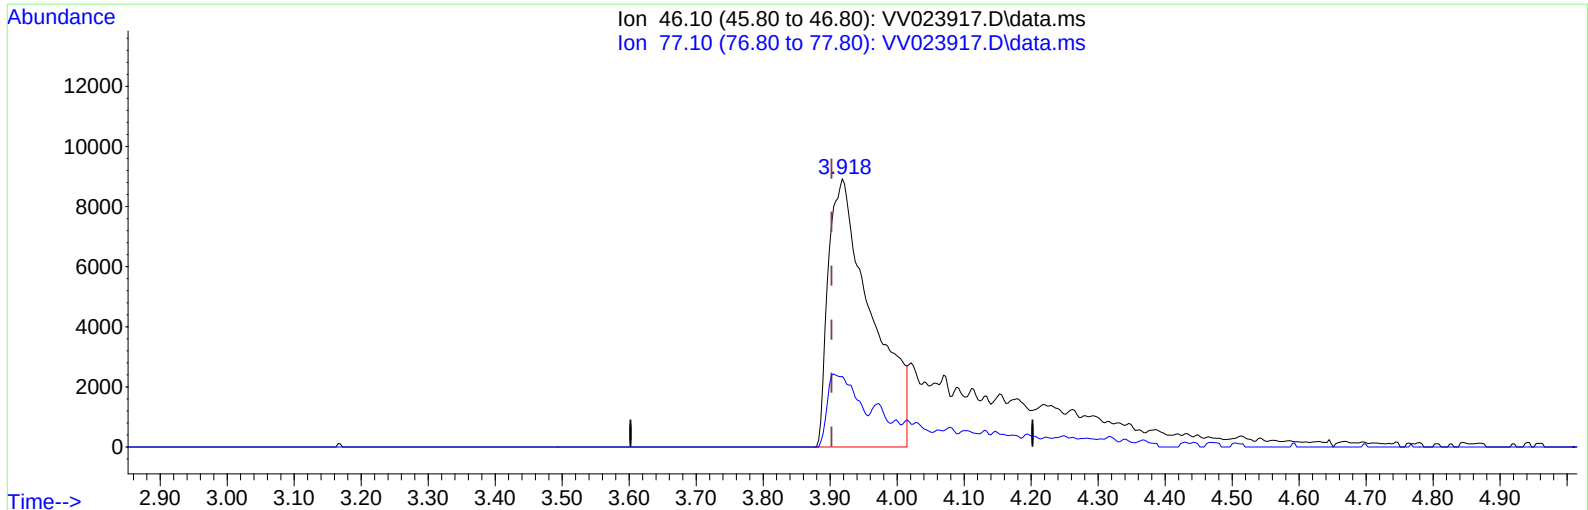

TIC: VV023917.D\data.ms

(20) 2-Butanone-d5 (S)

3.918min (+ 0.016) 36.71 ug/L

response 39928

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.40	18.87#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121021\
 Data File : VW023917.D
 Acq On : 11 Dec 2021 03:50
 Operator : SY/MD
 Sample : M5025-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D09

Manual IntegrationsAPPROVED

Quant Time: Dec 11 06:06:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	103545	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	108360	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	55030	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	23213	4.170	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	83.400%	
7) Chloroethane-d5	1.568	69	21909	4.717	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	94.400%	
11) 1,1-Dichloroethene-d2	2.108	63	32511	2.992	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	59.800%#	
20) 2-Butanone-d5	3.918	46	48528m	44.622	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	89.240%	
24) Chloroform-d	4.352	84	59308	4.704	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.000%	
26) 1,2-Dichloroethane-d4	5.034	65	28478	4.851	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.000%	
32) Benzene-d6	5.053	84	96431	4.493	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	89.800%	
36) 1,2-Dichloropropane-d6	6.069	67	32374	5.000	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	100.000%	
41) Toluene-d8	7.317	98	75895	3.928	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	78.600%	
43) trans-1,3-Dichloroprop...	7.625	79	10921	4.065	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	81.400%	
46) 2-Hexanone-d5	8.092	63	54067	44.961	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	89.920%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	25442	4.736	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	35956	4.892	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.800%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023917.D
Acq On : 11 Dec 2021 03:50
Operator : SY/MD
Sample : M5025-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D09

Manual IntegrationsAPPROVED

Quant Time: Dec 11 06:06:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 11 04:33:17 2021
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/13/2021
Supervised By :Semsettin Yesilyurt 12/13/2021

