




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023918.D
Acq On : 11 Dec 2021 04:14
Operator : SY/MD
Sample : M5005-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW207

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:06:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 11 04:33:17 2021
Response via : Initial Calibration

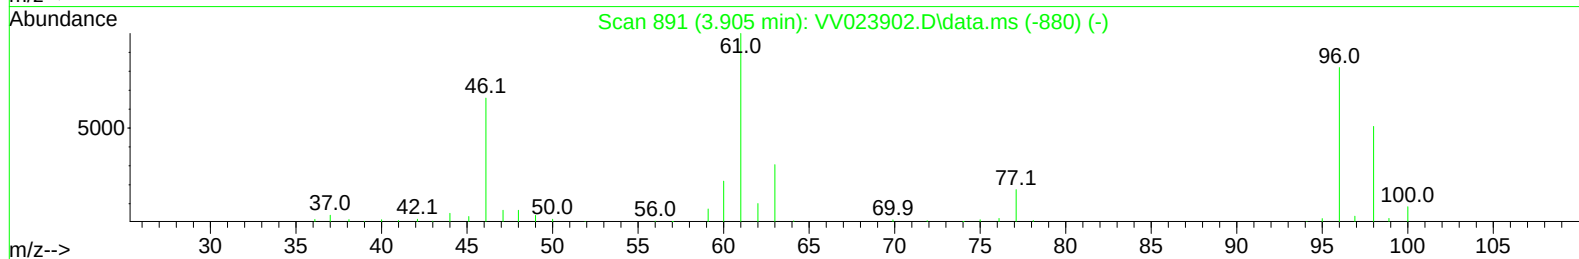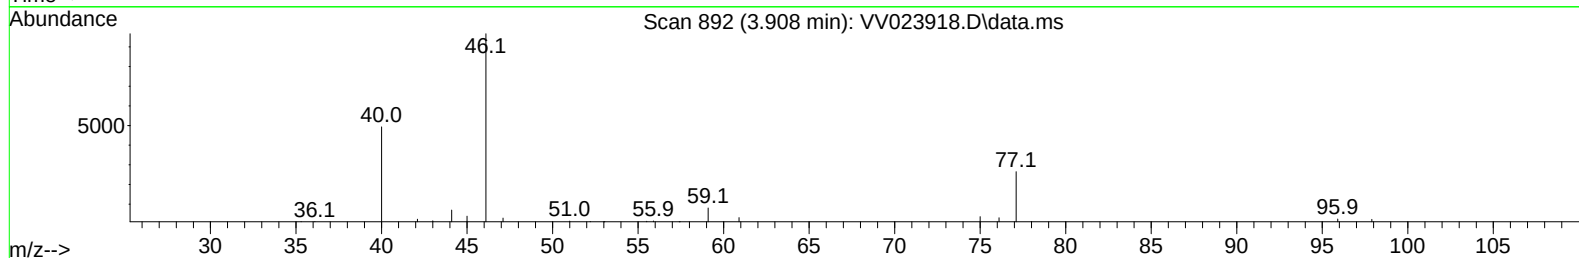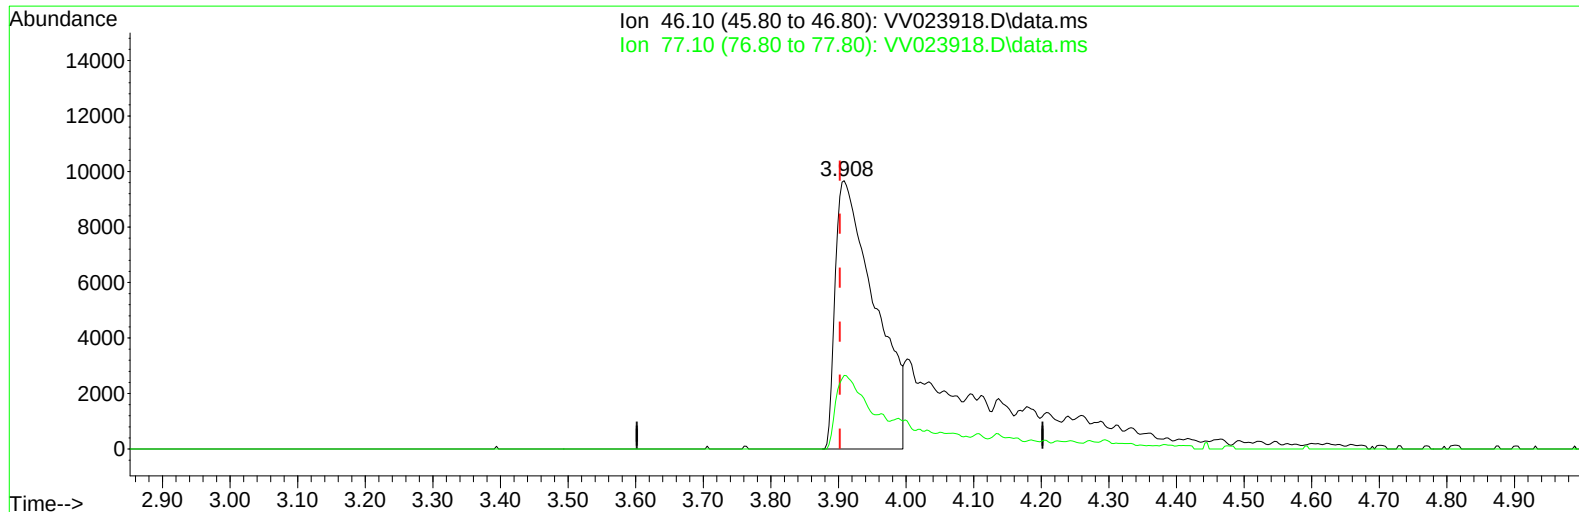

TIC: VV023918.D\data.ms

(20) 2-Butanone-d5 (S)

3.908min (+ 0.006) 36.82 ug/L

response 39406

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.40	20.28#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023918.D
Acq On : 11 Dec 2021 04:14
Operator : SY/MD
Sample : M5005-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW207

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:06:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 11 04:33:17 2021
Response via : Initial Calibration

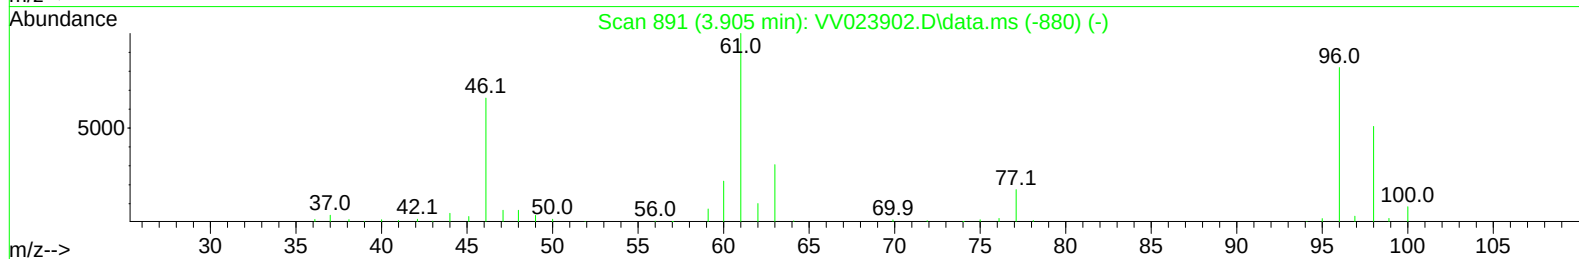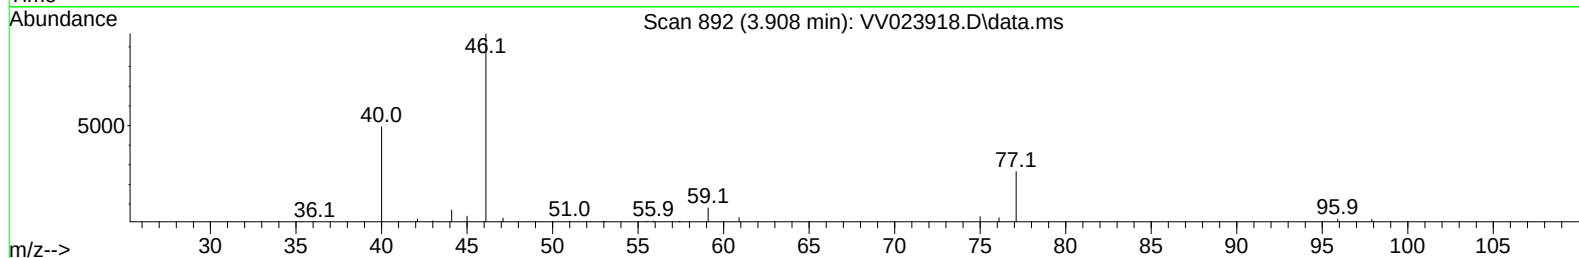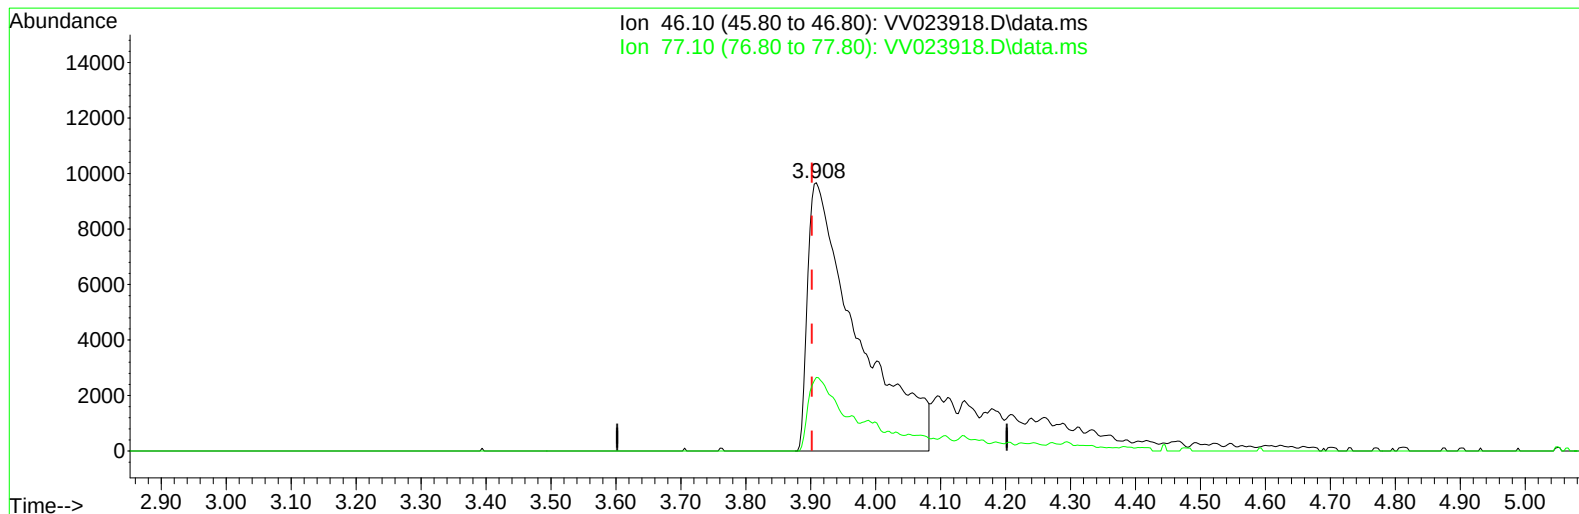

TIC: VV023918.D\data.ms

(20) 2-Butanone-d5 (S)

3.908min (+ 0.006) 48.02 ug/L m

response 51387

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.40	15.55#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121021\
 Data File : VW023918.D
 Acq On : 11 Dec 2021 04:14
 Operator : SY/MD
 Sample : M5005-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW207

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:06:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	101897	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	107211	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	51426	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	23338	4.260	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	85.200%	
7) Chloroethane-d5	1.568	69	22628	4.951	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	99.000%	
11) 1,1-Dichloroethene-d2	2.108	63	32513	3.041	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	60.800%	
20) 2-Butanone-d5	3.908	46	51387m	48.016	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	96.040%	
24) Chloroform-d	4.352	84	58465	4.712	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.200%	
26) 1,2-Dichloroethane-d4	5.034	65	28881	4.999	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.000%	
32) Benzene-d6	5.053	84	96141	4.528	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.600%	
36) 1,2-Dichloropropane-d6	6.072	67	31920	4.982	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	99.600%	
41) Toluene-d8	7.317	98	75746	3.962	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	79.200%	
43) trans-1,3-Dichloroprop...	7.625	79	10613	3.993	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	79.800%	
46) 2-Hexanone-d5	8.092	63	56070	47.126	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	94.260%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	24766	4.660	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	93.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	37934	5.522	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	110.400%	
Target Compounds						
13) Acetone	2.198	43	86865	101.453	ug/L	82
25) Chloroform	4.375	83	8034	0.532	ug/L	91
31) Carbon tetrachloride	4.822	117	2150	0.163	ug/L	87
34) Trichloroethene	5.928	95	831	0.097	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023918.D
Acq On : 11 Dec 2021 04:14
Operator : SY/MD
Sample : M5005-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW207

Manual IntegrationsAPPROVED

Quant Time: Dec 11 06:06:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 11 04:33:17 2021
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/13/2021
Supervised By :Semsettin Yesilyurt 12/13/2021

