




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023922.D
 Acq On : 11 Dec 2021 05:49
 Operator : SY/MD
 Sample : M5005-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW211

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:51:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

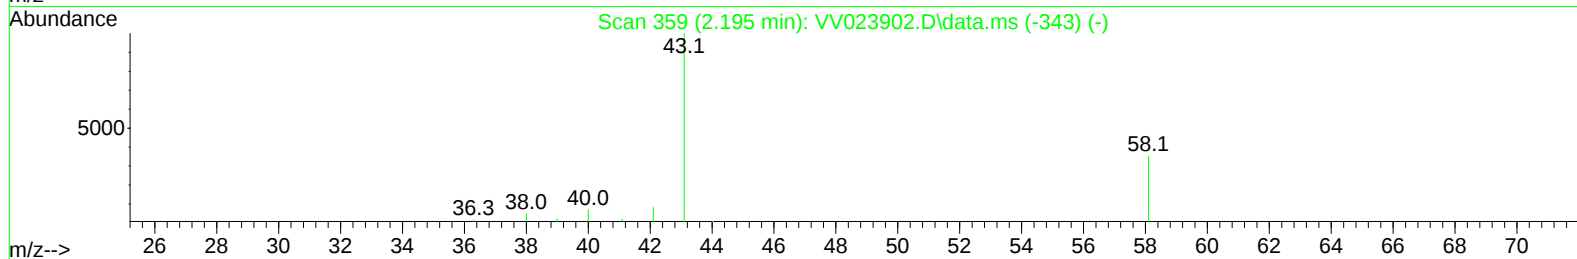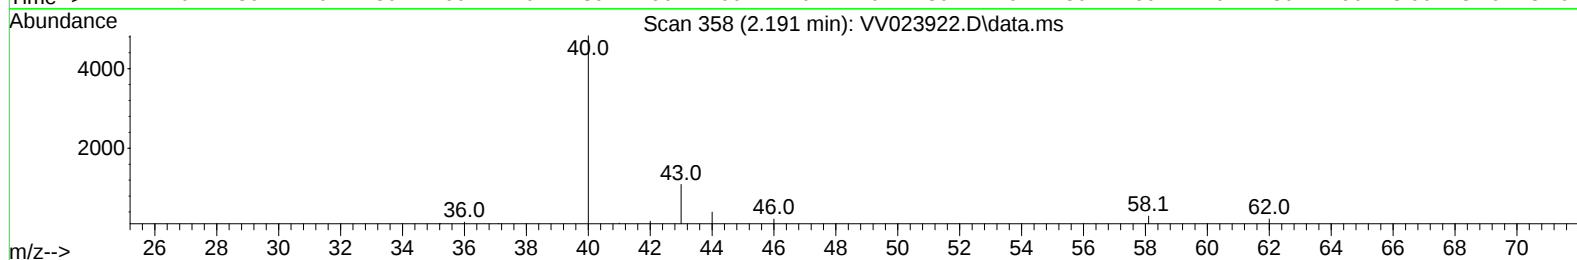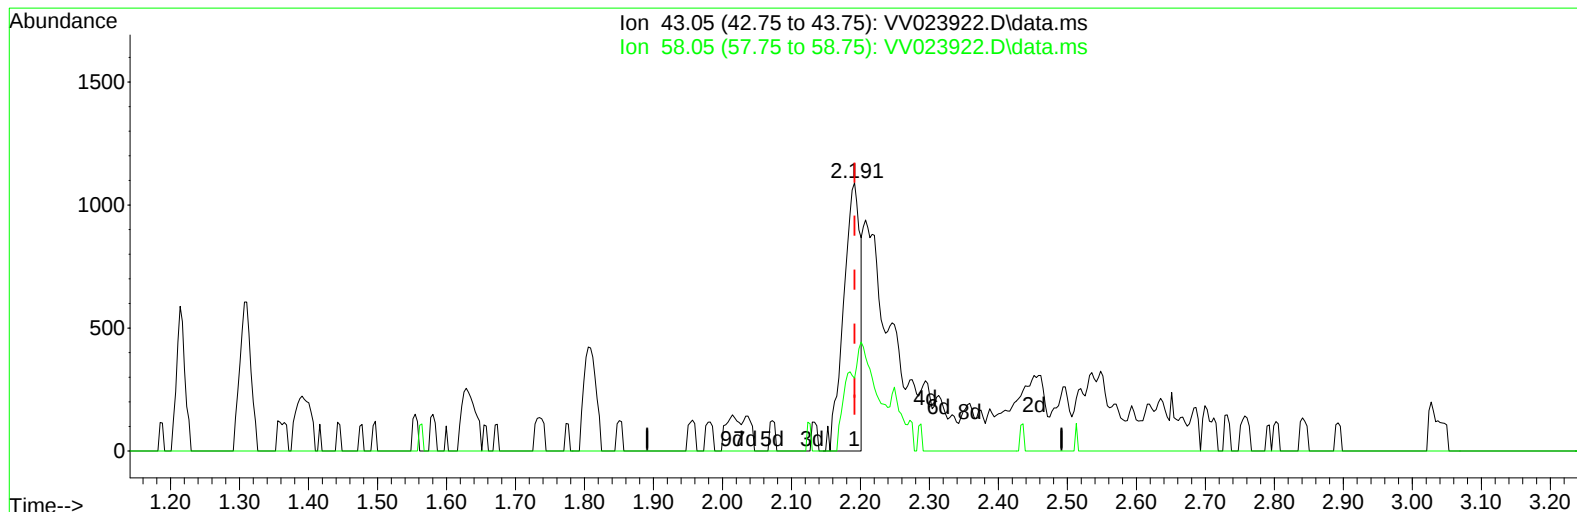

TIC: VV023922.D\data.ms

(13) Acetone (T)

2.191min (0.000) 1.96 ug/L

response 1829

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	21.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023922.D
 Acq On : 11 Dec 2021 05:49
 Operator : SY/MD
 Sample : M5005-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW211

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:51:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

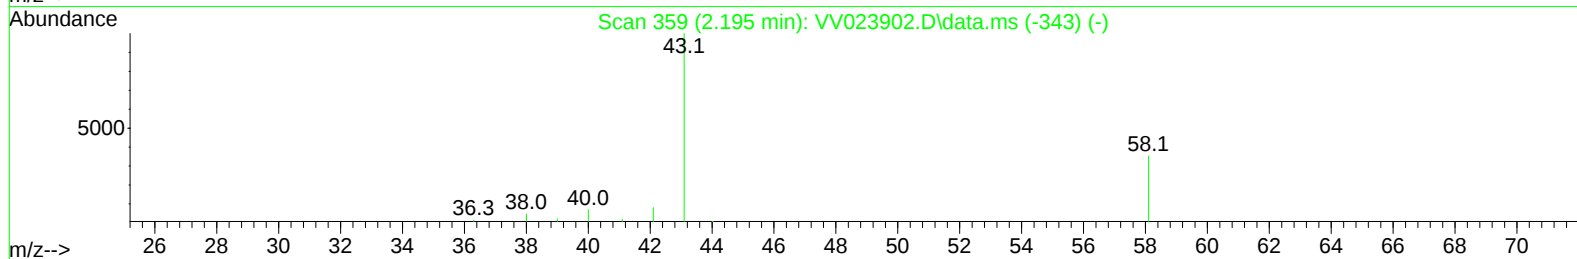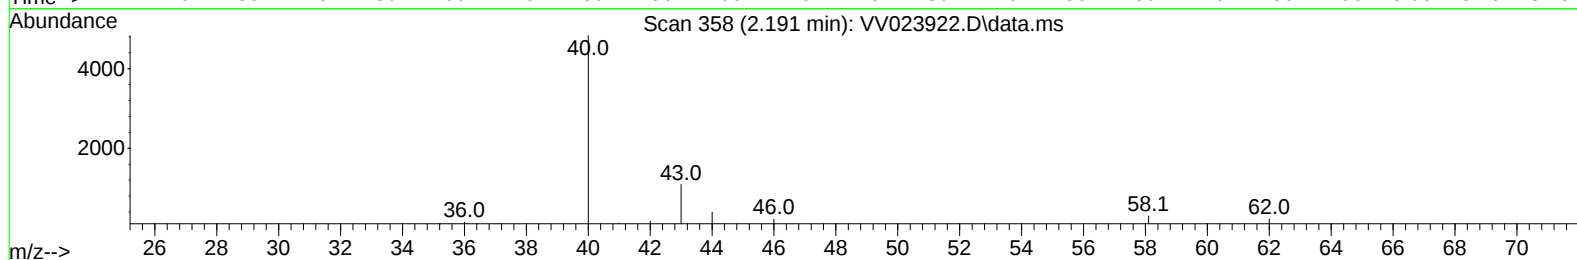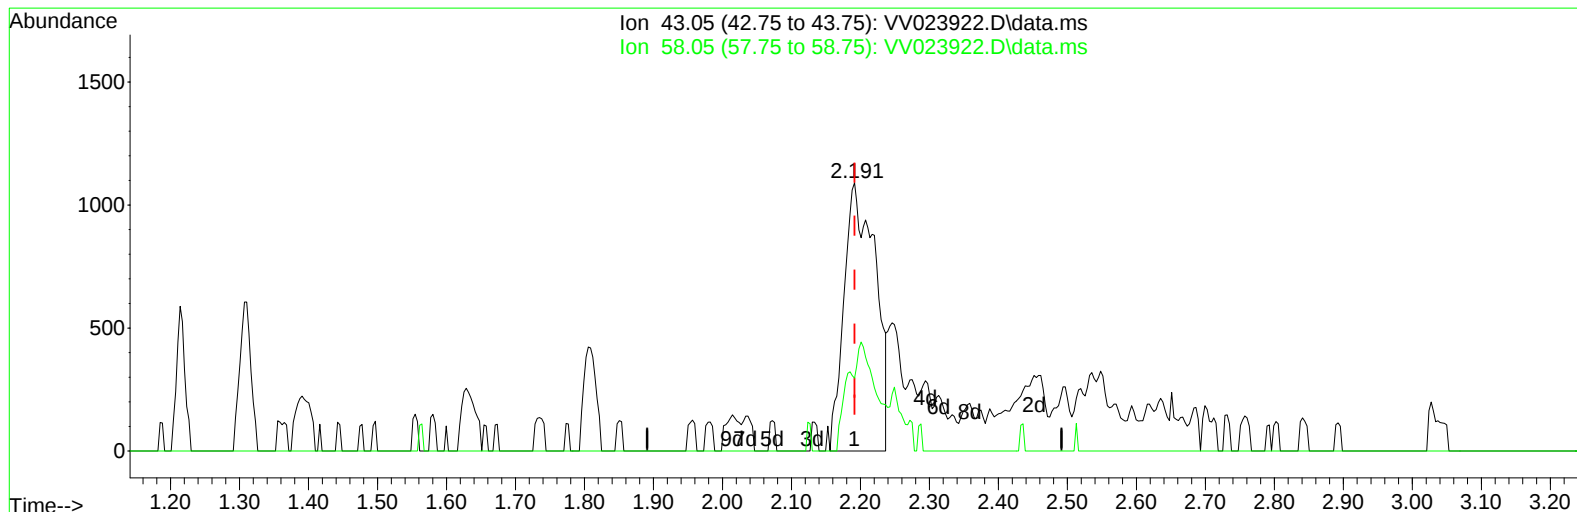

TIC: VV023922.D\data.ms

(13) Acetone (T)

2.191min (0.000) 3.65 ug/L m

response 3408

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	11.27
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023922.D
 Acq On : 11 Dec 2021 05:49
 Operator : SY/MD
 Sample : M5005-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW211

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:51:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

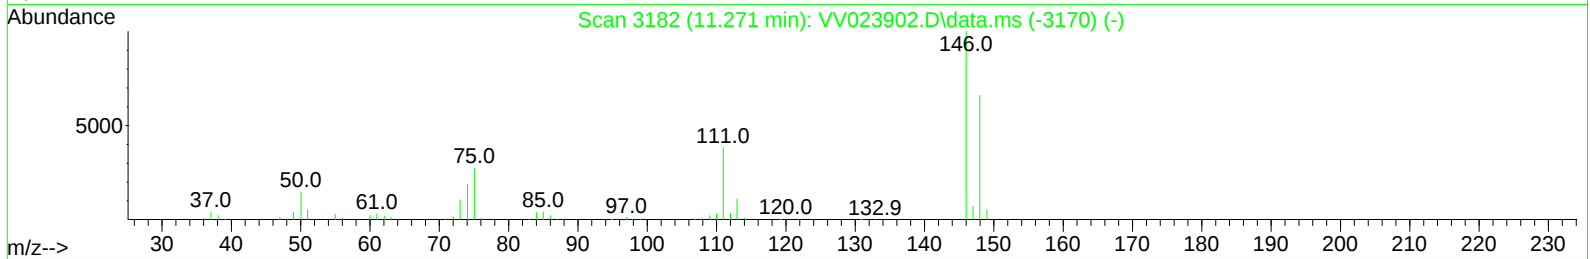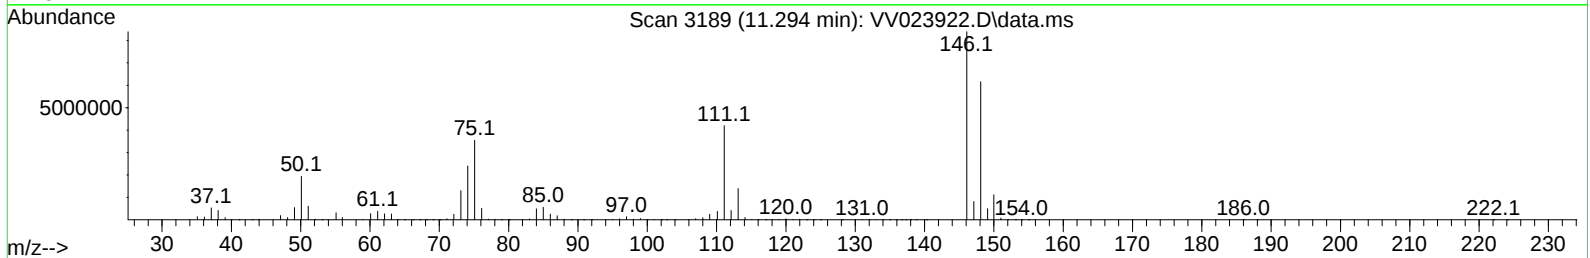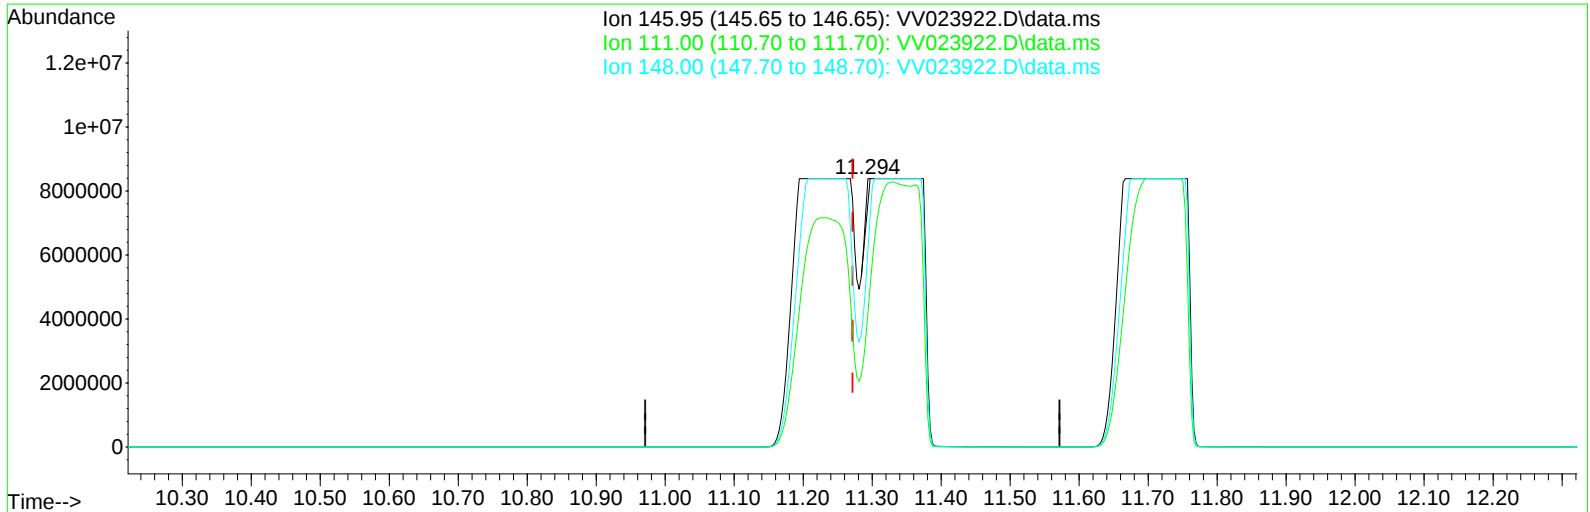

TIC: VV023922.D\data.ms

(65) 1,4-Dichlorobenzene (T)

11.294min (+ 0.023) 24.91 ug/L

response 644676

Ion	Exp%	Act%
145.95	100.00	100.00
111.00	36.60	50.03#
148.00	64.00	73.42
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023922.D
 Acq On : 11 Dec 2021 05:49
 Operator : SY/MD
 Sample : M5005-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW211

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:51:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

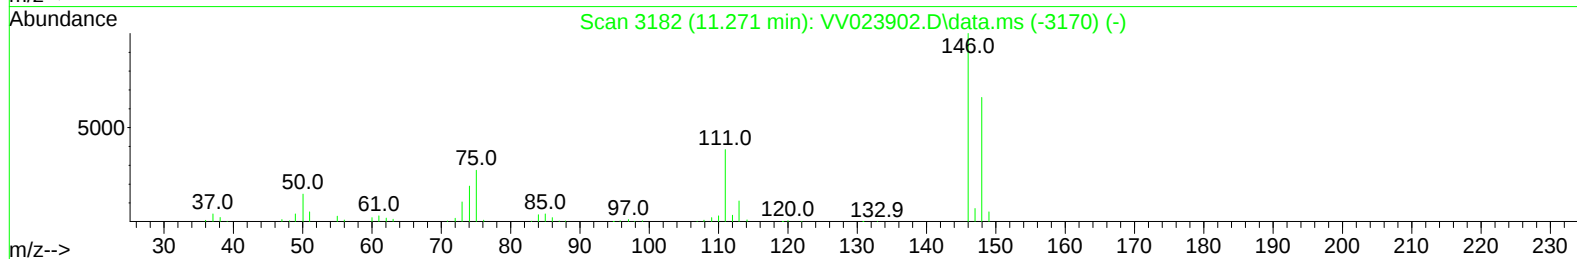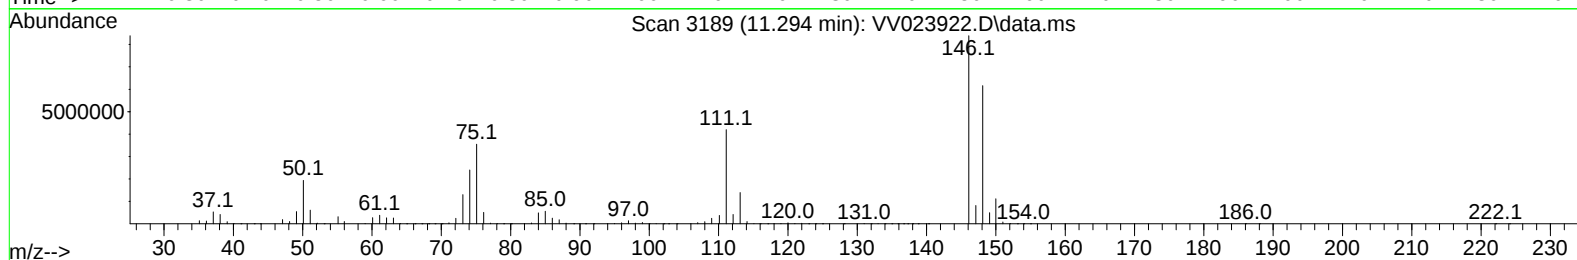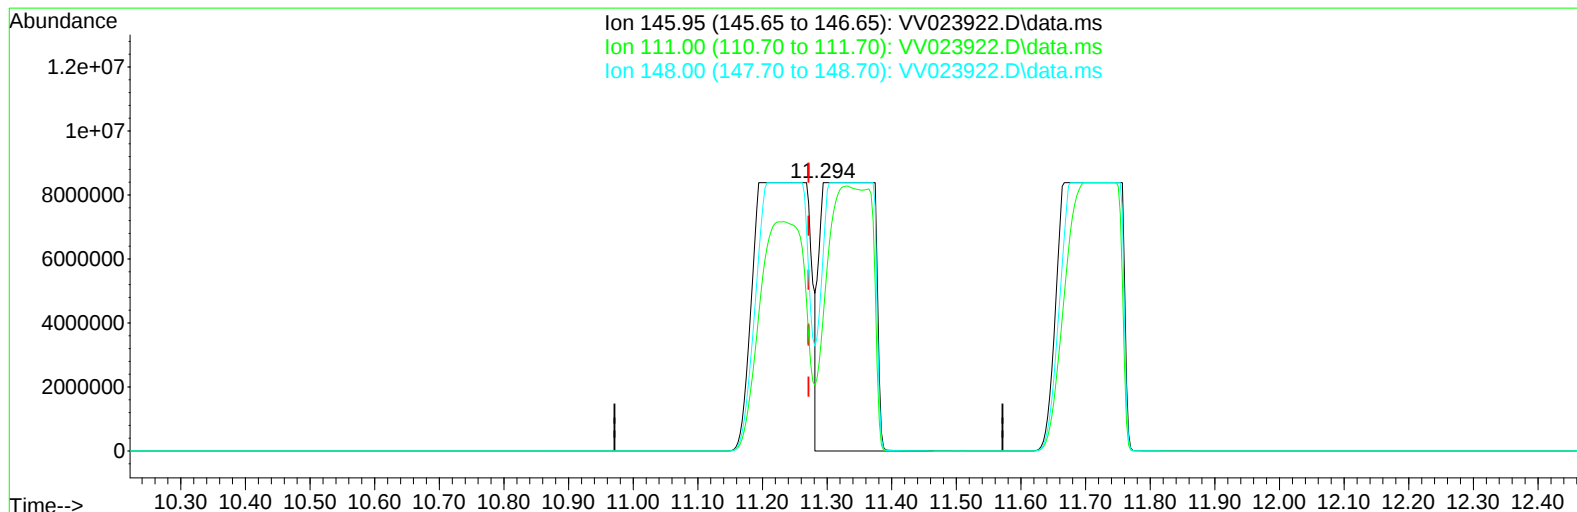

TIC: VV023922.D\data.ms

(65) 1,4-Dichlorobenzene (T)

11.294min (+ 0.023) 1833.04 ug/L m

response 47446513

Ion	Exp%	Act%
145.95	100.00	100.00
111.00	36.60	50.03#
148.00	64.00	73.42
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023922.D
Acq On : 11 Dec 2021 05:49
Operator : SY/MD
Sample : M5005-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW211

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:51:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 11 04:33:17 2021
Response via : Initial Calibration

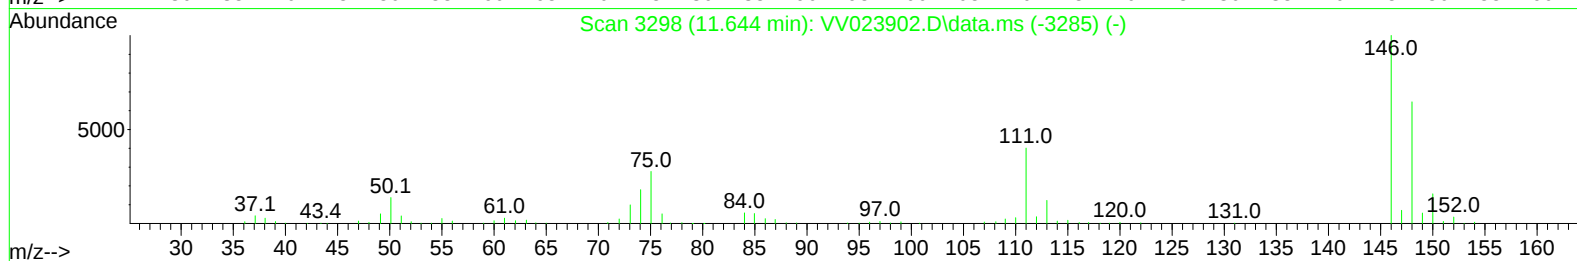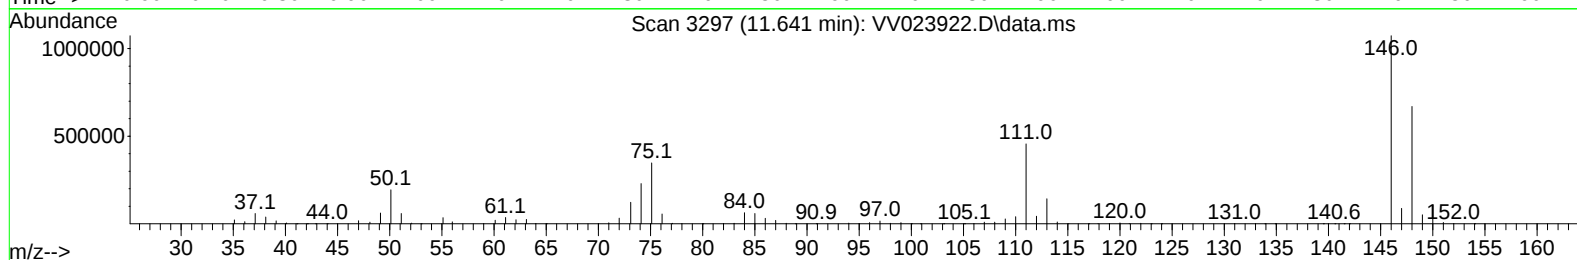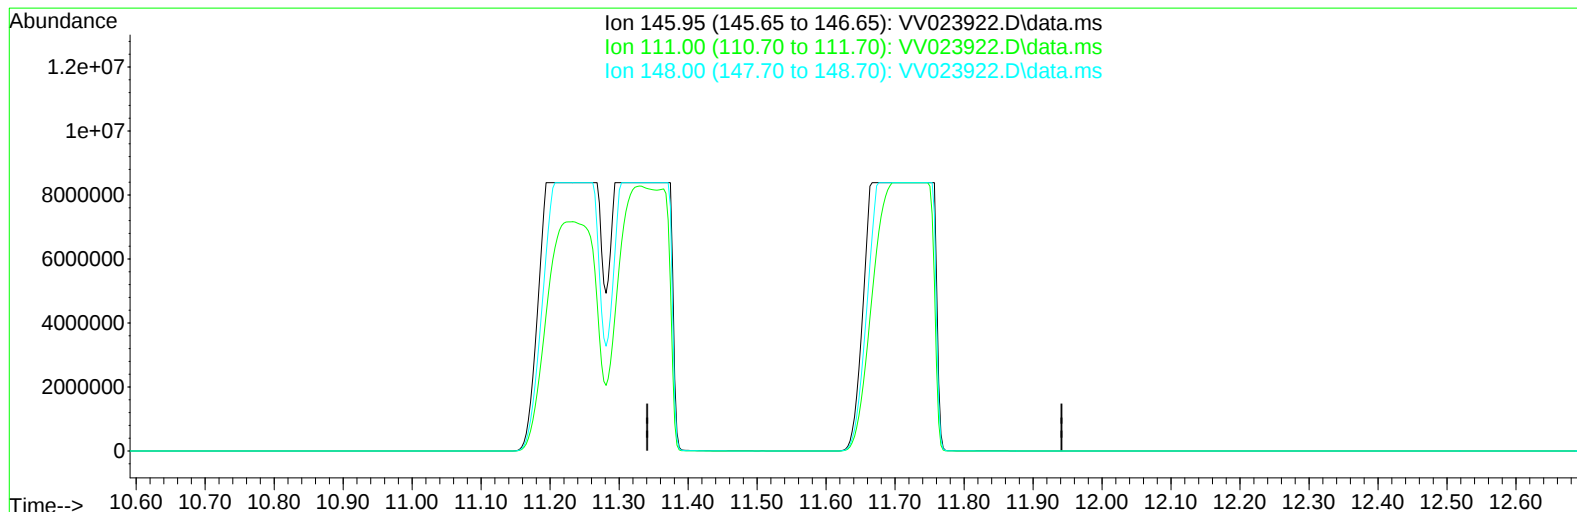

TIC: VV023922.D\data.ms

(67) 1,2-Dichlorobenzene (T)

11.641min (-11.641) 0.00 ug/L

response 0

Ion	Exp%	Act%
145.95	100.00	0.00
111.00	39.90	0.00#
148.00	63.10	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023922.D
Acq On : 11 Dec 2021 05:49
Operator : SY/MD
Sample : M5005-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW211

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:51:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 11 04:33:17 2021
Response via : Initial Calibration

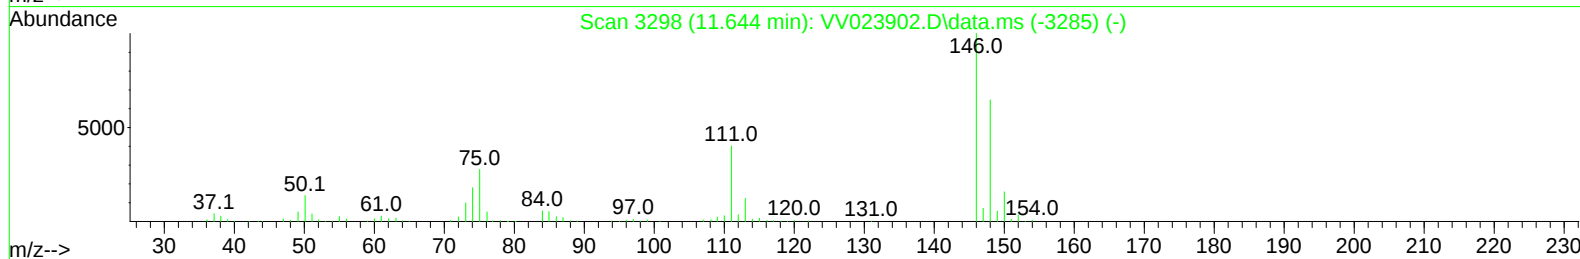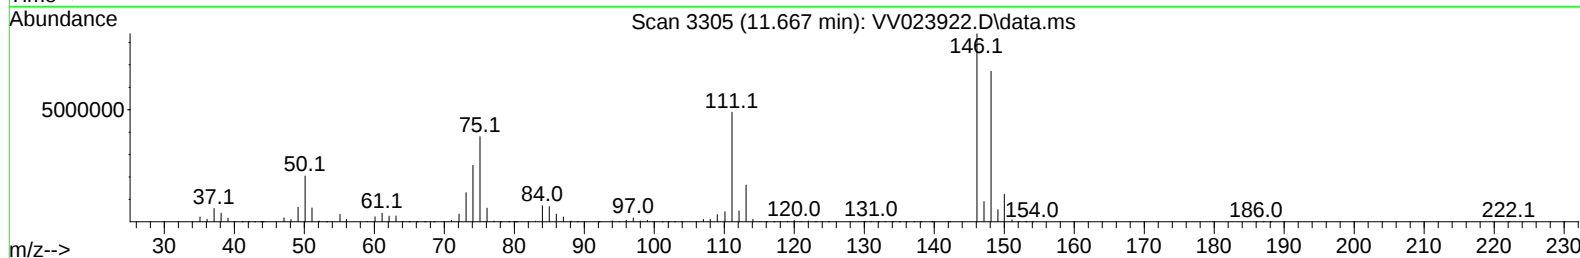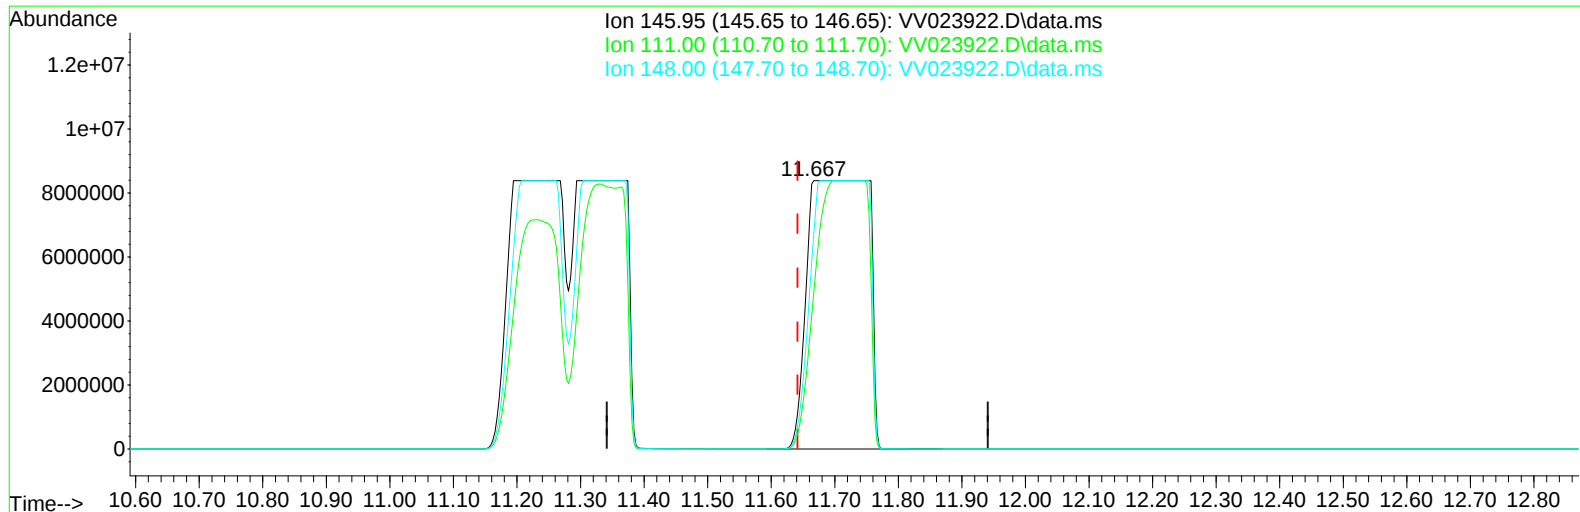

TIC: VV023922.D\data.ms

(67) 1,2-Dichlorobenzene (T)

11.667min (+ 0.026) 2350.96 ug/L m

response 55508450

Ion	Exp%	Act%
145.95	100.00	100.00
111.00	39.90	58.21#
148.00	63.10	80.08#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023922.D
 Acq On : 11 Dec 2021 05:49
 Operator : SY/MD
 Sample : M5005-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW211

Manual IntegrationsAPPROVED

Quant Time: Dec 11 06:51:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

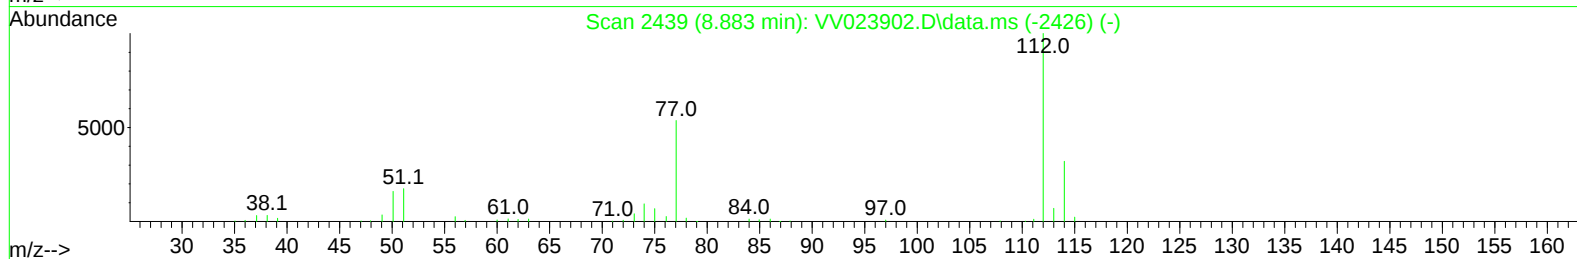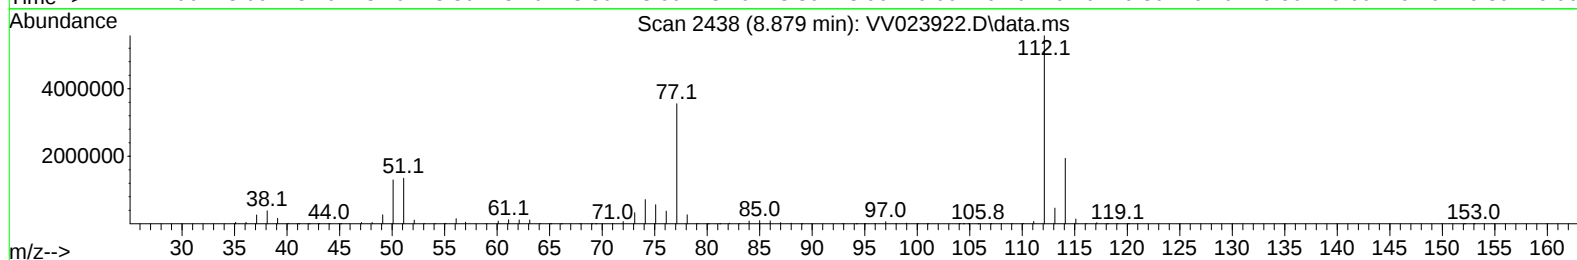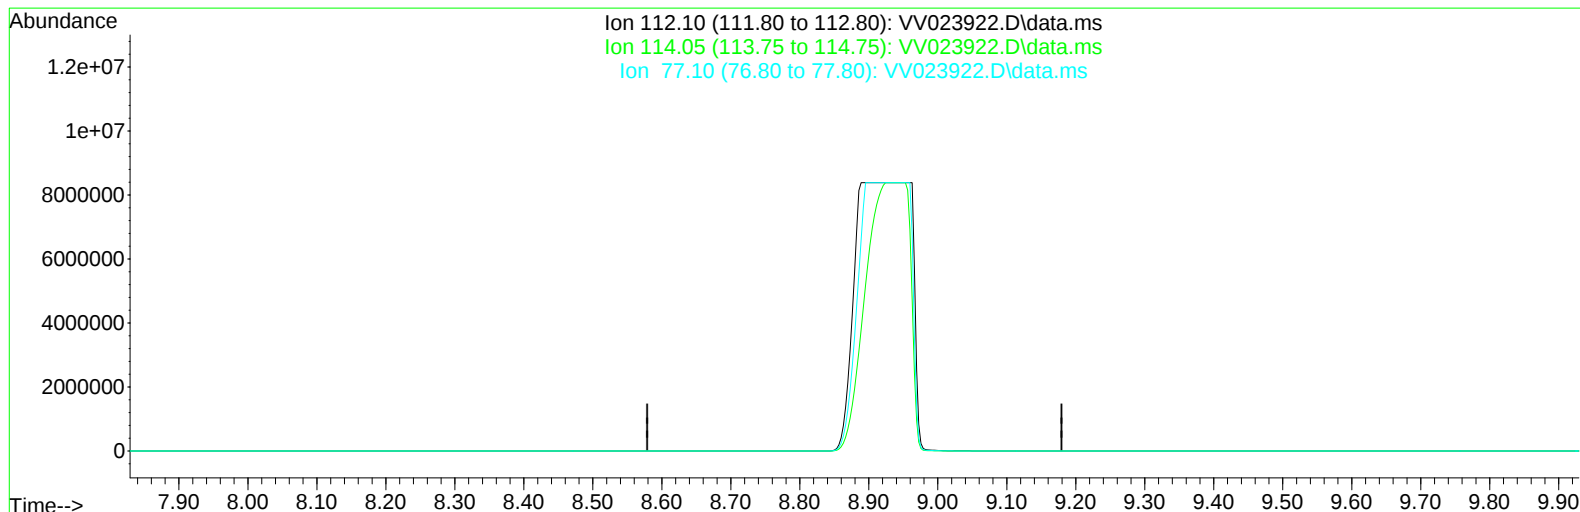

TIC: VV023922.D\data.ms

(51) Chlorobenzene (T)

8.879min (-8.879) 0.00 ug/L

response 0

Ion	Exp%	Act%
112.10	100.00	0.00
114.05	33.30	0.00#
77.10	54.10	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023922.D
 Acq On : 11 Dec 2021 05:49
 Operator : SY/MD
 Sample : M5005-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW211

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:51:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

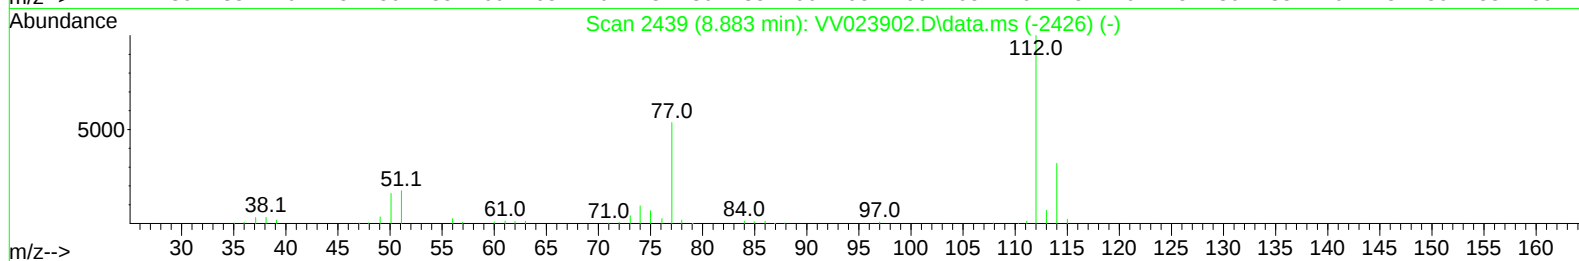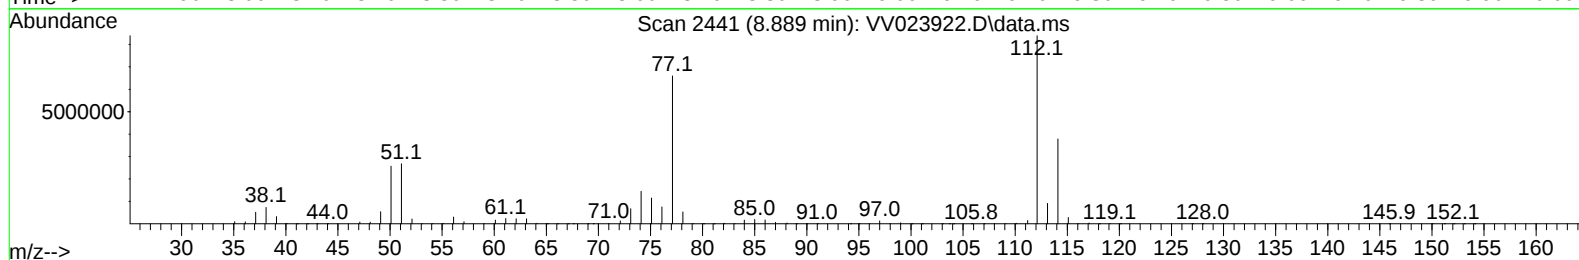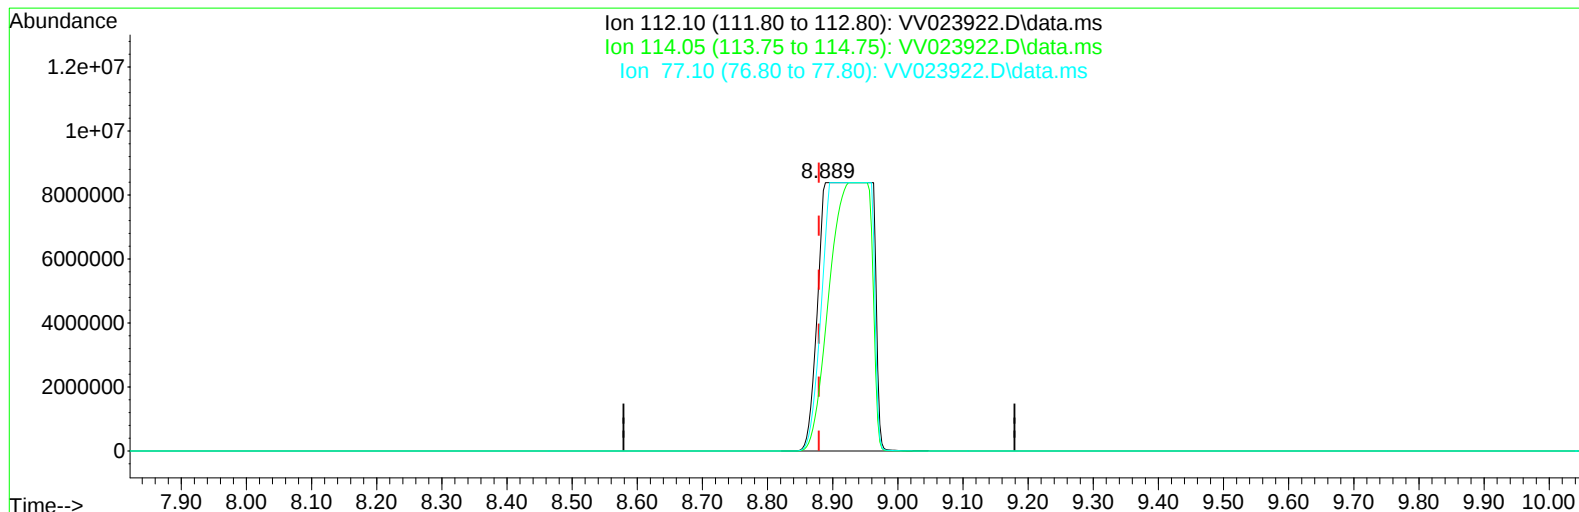

TIC: VV023922.D\data.ms

(51) Chlorobenzene (T)

8.889min (+ 0.010) 1668.06 ug/L m

response 47091834

Ion	Exp%	Act%
112.10	100.00	100.00
114.05	33.30	45.14#
77.10	54.10	78.64#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023922.D
 Acq On : 11 Dec 2021 05:49
 Operator : SY/MD
 Sample : M5005-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW211

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:51:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

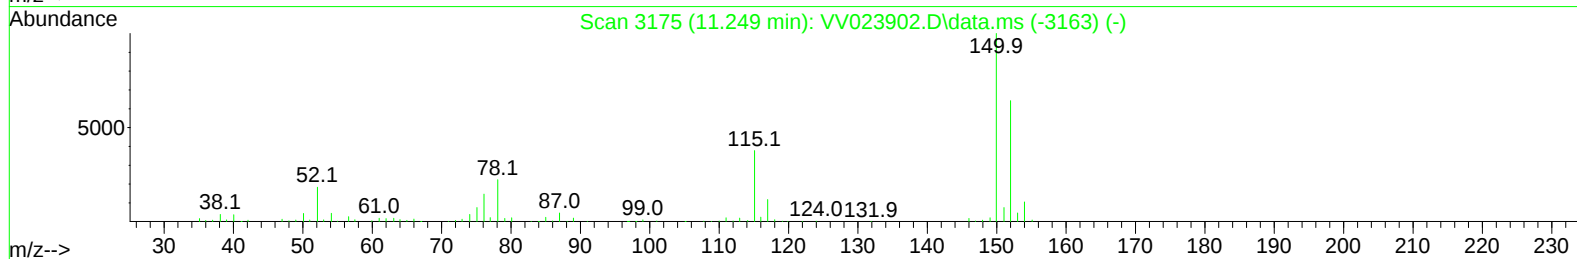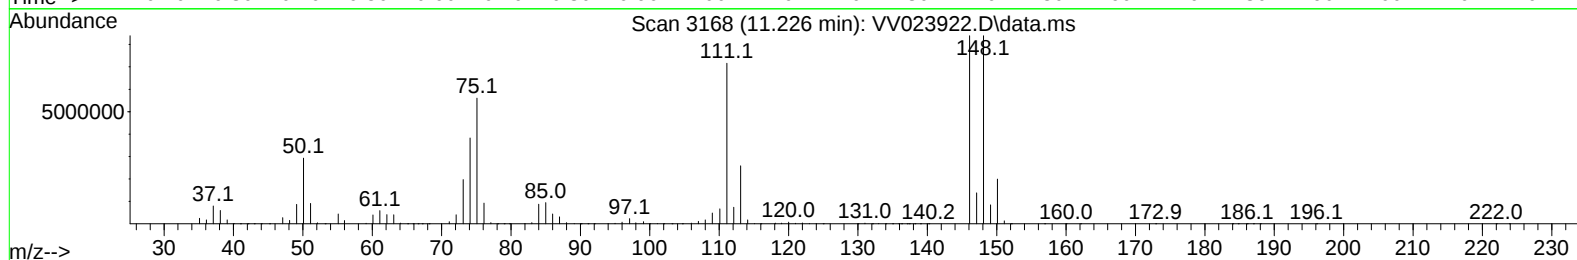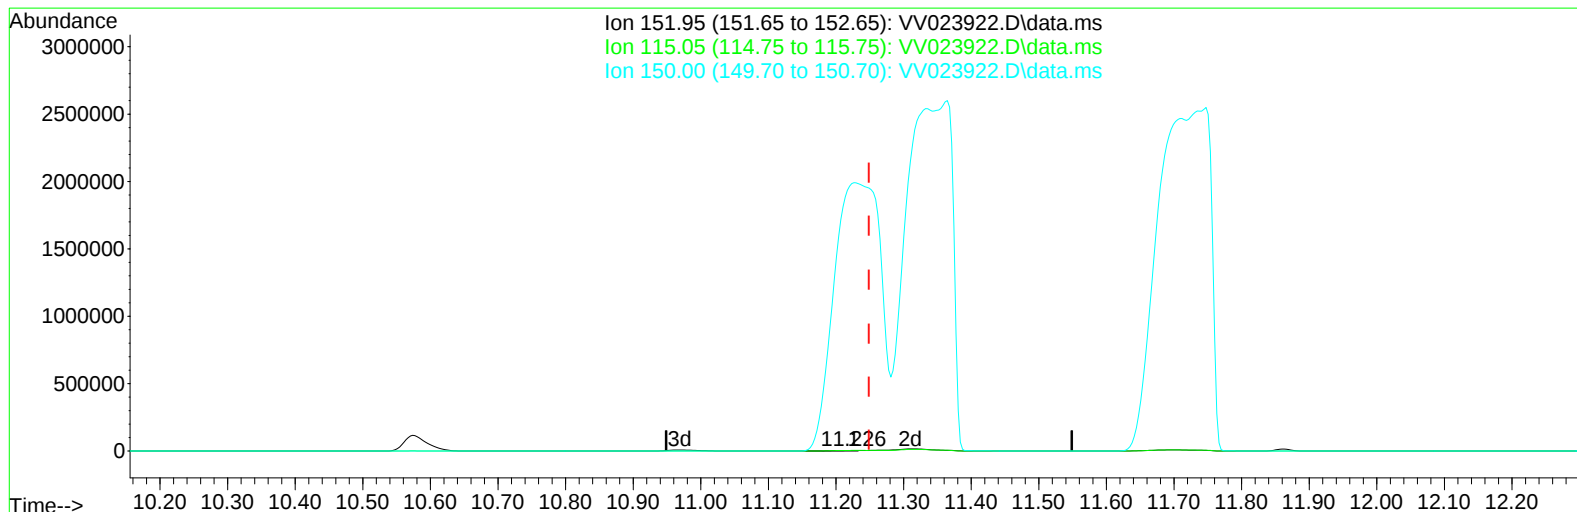

TIC: VV023922.D\data.ms

(58) 1,4-Dichlorobenzene-d4 (I)

11.226min (-0.022) 5.00 ug/L

response 9629

Ion	Exp%	Act%
151.95	100.00	100.00
115.05	56.70	171.32#
150.00	175.80	98970.64#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023922.D
Acq On : 11 Dec 2021 05:49
Operator : SY/MD
Sample : M5005-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW211

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:51:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 11 04:33:17 2021
Response via : Initial Calibration

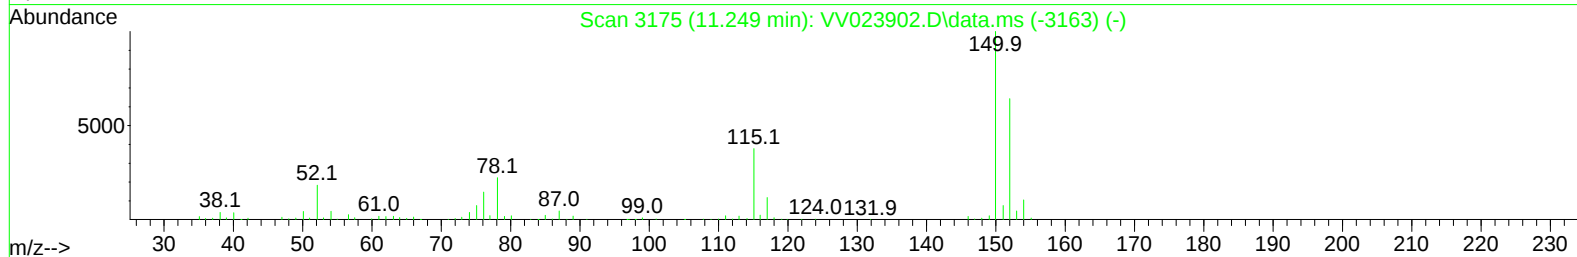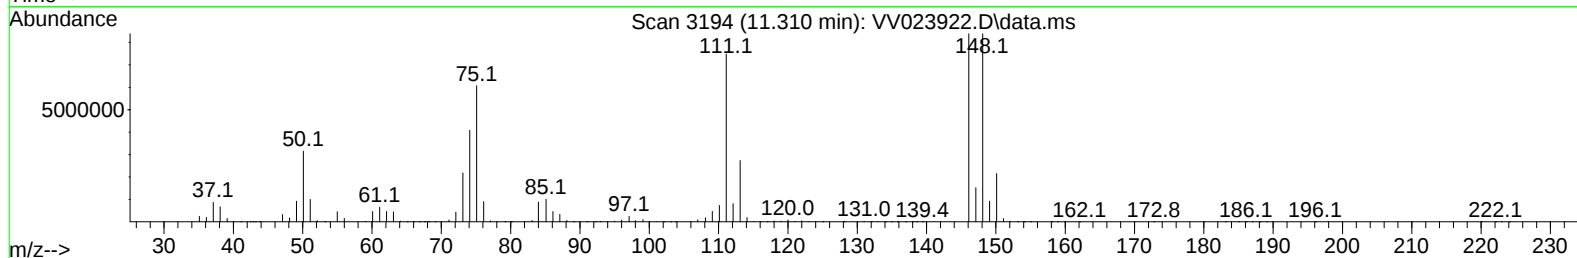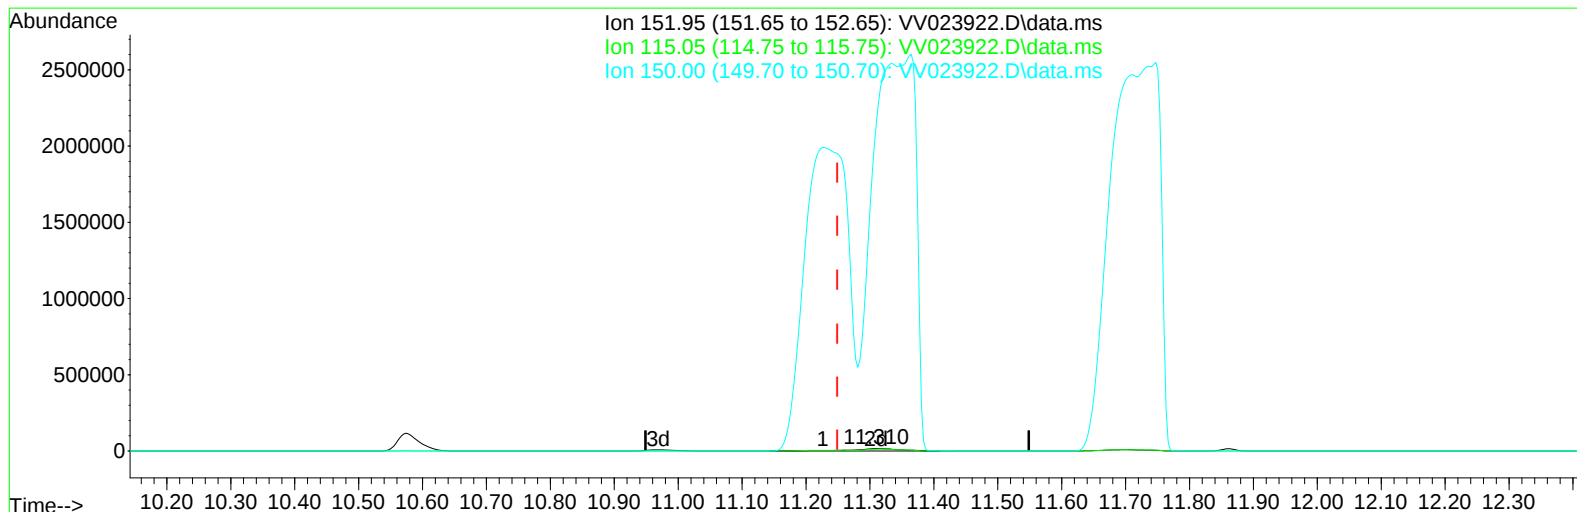

TIC: VV023922.D\data.ms

(58) 1,4-Dichlorobenzene-d4 (I)

11.310min (+ 0.061) 5.00 ug/L m

response 85825

Ion	Exp%	Act%
151.95	100.00	100.00
115.05	56.70	19.22
150.00	175.80	11103.85#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023922.D
 Acq On : 11 Dec 2021 05:49
 Operator : SY/MD
 Sample : M5005-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW211

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:51:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

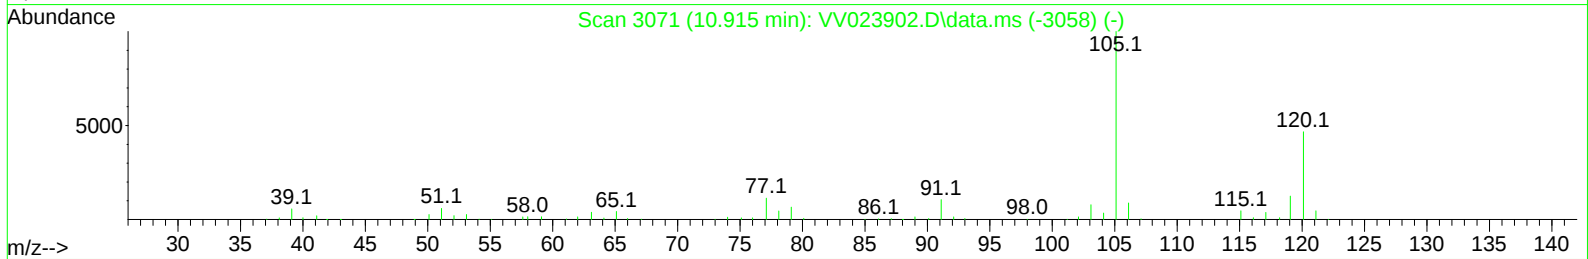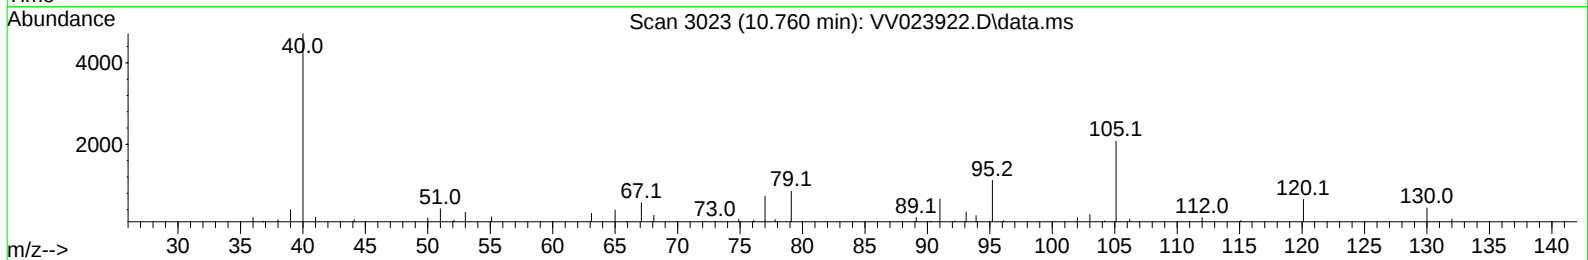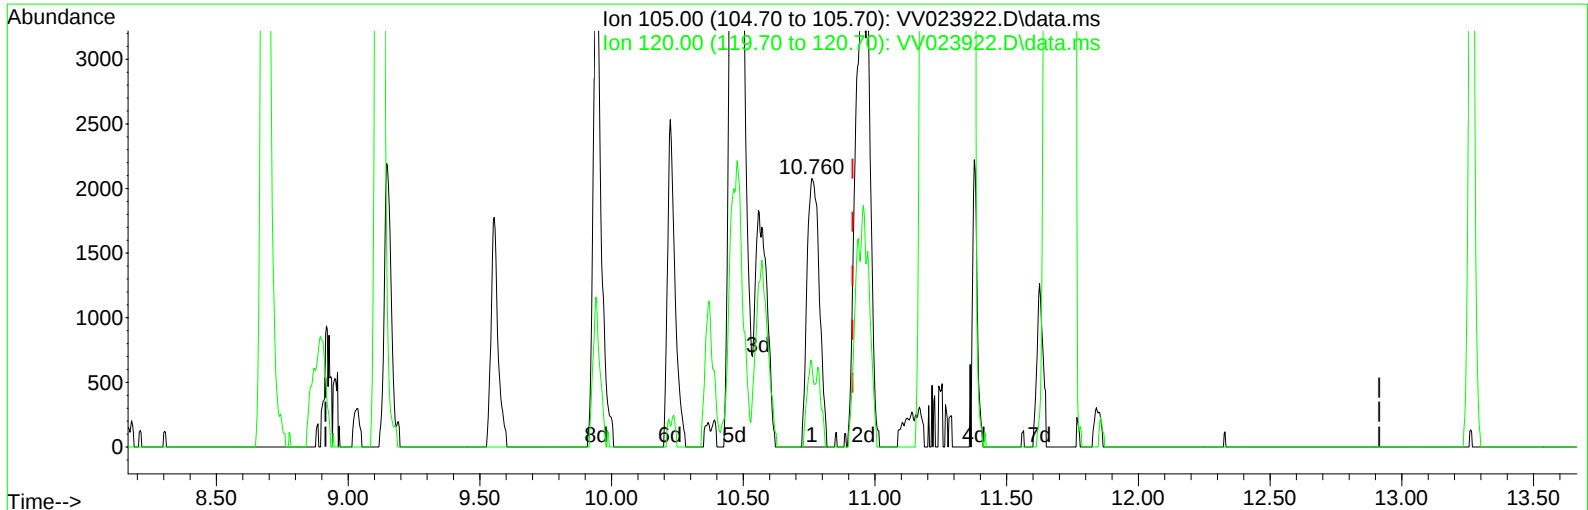

TIC: VV023922.D\data.ms

(63) 1,2,4-Trimethylbenzene (T)

10.760min (-0.154) 0.16 ug/L

response 6804

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	45.90	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023922.D
 Acq On : 11 Dec 2021 05:49
 Operator : SY/MD
 Sample : M5005-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW211

Manual IntegrationsAPPROVED

Quant Time: Dec 11 06:51:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

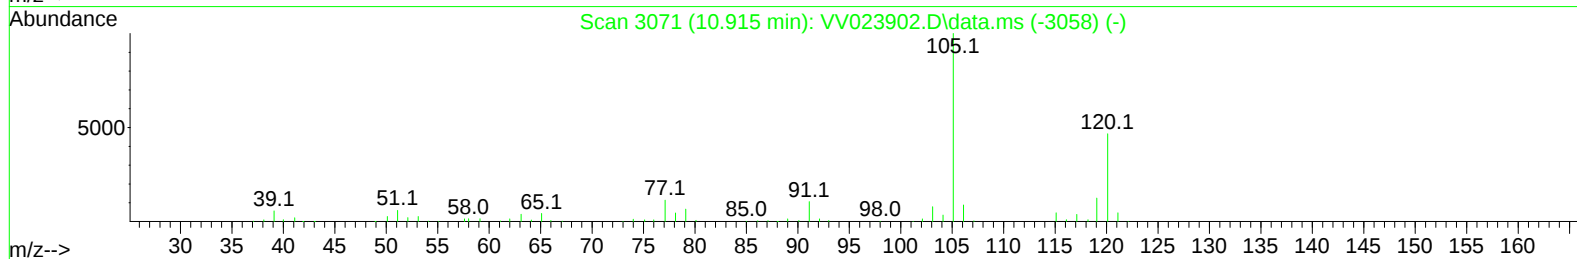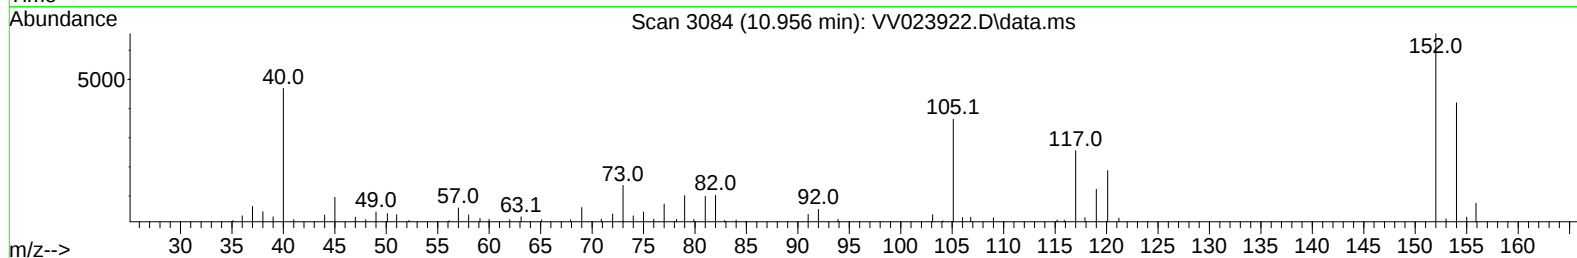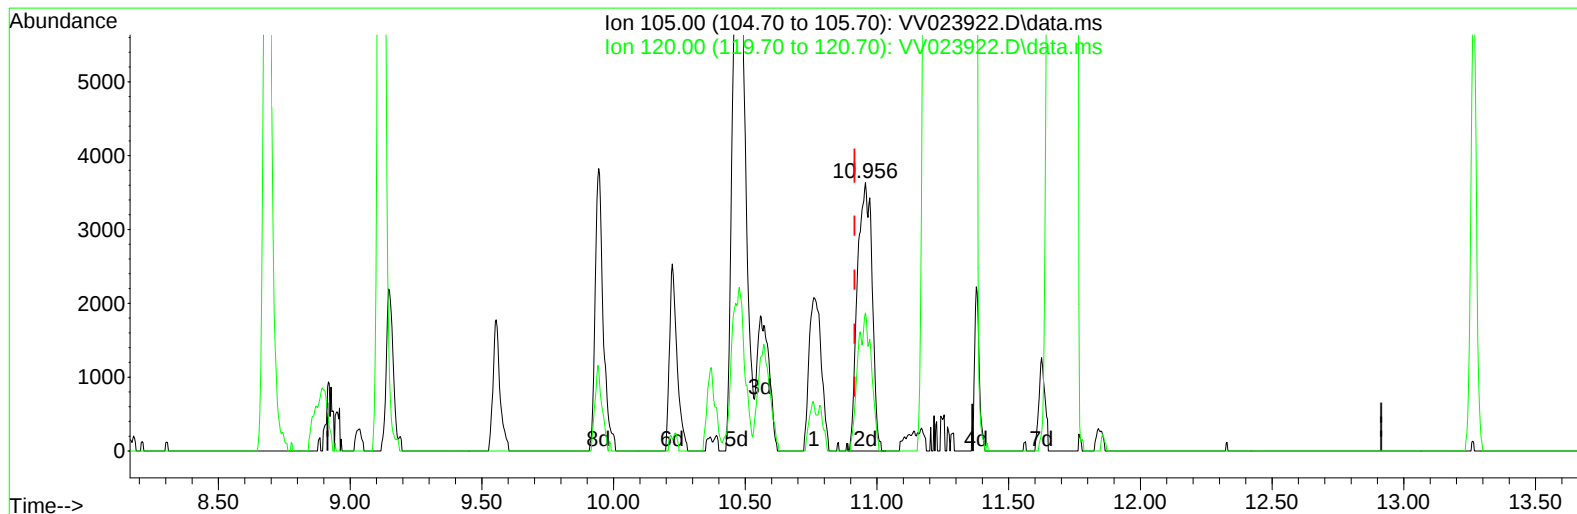

TIC: VV023922.D\data.ms

(63) 1,2,4-Trimethylbenzene (T)

10.956min (+ 0.042) 0.33 ug/L m

response 13943

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	45.90	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023922.D
 Acq On : 11 Dec 2021 05:49
 Operator : SY/MD
 Sample : M5005-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW211

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:51:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

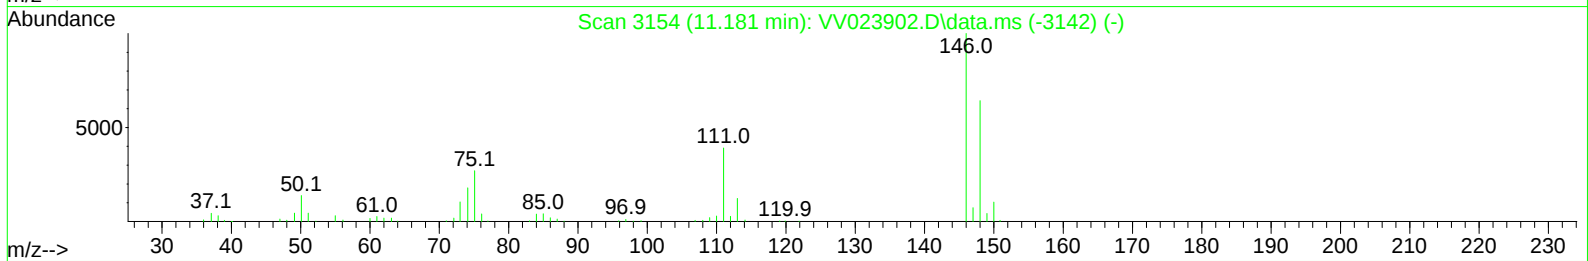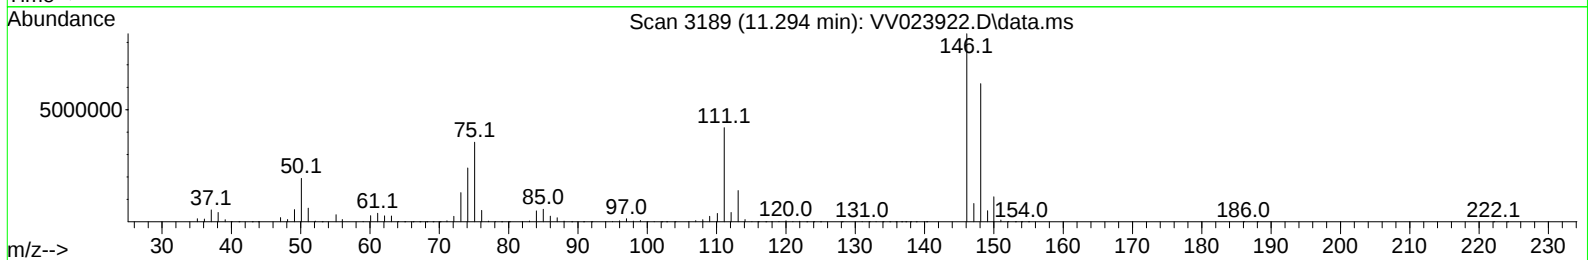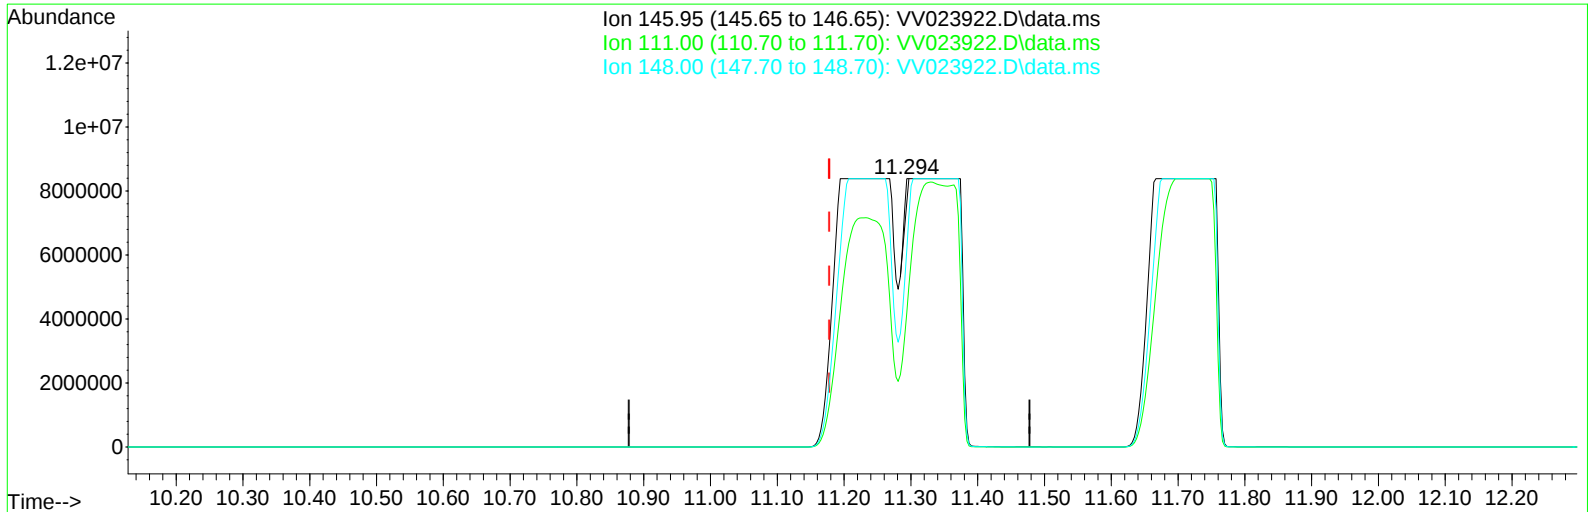

TIC: VV023922.D\data.ms

(64) 1,3-Dichlorobenzene (T)

11.294min (+ 0.116) 25.02 ug/L

response 644676

Ion	Exp%	Act%
145.95	100.00	100.00
111.00	37.60	50.03#
148.00	63.50	73.42
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023922.D
 Acq On : 11 Dec 2021 05:49
 Operator : SY/MD
 Sample : M5005-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW211

Manual IntegrationsAPPROVED

Quant Time: Dec 11 06:51:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

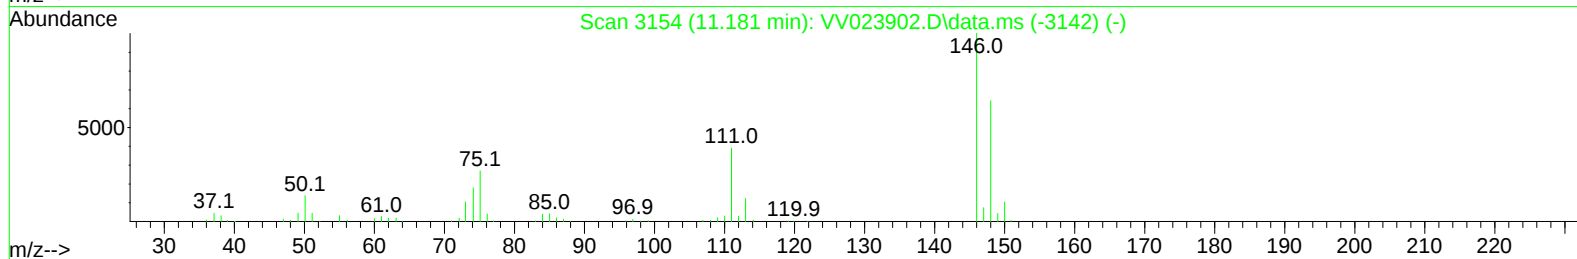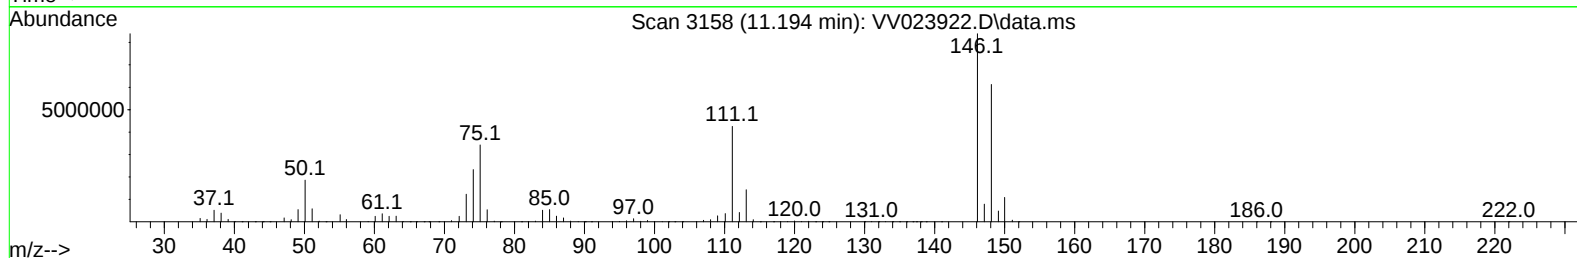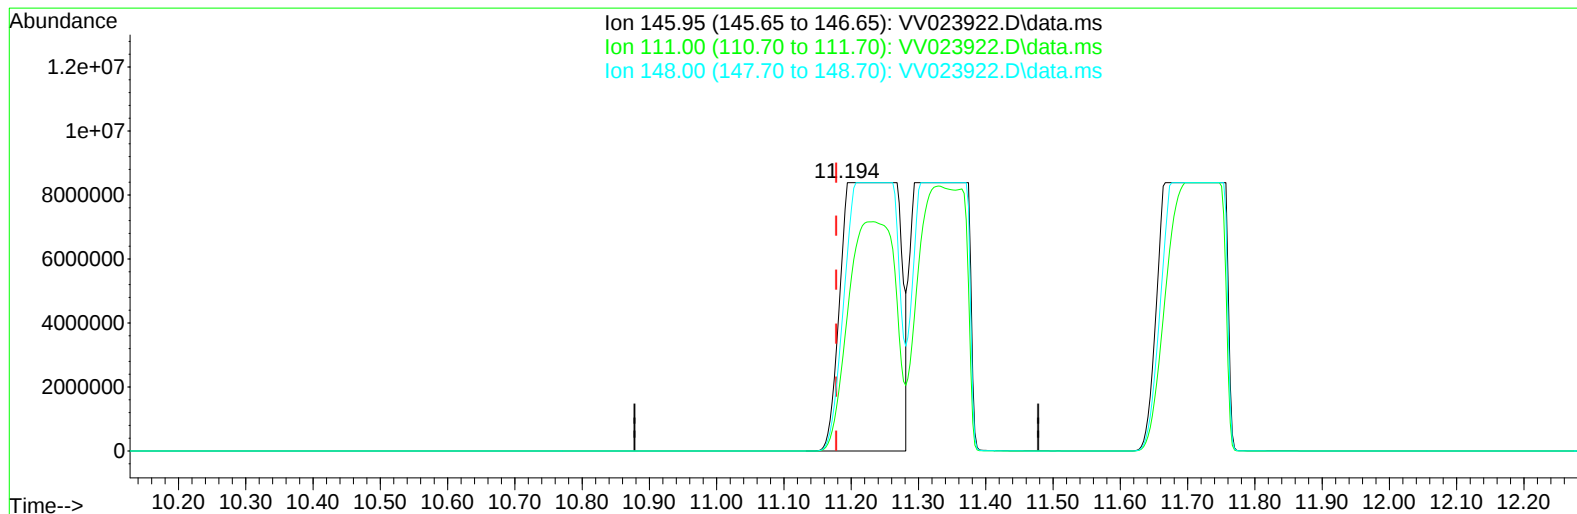

TIC: VV023922.D\data.ms

(64) 1,3-Dichlorobenzene (T)

11.194min (+ 0.016) 1932.81 ug/L m

response 49811299

Ion	Exp%	Act%
145.95	100.00	100.00
111.00	37.60	50.73#
148.00	63.50	72.98
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121021\
 Data File : VW023922.D
 Acq On : 11 Dec 2021 05:49
 Operator : SY/MD
 Sample : M5005-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW211

Manual IntegrationsAPPROVED

Quant Time: Dec 11 06:51:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	111067	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.892	117	132671	5.000	ug/L	0.04
58) 1,4-Dichlorobenzene-d4	11.310	152	85825m	5.000	ug/L	0.06
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	24042	4.027	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.600%
7) Chloroethane-d5	1.568	69	22215	4.459	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.200%
11) 1,1-Dichloroethene-d2	2.111	63	33135	2.843	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.800%#
20) 2-Butanone-d5	3.902	46	71436	61.238	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	122.480%
24) Chloroform-d	4.352	84	59675	4.412	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.200%
26) 1,2-Dichloroethane-d4	5.037	65	29892	4.747	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.000%
32) Benzene-d6	5.053	84	100974	3.843	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.800%
36) 1,2-Dichloropropane-d6	6.072	67	32807	4.138	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.800%
41) Toluene-d8	7.320	98	82886	3.504	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	70.000%
43) trans-1,3-Dichloroprop...	7.628	79	12769	3.882	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.600%
46) 2-Hexanone-d5	8.101	63	70028	47.563	ug/L	0.01
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.120%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	29609	4.502	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.000%
66) 1,2-Dichlorobenzene-d4	11.696	152	42591	3.715	ug/L	0.07
Spiked Amount	5.000	Range	80 - 120	Recovery	=	74.400%#
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.310	62	12258	1.368	ug/L	100
13) Acetone	2.191	43	3408m	3.652	ug/L	
14) Carbon disulfide	2.297	76	19559	0.905	ug/L	97
18) trans-1,2-Dichloroethene	2.760	96	67336	8.163	ug/L	96
22) cis-1,2-Dichloroethene	3.912	96	209582	24.002	ug/L	97
25) Chloroform	4.375	83	19442	1.181	ug/L	97
31) Carbon tetrachloride	4.831	117	4655	0.285	ug/L	97
33) Benzene	5.101	78	1196245	31.872	ug/L	100
34) Trichloroethene	5.915	95	101683	9.605	ug/L	99
42) Toluene	7.390	91	117152	2.774	ug/L	95
47) Tetrachloroethene	7.979	164	1014400	108.843	ug/L	97
51) Chlorobenzene	8.889	112	47091834m	1668.056	ug/L	
52) Ethylbenzene	9.030	91	8775	0.197	ug/L	96
53) m,p-xylene	9.146	106	8702	0.494	ug/L	88
54) o-xylene	9.554	106	7461	0.438	ug/L	98
60) Isopropylbenzene	9.943	105	8087	0.160	ug/L	# 54
63) 1,2,4-Trimethylbenzene	10.956	105	13943m	0.335	ug/L	
64) 1,3-Dichlorobenzene	11.194	146	49811299m	1932.807	ug/L	
65) 1,4-Dichlorobenzene	11.294	146	47446513m	1833.036	ug/L	

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023922.D
 Acq On : 11 Dec 2021 05:49
 Operator : SY/MD
 Sample : M5005-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW211

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:51:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
67) 1,2-Dichlorobenzene	11.667	146	55508450m	2350.965	ug/L		
70) 1,2,4-trichlorobenzene	13.265	180	658163	39.534	ug/L		98
72) 1,2,3-Trichlorobenzene	13.747	180	80328	5.465	ug/L		99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023922.D
 Acq On : 11 Dec 2021 05:49
 Operator : SY/MD
 Sample : M5005-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW211

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/13/2021
 Supervised By :Semsettin Yesilyurt 12/13/2021

Quant Time: Dec 11 06:51:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

