

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023884.D
 Acq On : 10 Dec 2021 14:20
 Operator : SY/MD
 Sample : VV1210WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK274

Quant Time: Dec 11 04:44:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	107624	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	112260	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59033	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	29620	5.119	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	102.400%	
7) Chloroethane-d5	1.568	69	25748	5.334	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	106.600%	
11) 1,1-Dichloroethene-d2	2.108	63	40226	3.562	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	71.200%	
20) 2-Butanone-d5	3.908	46	50128	44.347	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	88.700%	
24) Chloroform-d	4.346	84	63856	4.873	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.400%	
26) 1,2-Dichloroethane-d4	5.030	65	32280	5.290	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.800%	
32) Benzene-d6	5.047	84	114560	5.152	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	103.000%	
36) 1,2-Dichloropropane-d6	6.069	67	35808	5.338	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	106.800%	
41) Toluene-d8	7.313	98	97267	4.859	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.200%	
43) trans-1,3-Dichloroprop...	7.622	79	13520	4.858	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	97.200%	
46) 2-Hexanone-d5	8.088	63	60370	48.458	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	96.920%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	26706	4.799	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	42718	5.417	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	108.400%	
Target Compounds						Qvalue
16) Methylene chloride	2.506	84	3765	0.399	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023884.D
Acq On : 10 Dec 2021 14:20
Operator : SY/MD
Sample : VV1210WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK274

Quant Time: Dec 11 04:44:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 11 04:33:17 2021
Response via : Initial Calibration

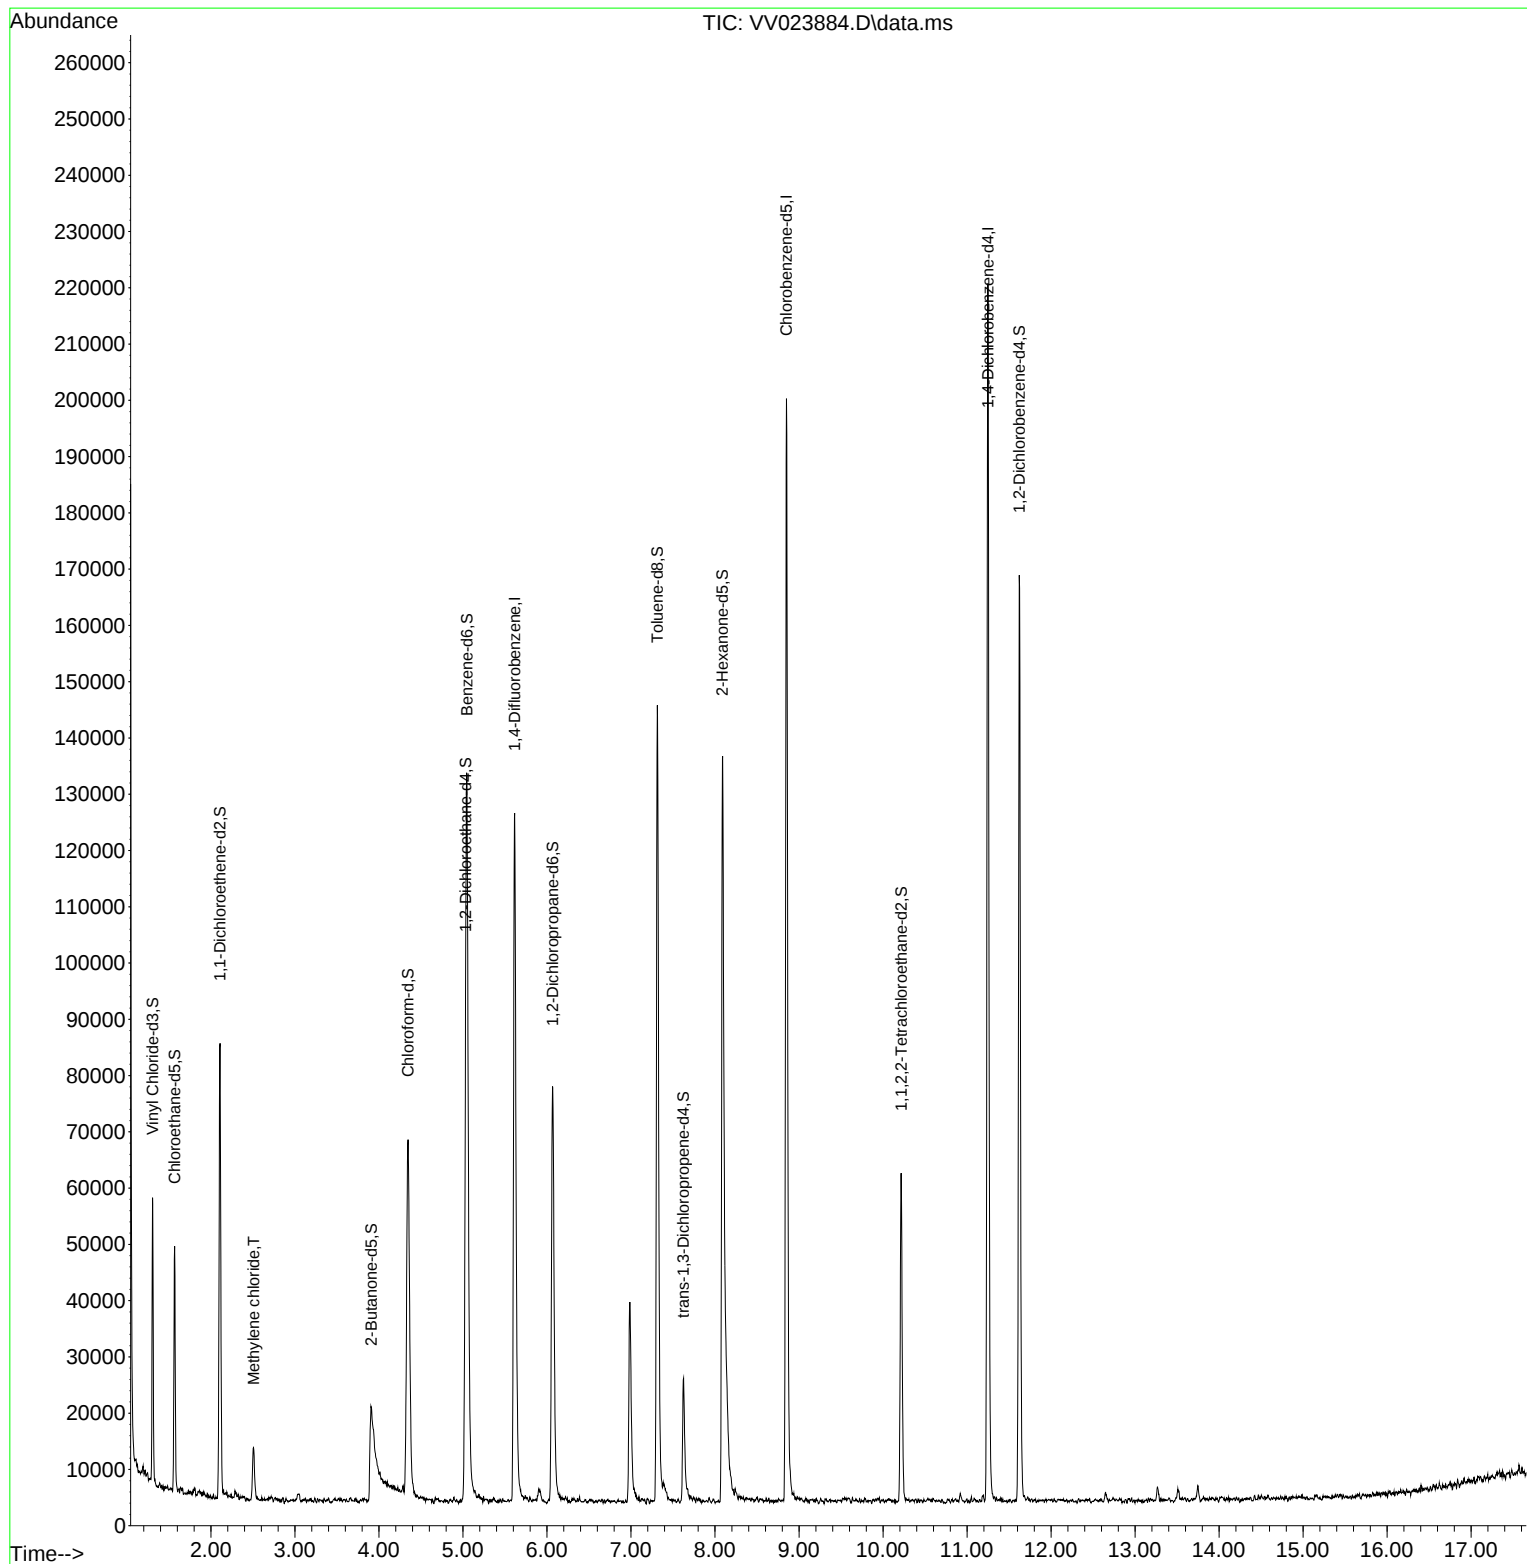

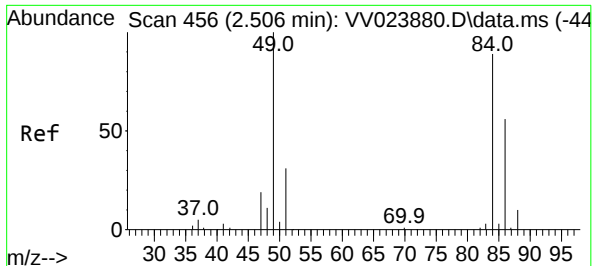

#16

Methylene chloride

Concen: 0.399 ug/L

RT: 2.506 min Scan# 4

Delta R.T. 0.000 min

Lab File: VV023884.D


Acq: 10 Dec 2021 14:20

Instrument :

MSVOA_V

ClientSampleId :

VBLK274

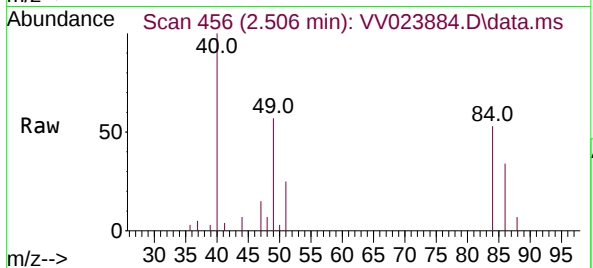

Tgt Ion: 84 Resp: 3765

Ion Ratio Lower Upper

84 100

86 64.8 42.6 79.0

49 107.6 79.7 147.9

