

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023887.D
 Acq On : 10 Dec 2021 15:32
 Operator : SY/MD
 Sample : M5003-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CX3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023887.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	44	50	65	rVB	100465	91298	28.31%	3.225%
2	1.304	75	82	93	rVB	45772	46129	14.31%	1.630%
3	1.568	154	164	173	rBV	41707	46606	14.45%	1.646%
4	2.108	322	332	347	rBV	72781	101647	31.52%	3.591%
5	3.896	878	888	912	rBV	34376	109617	34.00%	3.873%
6	4.352	1013	1030	1052	rBV3	58996	149003	46.21%	5.264%
7	5.047	1228	1246	1269	rBV3	117945	298923	92.71%	10.560%
8	5.619	1412	1424	1447	rBV	117168	240836	74.69%	8.508%
9	6.069	1549	1564	1590	rBV	69822	147021	45.60%	5.194%
10	6.989	1838	1850	1871	rBV2	33325	63977	19.84%	2.260%
11	7.317	1942	1952	1969	rBV	125833	225528	69.94%	7.967%
12	7.625	2039	2048	2064	rBV2	20346	37411	11.60%	1.322%
13	7.940	2135	2146	2156	rVB3	3519	6377	1.98%	0.225%
14	8.088	2181	2192	2221	rBV	162546	300368	93.15%	10.611%
15	8.854	2418	2430	2448	rBV	192422	318503	98.78%	11.252%
16	10.217	2843	2854	2867	rBV	56809	87302	27.08%	3.084%
17	10.384	2899	2906	2917	rVB4	4149	7289	2.26%	0.258%
18	11.249	3164	3175	3199	rBV	204555	322445	100.00%	11.391%
19	11.625	3276	3292	3308	rBV	142424	230352	71.44%	8.138%




Sum of corrected areas: 2830632

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023887.D
Acq On : 10 Dec 2021 15:32
Operator : SY/MD
Sample : M5003-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

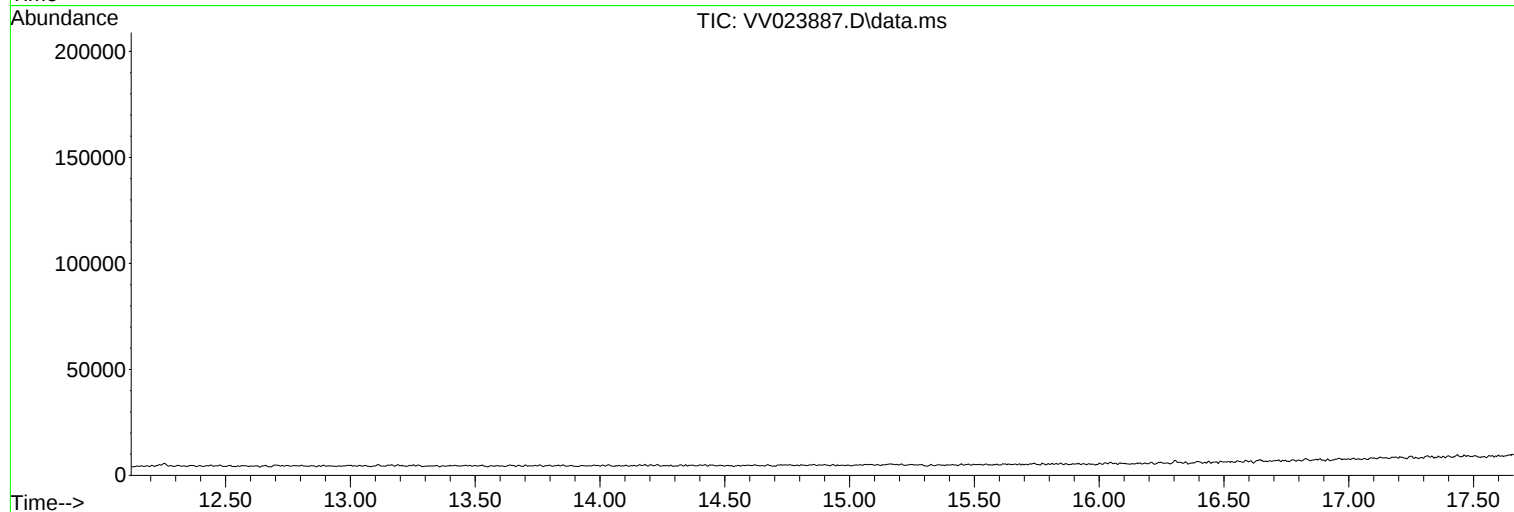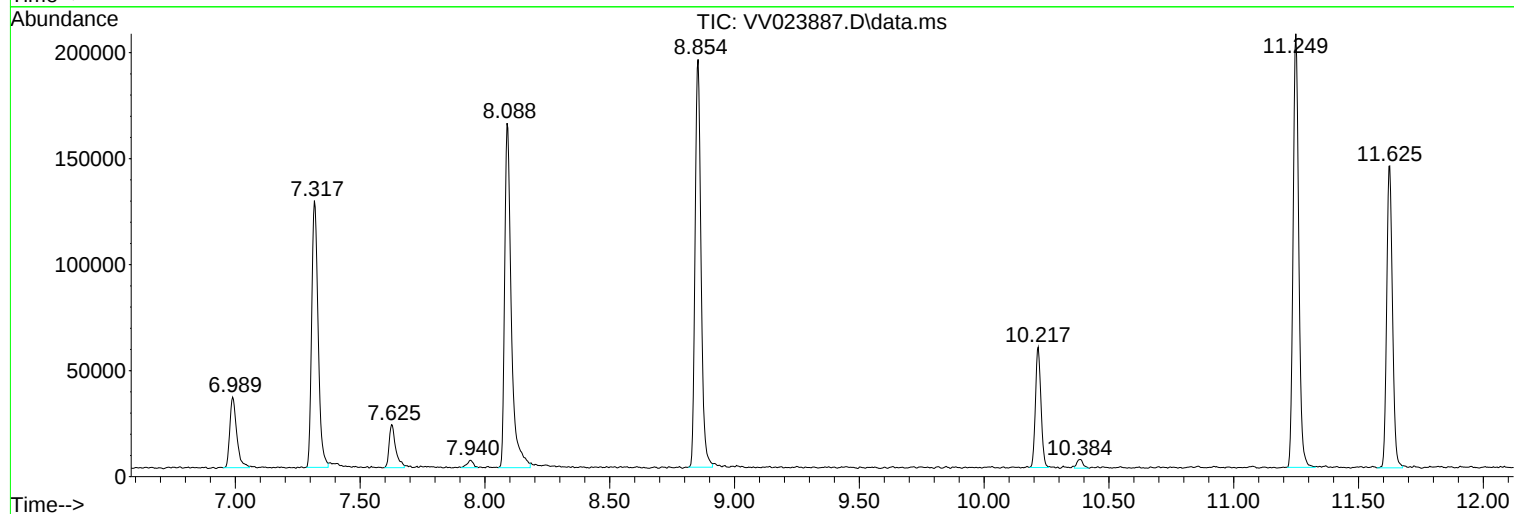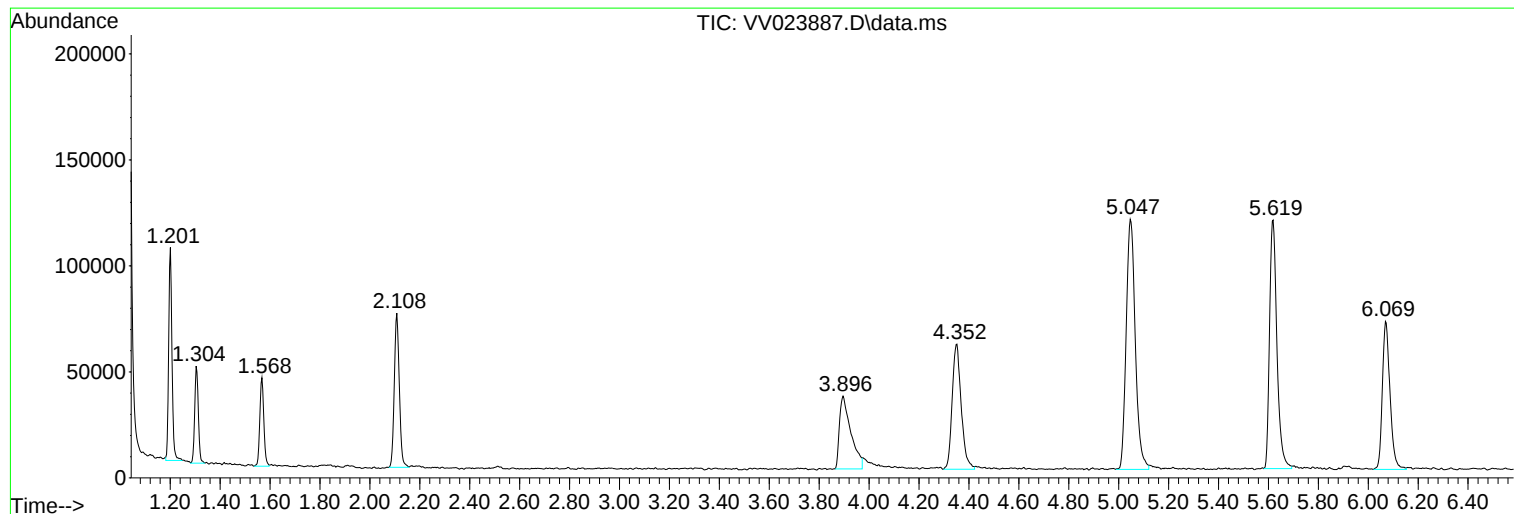

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023887.D
Acq On : 10 Dec 2021 15:32
Operator : SY/MD
Sample : M5003-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CX3










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.201	1.90 ug/L	91298	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methyl nitrite	61	CH3NO2	000624-91-9	5
2			Thiirane	60	C2H4S	000420-12-2	5
3			Ethyne, chloro-	60	C2HCl	000593-63-5	5
4			o-Ethylhydroxylamine	61	C2H7NO	000624-86-2	4
5			Methanamine, N-methoxy-	61	C2H7NO	001117-97-1	4

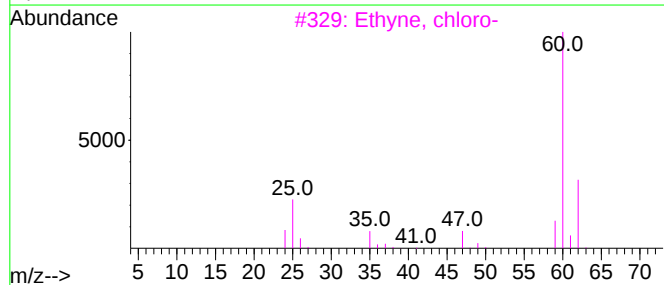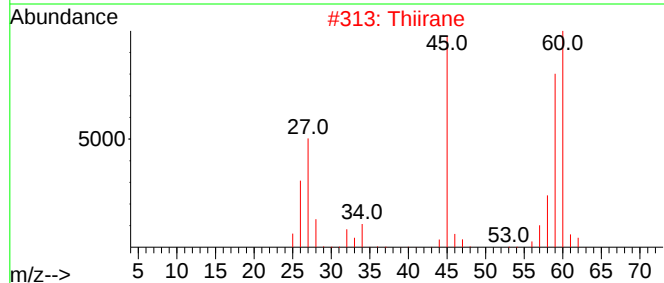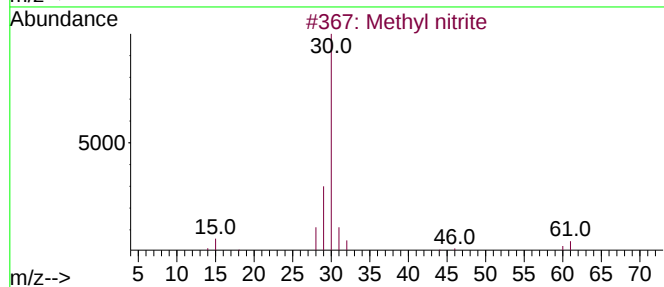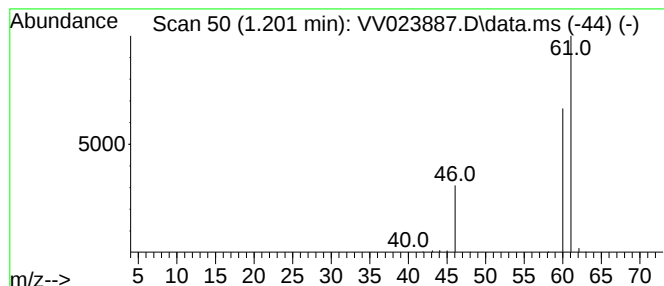

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023887.D
Acq On : 10 Dec 2021 15:32
Operator : SY/MD
Sample : M5003-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.201	1.9	ug/L	91298	1	5.619	240836	5.0