

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023899.D
 Acq On : 10 Dec 2021 20:14
 Operator : SY/MD
 Sample : M4984-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW5S6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023899.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	48	54	61	rBV4	8646	8297	2.63%	0.308%
2	1.304	74	82	93	rVB	41819	46387	14.68%	1.719%
3	1.568	158	164	174	rVB	39393	44324	14.03%	1.643%
4	2.108	322	332	345	rVB	69569	104647	33.12%	3.879%
5	3.912	882	893	898	rBV	20809	38552	12.20%	1.429%
6	4.352	1011	1030	1052	rBV	57698	152286	48.19%	5.645%
7	5.050	1227	1247	1269	rBV2	117174	293772	92.97%	10.889%
8	5.619	1413	1424	1444	rBV2	112633	233367	73.85%	8.650%
9	6.072	1552	1565	1585	rBV	69248	146229	46.27%	5.420%
10	6.992	1838	1851	1872	rBV2	33056	63987	20.25%	2.372%
11	7.317	1941	1952	1968	rBV	121349	214616	67.92%	7.955%
12	7.397	1972	1977	1984	rVB5	3540	4722	1.49%	0.175%
13	7.628	2040	2049	2073	rBV2	18684	36548	11.57%	1.355%
14	7.979	2153	2158	2165	rVB5	2645	3335	1.06%	0.124%
15	8.091	2180	2193	2223	rBV	148755	304697	96.42%	11.294%
16	8.255	2238	2244	2259	rVB9	2730	6466	2.05%	0.240%
17	8.853	2419	2430	2451	rBV	189095	313794	99.30%	11.631%
18	9.143	2512	2520	2533	rBV5	6140	10541	3.34%	0.391%
19	9.548	2638	2646	2656	rBV	7888	14763	4.67%	0.547%
20	9.815	2720	2729	2740	rVB5	2354	3901	1.23%	0.145%
21	10.217	2844	2854	2867	rVB2	54979	88480	28.00%	3.280%
22	10.381	2901	2905	2914	rVB6	2395	3180	1.01%	0.118%
23	10.770	3019	3026	3037	rVB8	3295	5183	1.64%	0.192%
24	10.918	3065	3072	3079	rBV4	3182	4682	1.48%	0.174%
25	11.249	3161	3175	3193	rBV	202994	316000	100.00%	11.713%
26	11.625	3279	3292	3313	rBV	141601	225591	71.39%	8.362%
27	12.348	3508	3517	3525	rBV7	6544	9595	3.04%	0.356%




Sum of corrected areas: 2697942

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023899.D
Acq On : 10 Dec 2021 20:14
Operator : SY/MD
Sample : M4984-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW5S6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

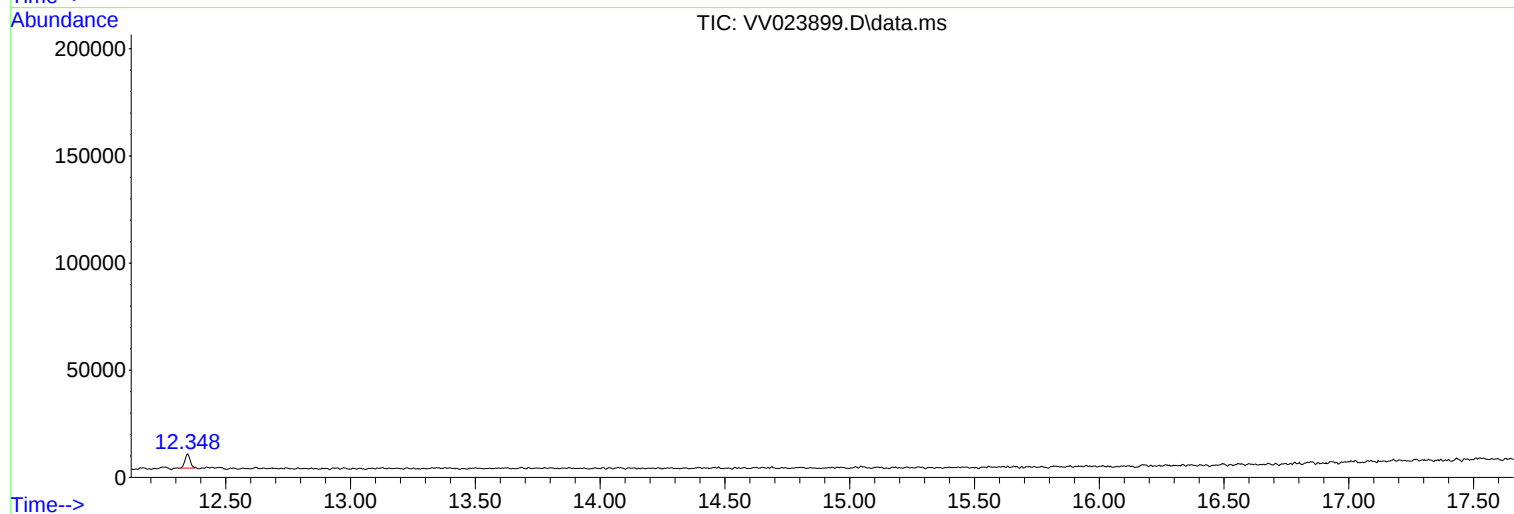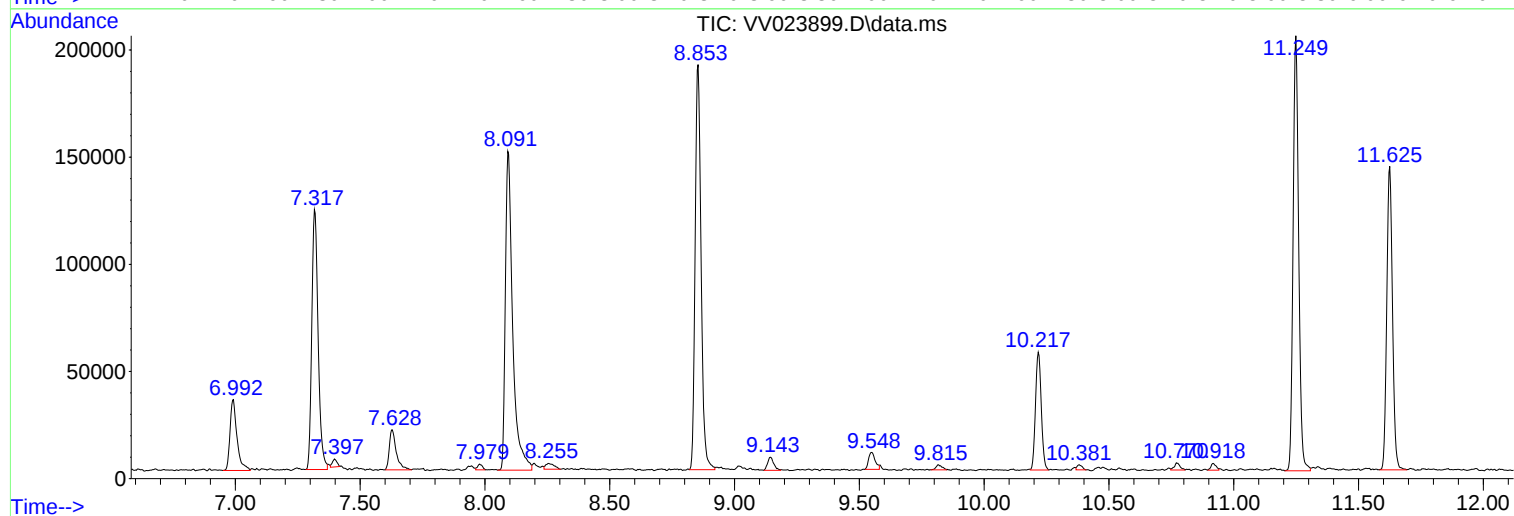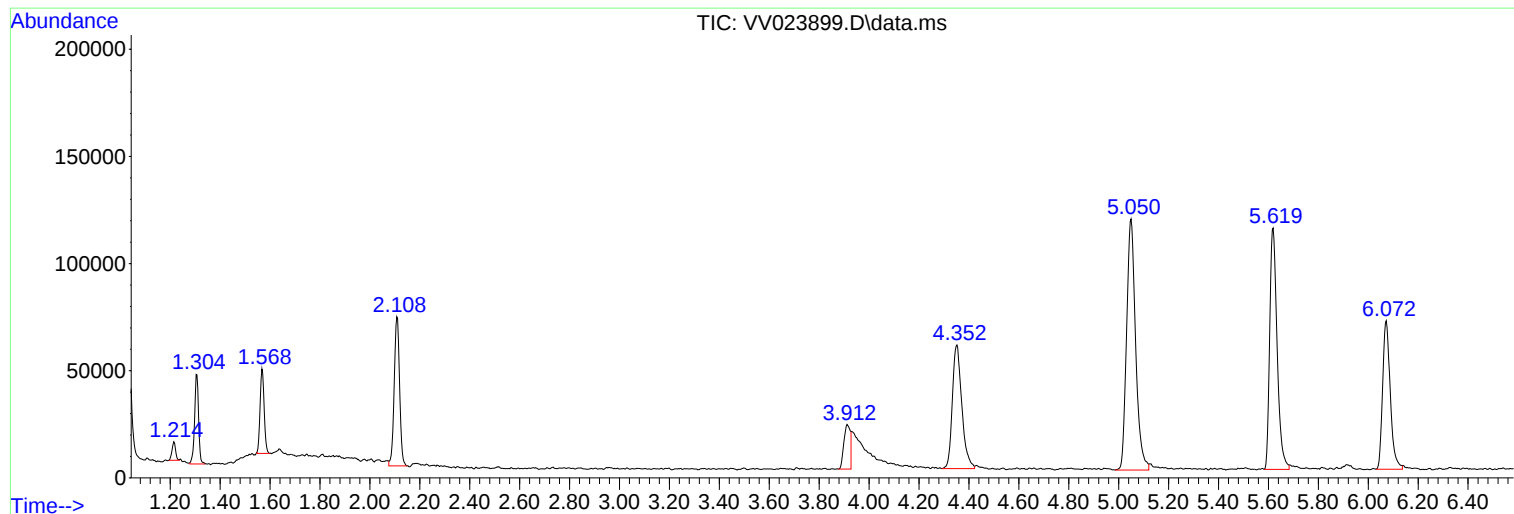

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023899.D
Acq On : 10 Dec 2021 20:14
Operator : SY/MD
Sample : M4984-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW5S6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023899.D
Acq On : 10 Dec 2021 20:14
Operator : SY/MD
Sample : M4984-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW5S6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc