

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023918.D
 Acq On : 11 Dec 2021 04:14
 Operator : SY/MD
 Sample : M5005-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW207

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023918.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	93	rBV	40657	40897	13.31%	1.495%
2	1.568	156	164	171	rBV	38712	43078	14.02%	1.575%
3	2.108	322	332	345	rBV	63724	91960	29.93%	3.363%
4	2.198	345	360	394	rBV2	30950	147000	47.84%	5.375%
5	3.908	883	892	928	rBV2	17526	79915	26.01%	2.922%
6	4.352	1014	1030	1058	rVB3	58750	159617	51.95%	5.837%
7	4.831	1170	1179	1191	rBV8	2880	6421	2.09%	0.235%
8	5.050	1232	1247	1269	rBV3	108344	275908	89.80%	10.089%
9	5.619	1412	1424	1450	rBV2	110744	231134	75.23%	8.452%
10	5.915	1507	1516	1528	rVB9	3865	8636	2.81%	0.316%
11	6.072	1549	1565	1586	rBV2	66520	141897	46.18%	5.189%
12	6.992	1841	1851	1872	rBV	29676	57026	18.56%	2.085%
13	7.317	1940	1952	1968	rBV	107539	191401	62.30%	6.999%
14	7.629	2039	2049	2066	rBV3	16365	31338	10.20%	1.146%
15	8.092	2184	2193	2226	rBV	125631	300098	97.67%	10.974%
16	8.854	2418	2430	2450	rBV	186208	307249	100.00%	11.235%
17	10.217	2842	2854	2866	rBV	52841	87217	28.39%	3.189%
18	11.249	3164	3175	3192	rBV	187709	294689	95.91%	10.776%
19	11.535	3253	3264	3277	rBV4	11568	22821	7.43%	0.835%
20	11.625	3281	3292	3309	rVB	135498	216371	70.42%	7.912%




Sum of corrected areas: 2734673

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023918.D
Acq On : 11 Dec 2021 04:14
Operator : SY/MD
Sample : M5005-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW207

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

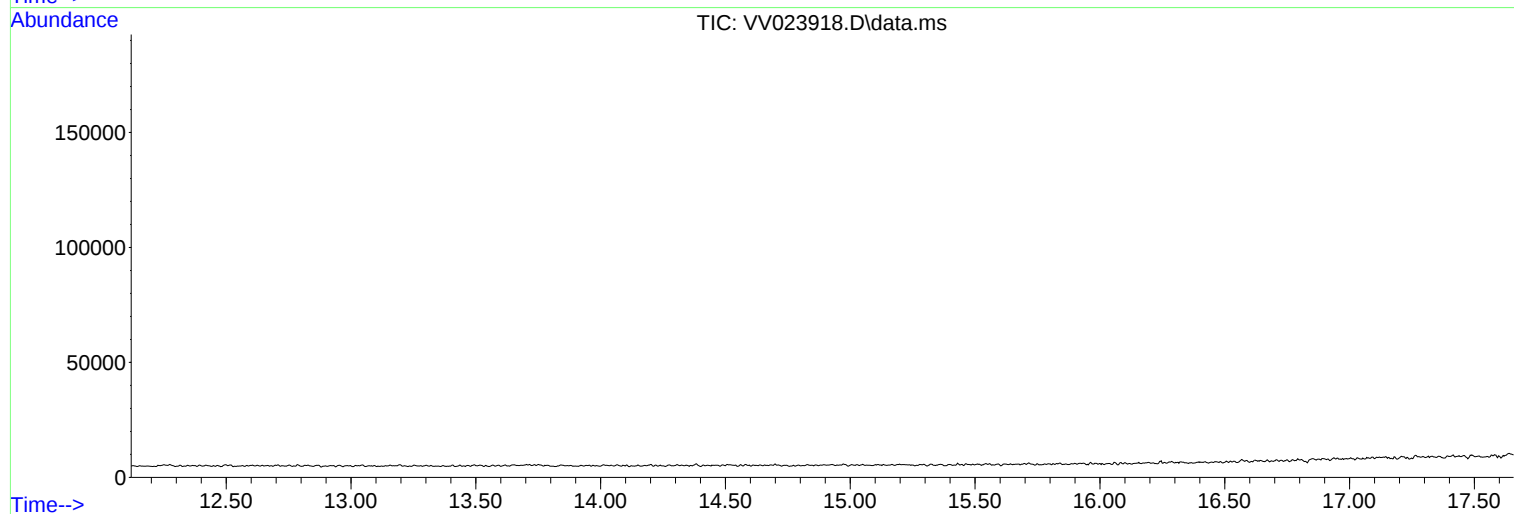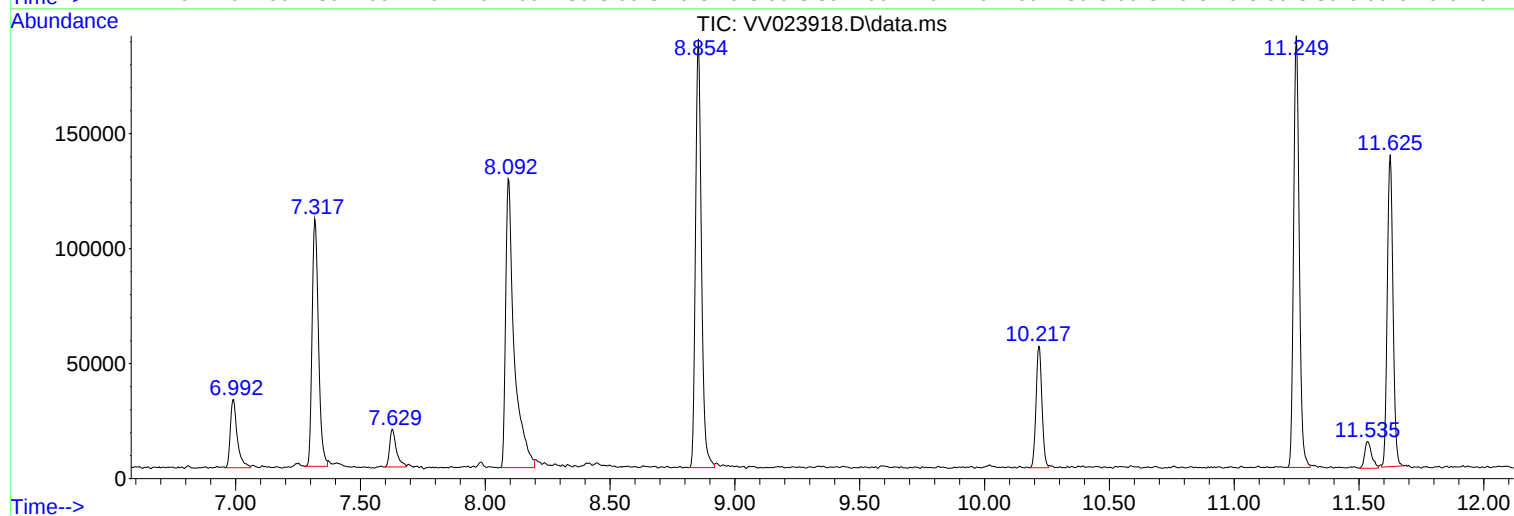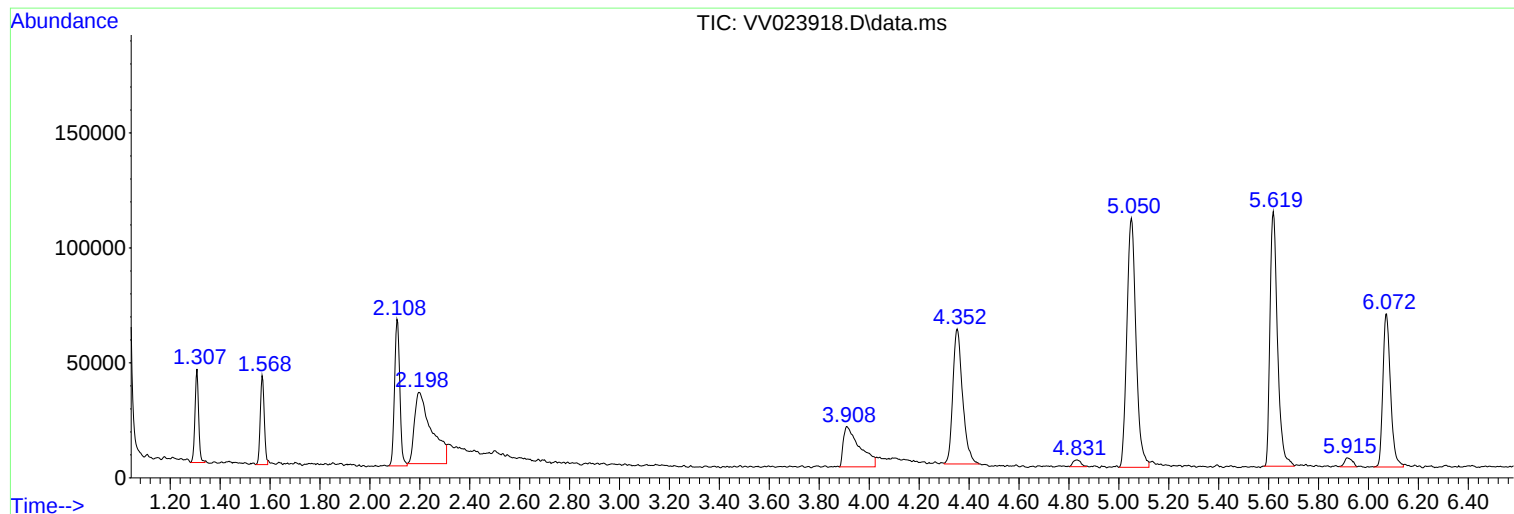

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023918.D
Acq On : 11 Dec 2021 04:14
Operator : SY/MD
Sample : M5005-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW207

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
Data File : VV023918.D
Acq On : 11 Dec 2021 04:14
Operator : SY/MD
Sample : M5005-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW207

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc