


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121021\
 Data File : VV023876.D
 Acq On : 10 Dec 2021 09:44
 Operator : SY/MD
 Sample : BFB249
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB249

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Dec 11 04:33:17 2021

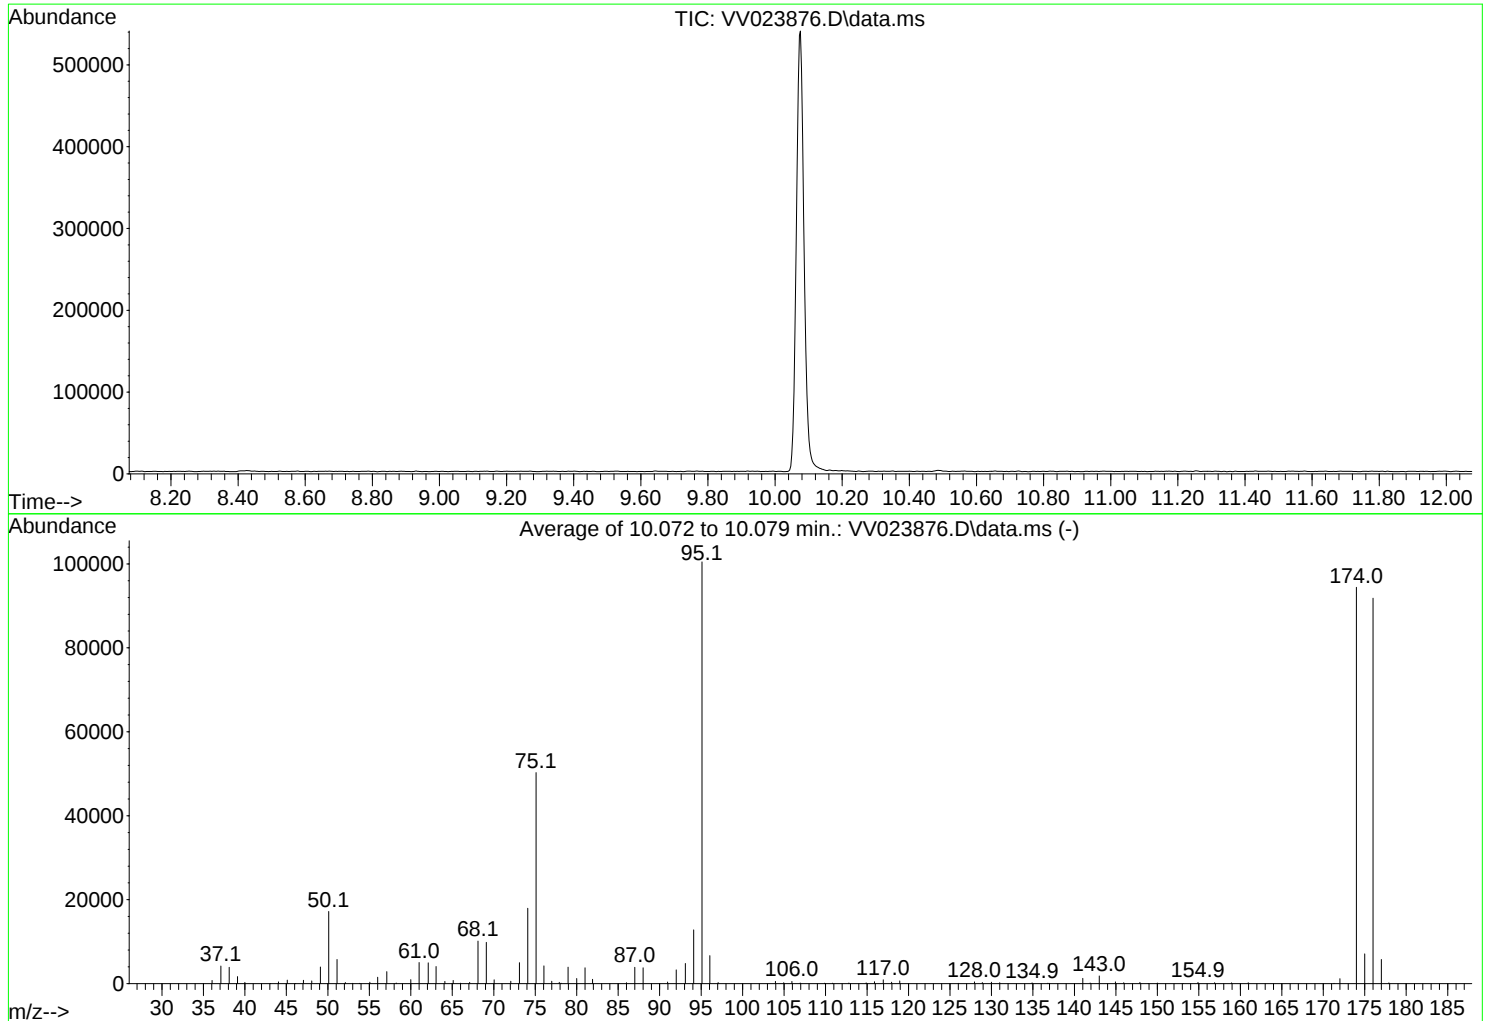

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	17178	PASS
75	95	30	80	50.0	50285	PASS
95	95	100	100	100.0	100491	PASS
96	95	5	9	6.6	6679	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	94.0	94416	PASS
175	174	5	9	7.5	7084	PASS
176	174	95	105	97.2	91819	PASS
177	176	5	10	6.3	5776	PASS

m/z	Abundance
40.00	2666.0
44.00	140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB249

m/z	Abundance
36.10	830.0
37.10	4307.0
38.10	4240.0
39.10	1890.0
40.00	2857.0
44.10	561.0
45.10	993.0
46.10	105.0
47.10	1018.0
48.00	690.0
49.10	4217.0
50.10	17688.0
51.10	6020.0
52.10	262.0
53.10	103.0
55.10	349.0
56.00	1554.0
57.10	3027.0
58.20	121.0
60.00	906.0
61.00	4946.0
62.10	5316.0
63.10	4307.0
64.10	592.0
65.10	750.0
66.00	114.0
67.10	257.0
68.10	10617.0
69.10	10271.0
70.10	902.0
72.10	584.0
73.10	5078.0
74.10	18336.0
75.10	52048.0
76.10	4286.0
77.00	631.0
77.90	478.0
79.00	3964.0
80.00	1209.0
81.00	3712.0
81.90	1039.0
86.00	187.0
87.00	4079.0
88.00	4022.0
91.00	404.0
92.00	3188.0
93.10	4950.0
94.10	13010.0
95.10	103640.0
96.10	7125.0
97.00	233.0
104.00	579.0
104.90	198.0
106.00	523.0
107.00	144.0
110.00	108.0
110.90	145.0
112.80	156.0
114.90	171.0
115.90	476.0
117.00	926.0
118.00	376.0
118.90	706.0
127.90	459.0
128.90	248.0
130.00	349.0
131.00	185.0
134.90	189.0
136.80	216.0
141.00	1321.0
141.90	189.0
143.00	1900.0
145.00	457.0
145.90	222.0
147.90	256.0
148.90	110.0
150.00	197.0
154.90	338.0
156.90	272.0
159.00	193.0
160.90	217.0
172.00	1148.0
174.00	95520.0
175.00	7506.0
176.00	91936.0
177.00	6029.0
177.90	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB249

m/z	Abundance
36.00	797.0
37.10	4326.0
38.10	4012.0
39.10	1722.0
40.00	2926.0
44.10	540.0
45.10	884.0
47.00	787.0
48.10	665.0
49.10	4194.0
50.10	17664.0
51.10	6000.0
52.10	259.0
52.90	106.0
53.90	117.0
55.10	356.0
56.00	1612.0
57.10	2977.0
58.30	179.0
60.00	966.0
61.00	5311.0
62.10	5136.0
63.10	4201.0
64.10	517.0
65.10	777.0
66.00	118.0
67.10	319.0
68.10	10558.0
69.10	10157.0
70.10	945.0
72.00	593.0
73.10	5138.0
74.10	18640.0
75.10	51880.0
76.10	4380.0
77.00	620.0
77.90	422.0
78.90	4028.0
80.00	1277.0
81.00	3925.0
81.90	1071.0
86.00	260.0
87.00	3985.0
88.00	3929.0
91.00	362.0
92.00	3440.0
93.10	4994.0
94.10	13232.0
95.10	104024.0
96.10	6928.0
97.10	276.0
103.90	541.0
105.00	230.0
105.90	568.0
107.00	154.0
109.90	112.0
110.90	109.0
112.80	187.0
114.90	206.0
115.90	458.0
117.00	942.0
118.00	368.0
119.00	657.0
126.00	110.0
128.00	428.0
128.90	277.0
130.00	351.0
131.00	244.0
134.90	206.0
136.80	190.0
141.00	1338.0
141.90	179.0
143.00	1931.0
144.90	457.0
146.00	224.0
147.90	299.0
150.00	178.0
154.90	338.0
156.90	233.0
159.00	182.0
160.90	239.0
172.00	1246.0
174.00	97536.0
175.00	7307.0
176.00	94776.0
177.00	5920.0
177.90	197.0

Instrument :
MSVOA_V
ClientSampleId :
BFB249

m/z	Abundance
36.00	697.0
37.10	3958.0
38.10	3431.0
39.10	1440.0
40.00	3125.0
43.10	127.0
44.10	576.0
45.10	682.0
47.00	581.0
48.00	594.0
49.10	3540.0
50.10	16182.0
51.10	5205.0
52.10	241.0
53.80	115.0
55.00	330.0
56.00	1394.0
57.10	2584.0
58.30	181.0
60.00	1016.0
61.00	4876.0
62.10	4400.0
63.00	3764.0
64.10	448.0
65.10	753.0
66.00	122.0
67.10	324.0
68.10	9300.0
69.10	9120.0
70.00	887.0
72.00	585.0
73.10	4765.0
74.10	16856.0
75.10	46928.0
76.00	4036.0
77.00	494.0
78.10	321.0
78.90	3749.0
80.00	1153.0
81.00	3654.0
81.90	1031.0
86.00	277.0
87.00	3665.0
88.00	3395.0
90.90	327.0
92.00	3204.0
93.10	4524.0
94.10	12166.0
95.10	93808.0
96.00	5983.0
97.10	251.0
103.90	473.0
105.00	221.0
105.90	550.0
106.90	166.0
109.80	131.0
110.80	102.0
112.80	182.0
114.90	204.0
115.90	404.0
116.90	855.0
117.90	343.0
119.00	571.0
126.00	107.0
127.90	399.0
128.90	253.0
130.00	314.0
131.00	257.0
134.90	190.0
137.00	184.0
141.00	1162.0
141.90	145.0
143.00	1709.0
144.90	399.0
146.00	205.0
147.90	310.0
150.00	150.0
153.10	103.0
154.90	265.0
156.90	186.0
158.90	190.0
161.00	204.0
171.30	208.0
172.00	1180.0
174.00	90192.0
175.00	6439.0
176.00	88744.0
177.00	5380.0
177.90	194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB249