




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039522.D
Acq On : 10 Dec 2025 11:23
Operator : SY/MD
Sample : Q3788-12
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-16B-87.5-120525-SIM

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

Quant Time: Dec 11 00:05:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

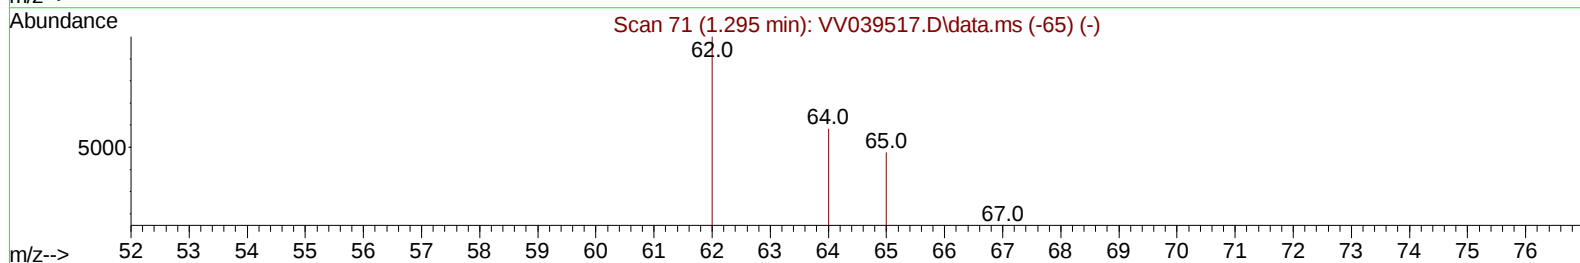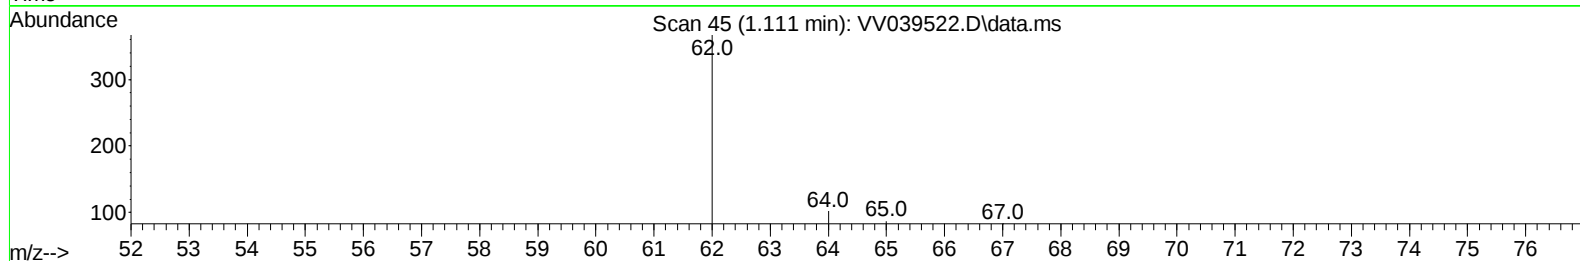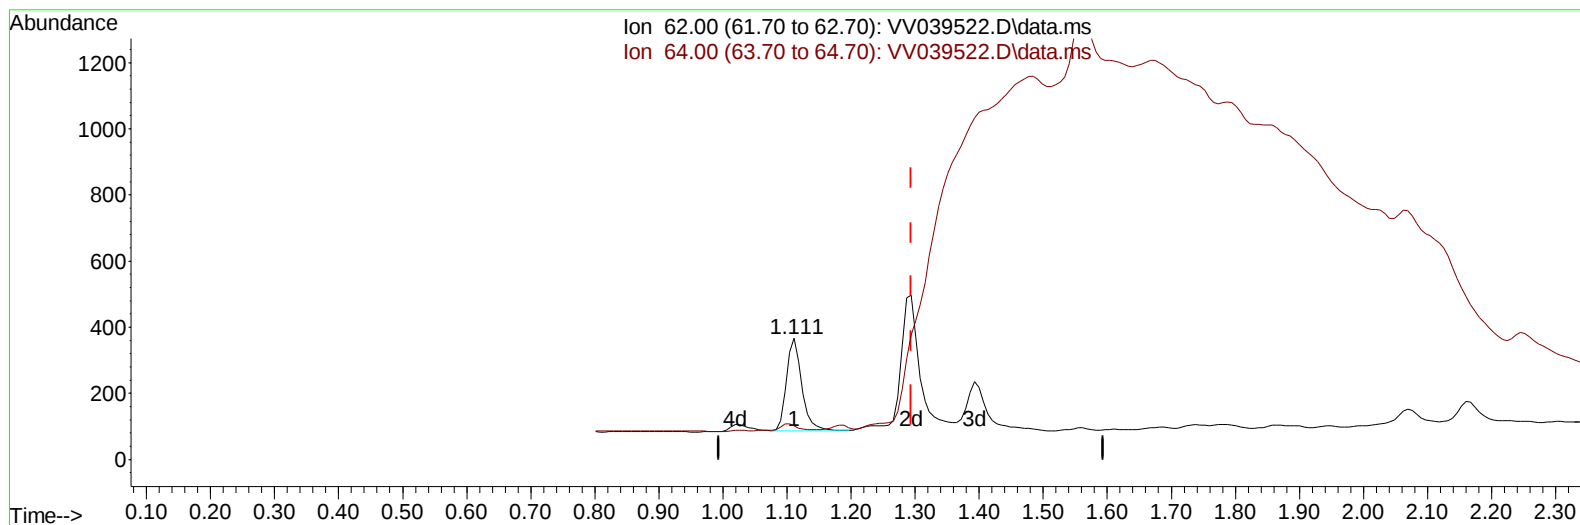

TIC: VV039522.D\data.ms

(3) Vinyl chloride (T)

1.111min (-0.183) 0.03 ug/L

response 466

Ion	Exp%	Act%
62.00	100.00	100.00
64.00	35.40	27.79
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039522.D
Acq On : 10 Dec 2025 11:23
Operator : SY/MD
Sample : Q3788-12
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-16B-87.5-120525-SIM

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

Quant Time: Dec 11 00:05:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

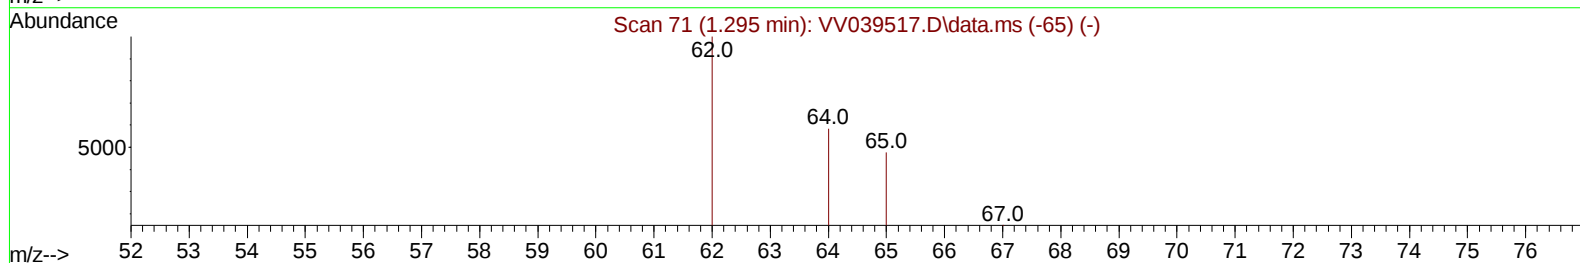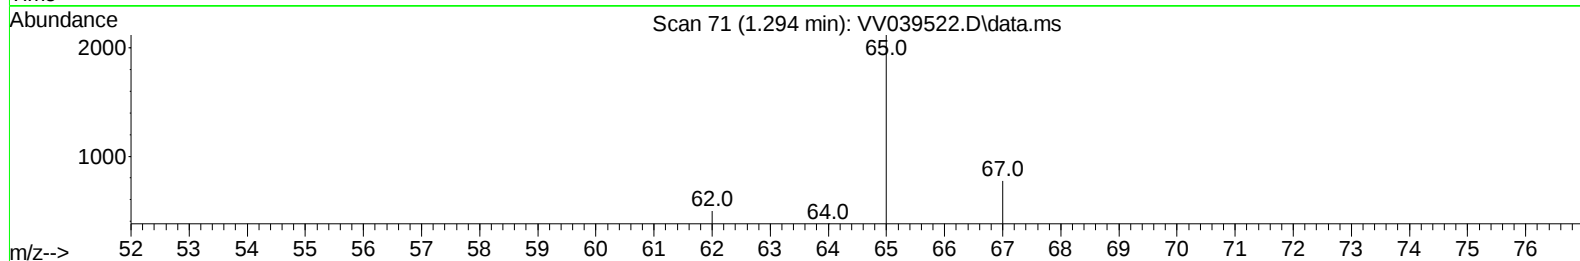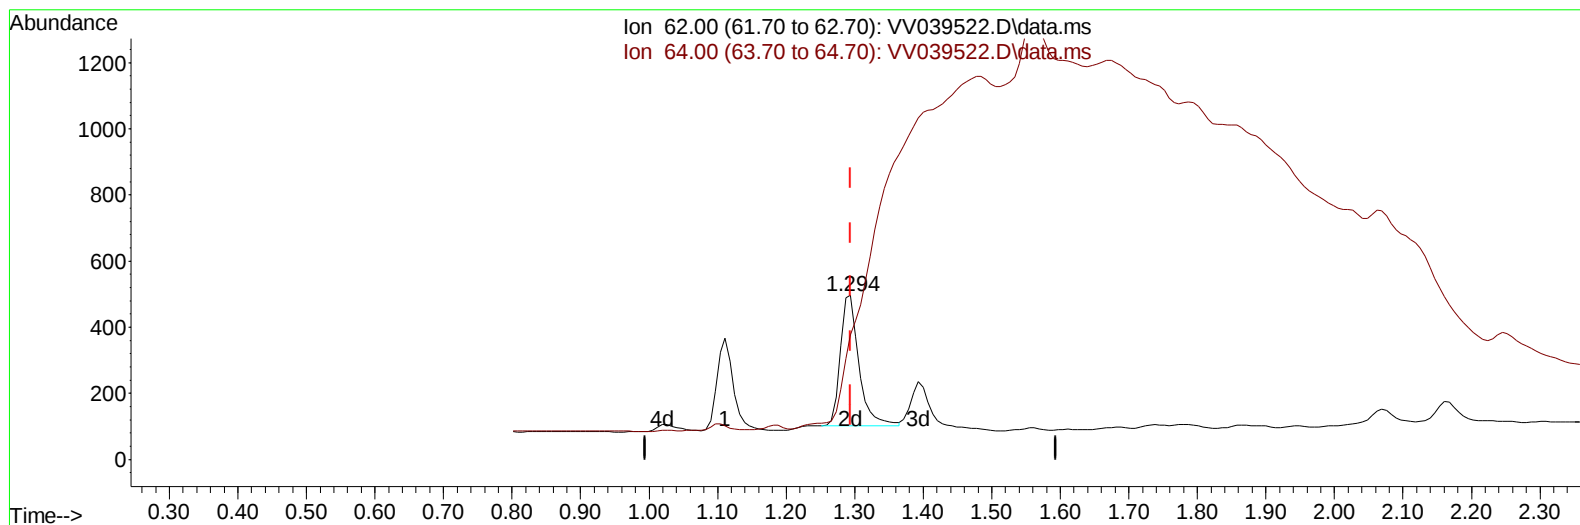

TIC: VV039522.D\data.ms

(3) Vinyl chloride (T)

1.294min (+ 0.000) 0.05 ug/L m

response 746

Ion	Exp%	Act%
62.00	100.00	100.00
64.00	35.40	76.01#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
 Data File : VV039522.D
 Acq On : 10 Dec 2025 11:23
 Operator : SY/MD
 Sample : Q3788-12
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MW-16B-87.5-120525-SIM

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/11/2025
 Supervised By :Semsettin Yesilyurt 12/12/2025

Quant Time: Dec 11 00:05:59 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 09 08:40:48 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	7573	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	6749	0.500	ug/L	0.00
12) 1,4-Dichlorobenzene-d4	11.175	152	7636	0.500	ug/L	# 0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.287	65	4136	0.556	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	112.000%		
4) 1,2-Dichloroethane-d4	4.969	65	2145	0.425	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	86.000%		
7) 1,2-Dichloropropane-d6	5.995	67	2430	0.427	ug/L	-0.02
Spiked Amount 0.500	Range 60 - 140		Recovery =	86.000%		
8) Toluene-d8	7.253	98	4504	0.469	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	94.000%		
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1666	0.519	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	104.000%		
Target Compounds						
3) Vinyl chloride	1.294	62	746m	0.046	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039522.D
Acq On : 10 Dec 2025 11:23
Operator : SY/MD
Sample : Q3788-12
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-16B-87.5-120525-SIM

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

Quant Time: Dec 11 00:05:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

