




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039525.D
Acq On : 10 Dec 2025 13:01
Operator : SY/MD
Sample : Q3813-02
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BR-04DR-451-120825-SIM

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

Quant Time: Dec 11 00:06:30 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

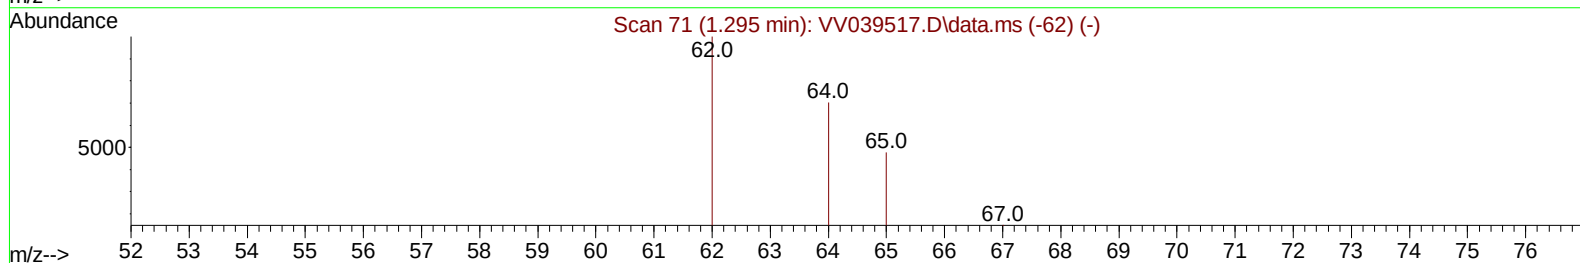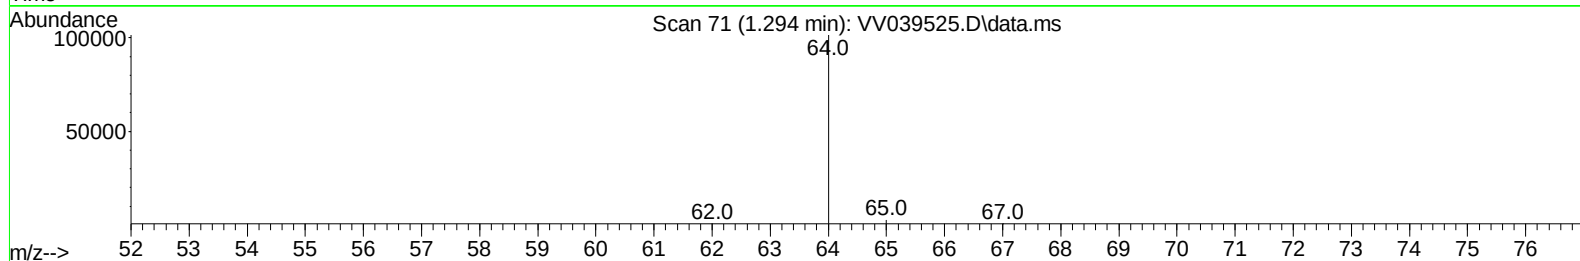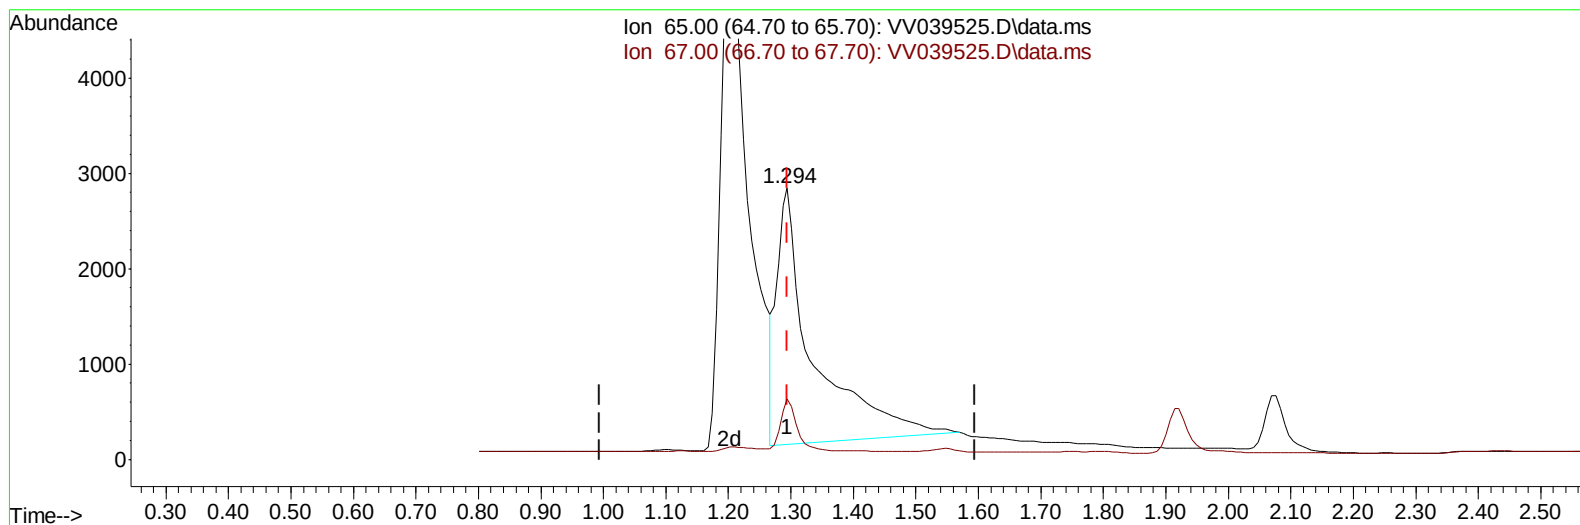

TIC: VV039525.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.294min (+ 0.000) 1.81 ug/L

response 11036

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	9.69#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039525.D
Acq On : 10 Dec 2025 13:01
Operator : SY/MD
Sample : Q3813-02
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BR-04DR-451-120825-SIM

Manual IntegrationsAPPROVED

Quant Time: Dec 11 00:06:30 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

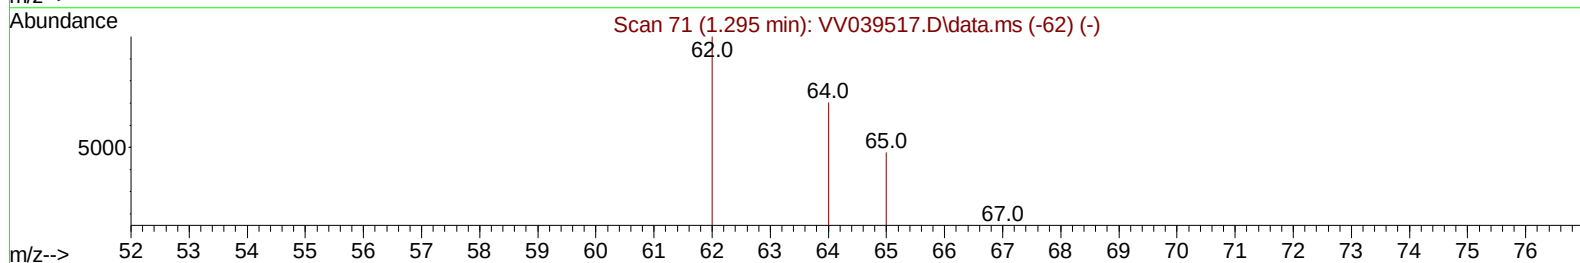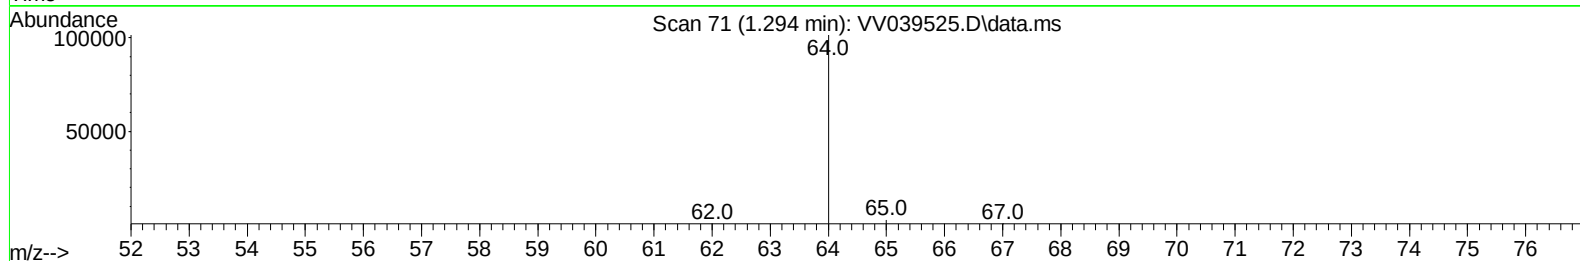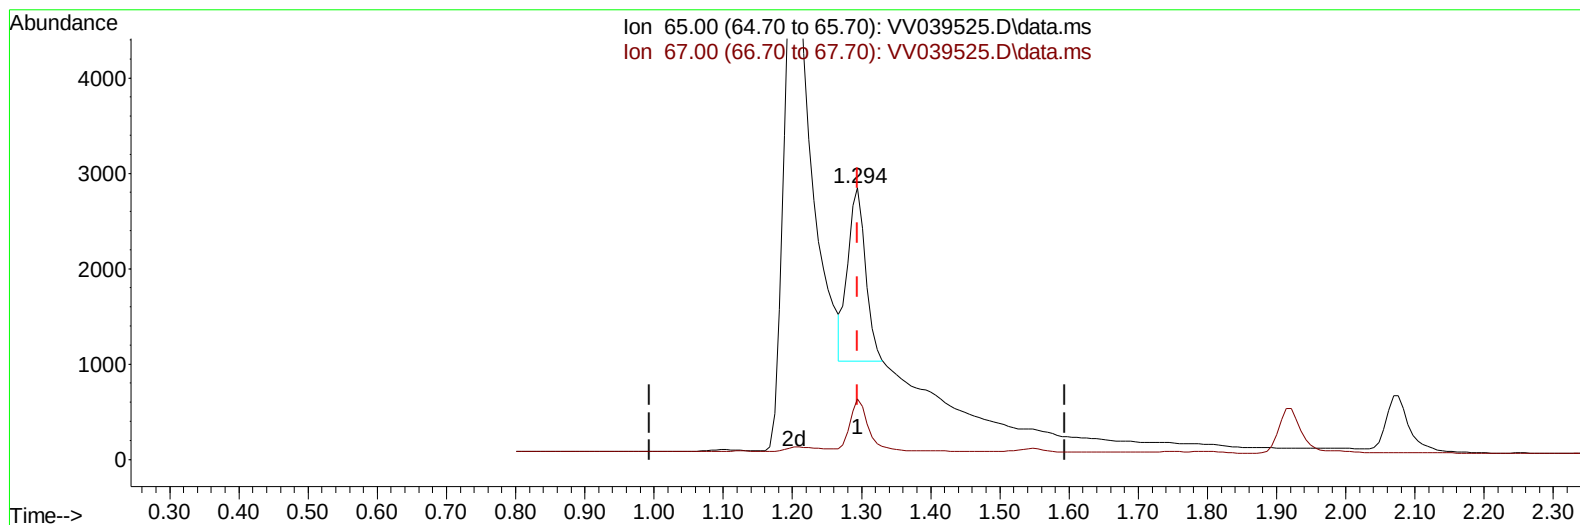

TIC: VV039525.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.294min (+ 0.000) 0.53 ug/L m

response 3249

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	32.90
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
 Data File : VV039525.D
 Acq On : 10 Dec 2025 13:01
 Operator : SY/MD
 Sample : Q3813-02
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BR-04DR-451-120825-SIM

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/11/2025
 Supervised By :Semsettin Yesilyurt 12/12/2025

Quant Time: Dec 11 00:06:30 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 09 08:40:48 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	6208	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	6043	0.500	ug/L	0.02
12) 1,4-Dichlorobenzene-d4	11.197	152	3061	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.294	65	3249m	0.533	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	106.000%		
4) 1,2-Dichloroethane-d4	4.969	65	2014	0.487	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	98.000%		
7) 1,2-Dichloropropane-d6	5.995	67	2050	0.402	ug/L	-0.02
Spiked Amount 0.500	Range 60 - 140		Recovery =	80.000%		
8) Toluene-d8	7.253	98	4098	0.476	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	96.000%		
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1420	0.494	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	98.000%		
Target Compounds						
6) Trichloroethene	5.828	95	61290	8.365	ug/L	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039525.D
Acq On : 10 Dec 2025 13:01
Operator : SY/MD
Sample : Q3813-02
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BR-04DR-451-120825-SIM

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

Quant Time: Dec 11 00:06:30 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

