




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039526.D
Acq On : 10 Dec 2025 13:29
Operator : SY/MD
Sample : Q3813-03
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EB01-120825

Manual IntegrationsAPPROVED

Quant Time: Dec 11 00:06:41 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

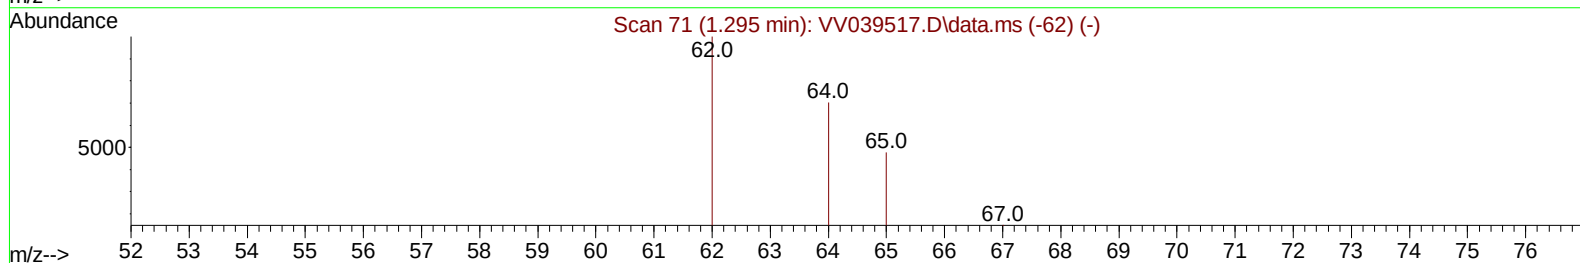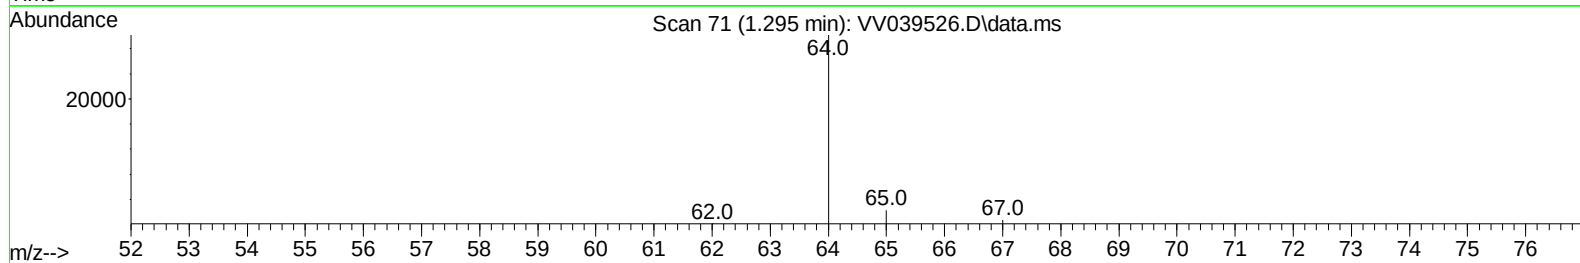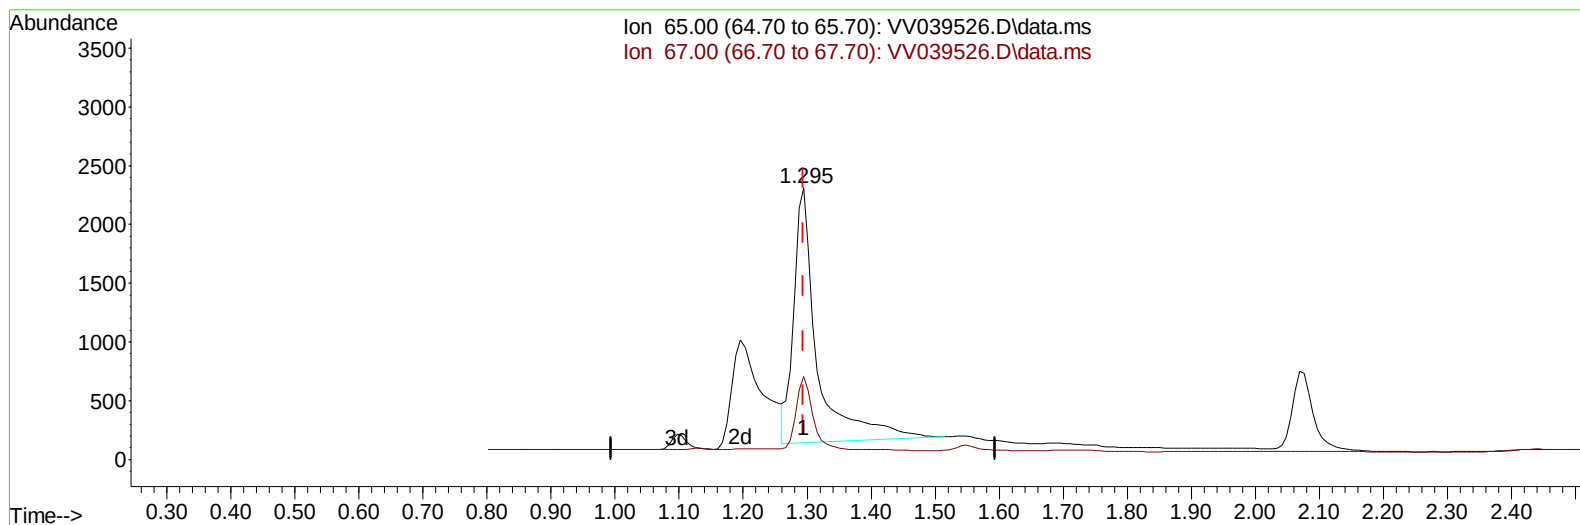

TIC: VV039526.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.295min (+ 0.001) 0.79 ug/L

response 5595

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	19.84#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039526.D
Acq On : 10 Dec 2025 13:29
Operator : SY/MD
Sample : Q3813-03
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EB01-120825

Manual IntegrationsAPPROVED

Quant Time: Dec 11 00:06:41 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

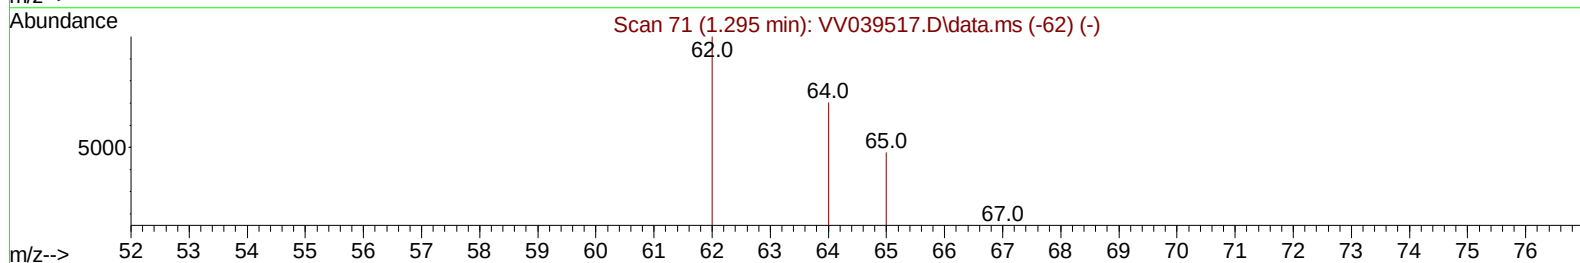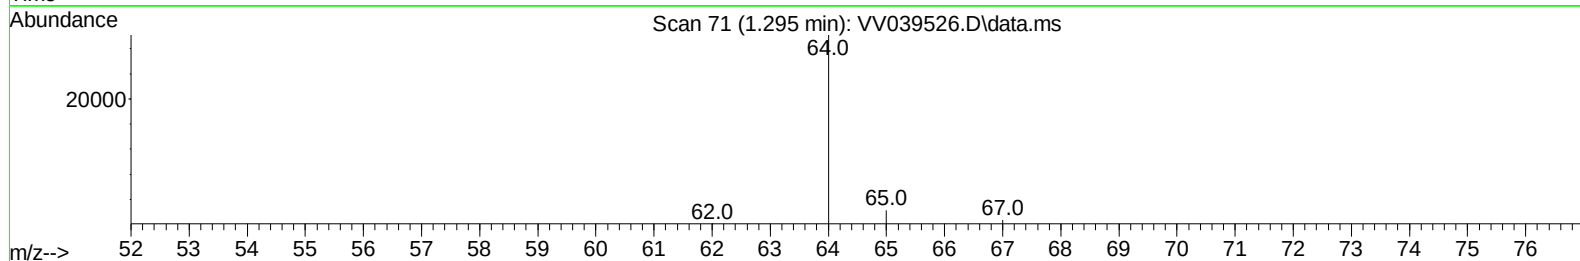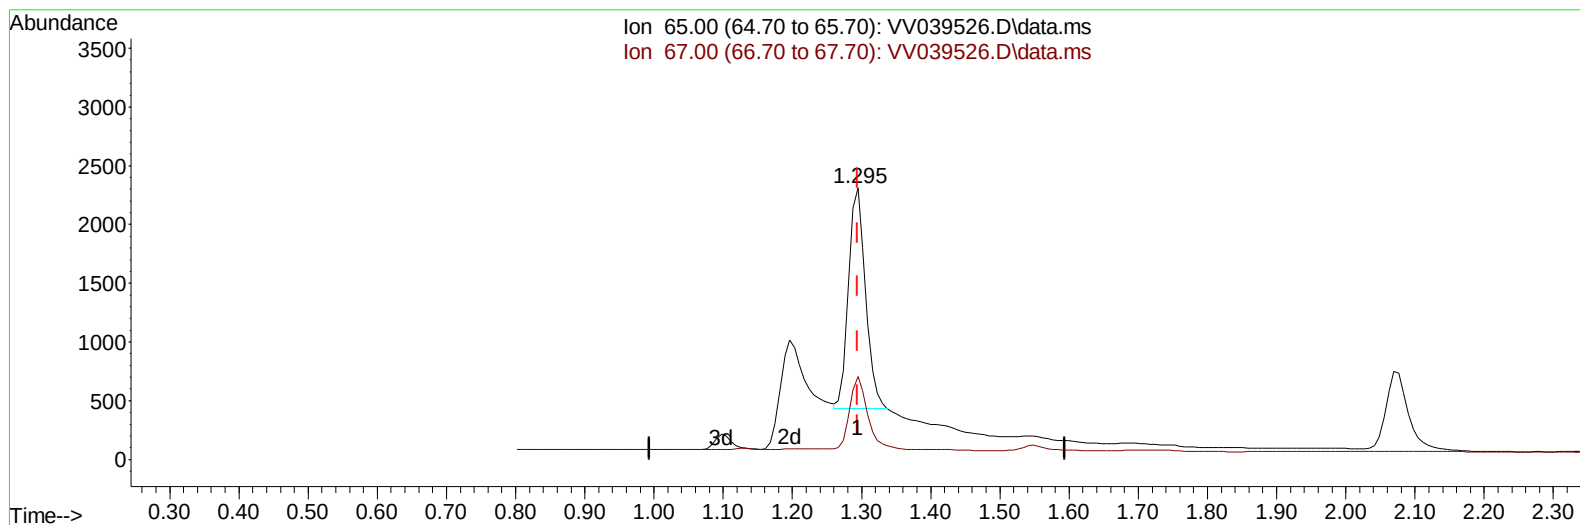

TIC: VV039526.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.295min (+ 0.001) 0.45 ug/L m

response 3185

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	34.85
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
 Data File : VV039526.D
 Acq On : 10 Dec 2025 13:29
 Operator : SY/MD
 Sample : Q3813-03
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EB01-120825

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/11/2025
 Supervised By :Semsettin Yesilyurt 12/12/2025

Quant Time: Dec 11 00:06:41 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 09 08:40:48 2025
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.566	114		7218	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117		6792	0.500	ug/L	0.00
12) 1,4-Dichlorobenzene-d4	11.175	152		3677	0.500	ug/L	0.00
System Monitoring Compounds							
2) Vinyl Chloride-d3	1.295	65		3185m	0.449	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	90.000%	
4) 1,2-Dichloroethane-d4	4.970	65		2013	0.419	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	84.000%	
7) 1,2-Dichloropropane-d6	5.996	67		2321	0.405	ug/L	-0.02
Spiked Amount	0.500	Range	60 - 140	Recovery	=	82.000%	
8) Toluene-d8	7.254	98		4445	0.460	ug/L	0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	92.000%	
10) 1,1,2,2-Tetrachloroeth...	10.133	84		1713	0.530	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	106.000%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039526.D
Acq On : 10 Dec 2025 13:29
Operator : SY/MD
Sample : Q3813-03
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EB01-120825

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

Quant Time: Dec 11 00:06:41 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

