




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039529.D
Acq On : 10 Dec 2025 14:33
Operator : SY/MD
Sample : VIBLK236
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK236

Manual IntegrationsAPPROVED

Quant Time: Dec 11 00:07:15 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

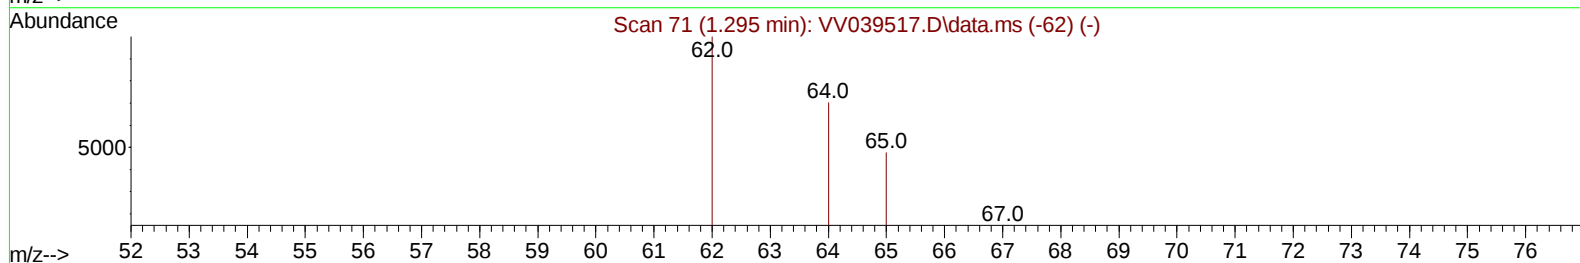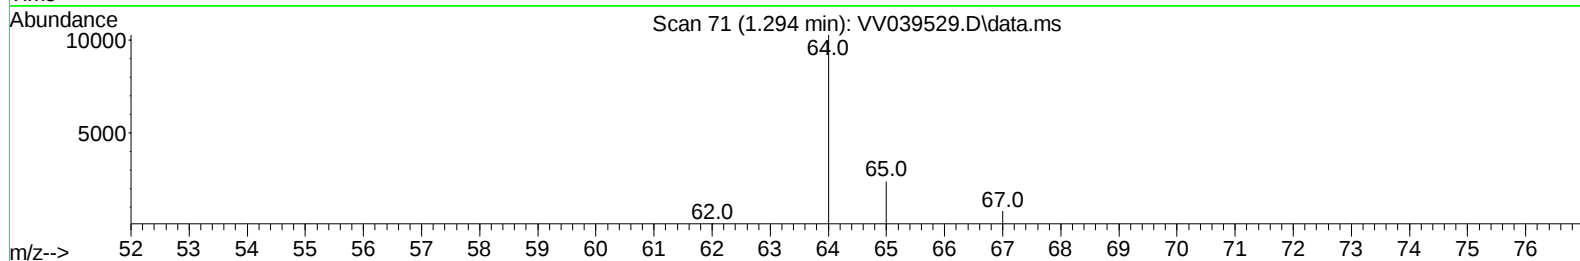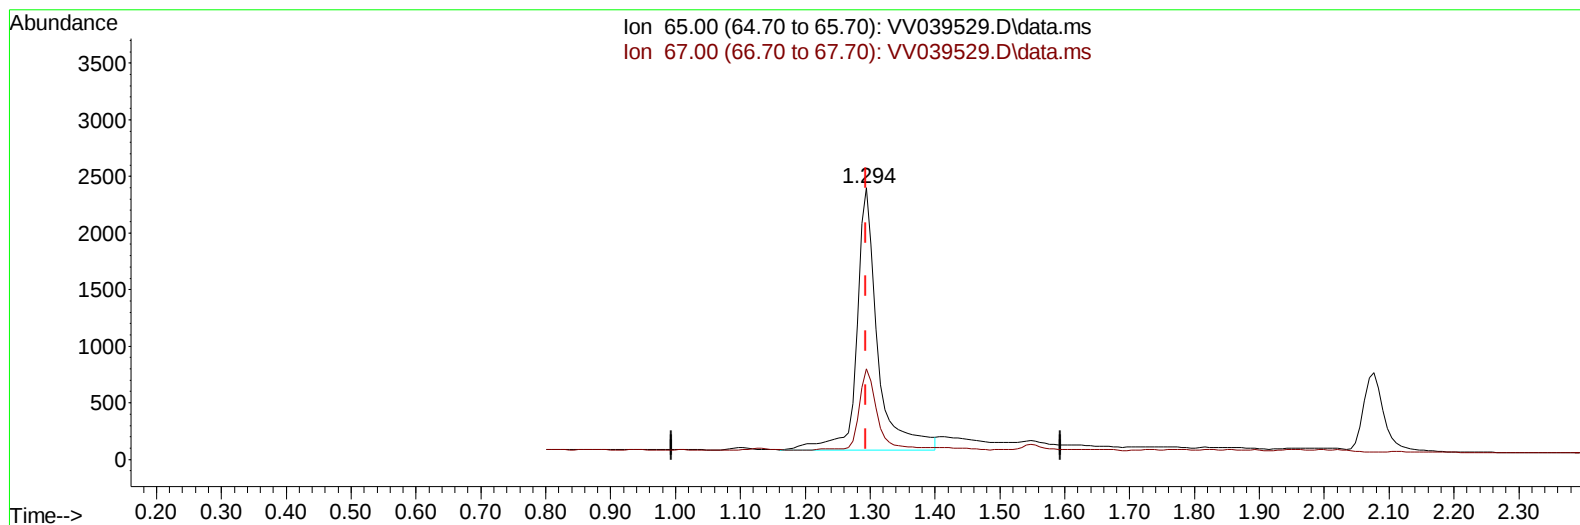

TIC: VV039529.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.294min (+ 0.000) 0.78 ug/L

response 5172

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	26.59
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039529.D
Acq On : 10 Dec 2025 14:33
Operator : SY/MD
Sample : VIBLK236
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK236

Manual IntegrationsAPPROVED

Quant Time: Dec 11 00:07:15 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

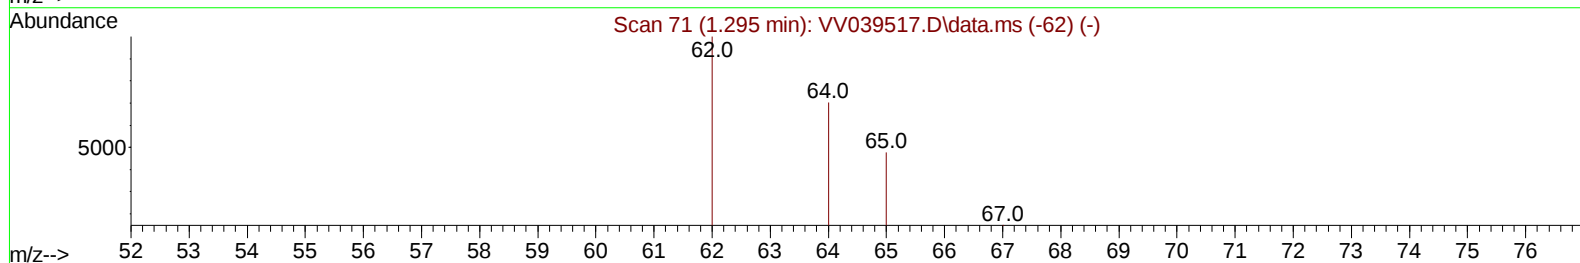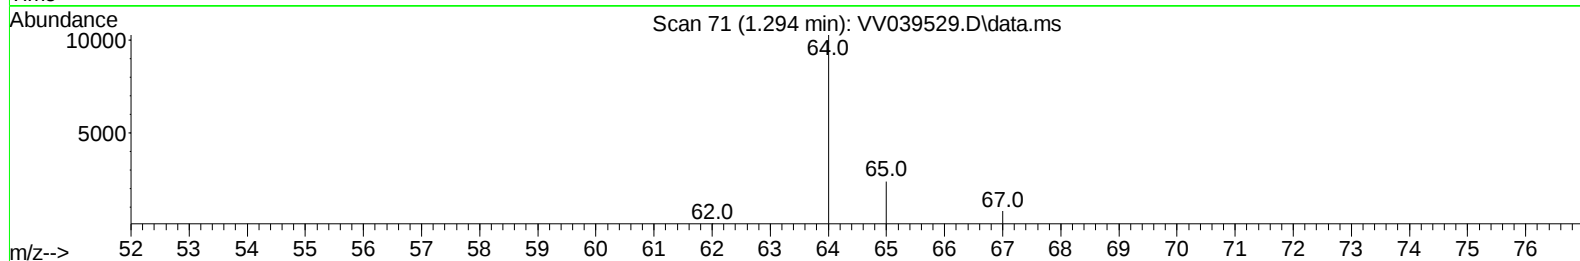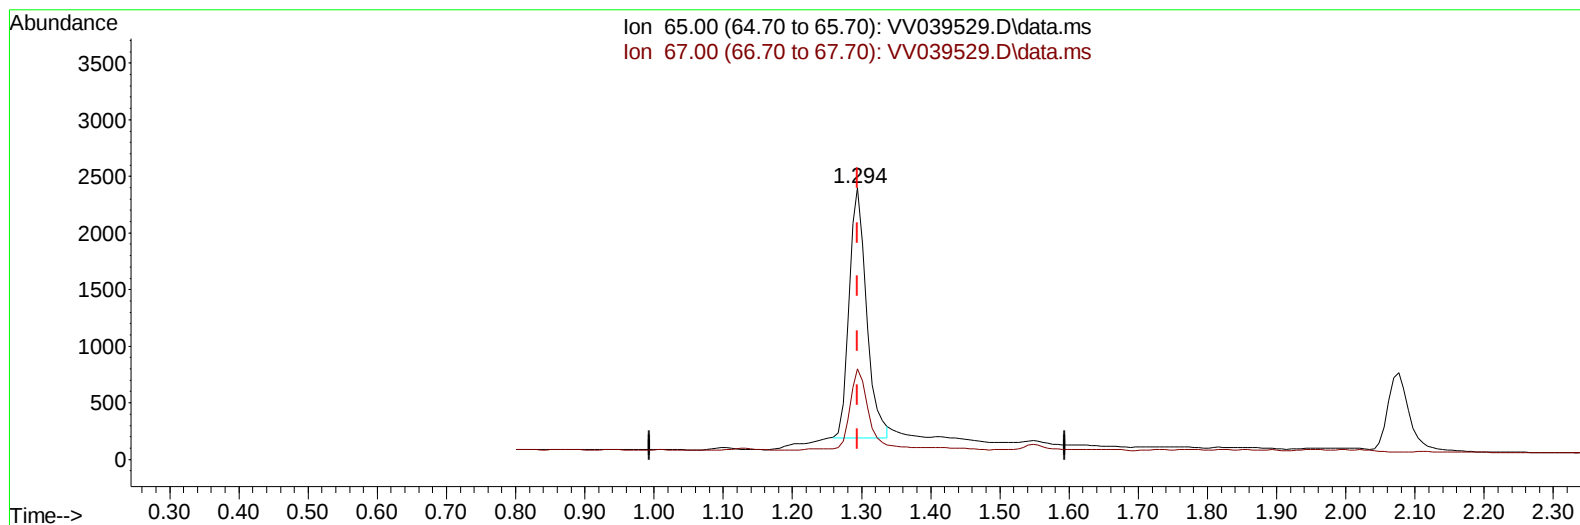

TIC: VV039529.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.294min (+ 0.000) 0.58 ug/L m

response 3858

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	35.64
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
 Data File : VV039529.D
 Acq On : 10 Dec 2025 14:33
 Operator : SY/MD
 Sample : VIBLK236
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK236

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/11/2025
 Supervised By :Semsettin Yesilyurt 12/12/2025

Quant Time: Dec 11 00:07:15 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 09 08:40:48 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	6720	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	6707	0.500	ug/L	0.02
12) 1,4-Dichlorobenzene-d4	11.197	152	3493	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.294	65	3858m	0.585	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	116.000%		
4) 1,2-Dichloroethane-d4	4.970	65	2236	0.500	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	100.000%		
7) 1,2-Dichloropropane-d6	5.996	67	2630	0.465	ug/L	-0.02
Spiked Amount 0.500	Range 60 - 140		Recovery =	92.000%		
8) Toluene-d8	7.254	98	4879	0.511	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	102.000%		
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1965	0.616	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	124.000%#		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039529.D
Acq On : 10 Dec 2025 14:33
Operator : SY/MD
Sample : VIBLK236
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK236

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

Quant Time: Dec 11 00:07:15 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

