




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039530.D
Acq On : 10 Dec 2025 14:54
Operator : SY/MD
Sample : Q3813-05
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Dec 11 00:07:26 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

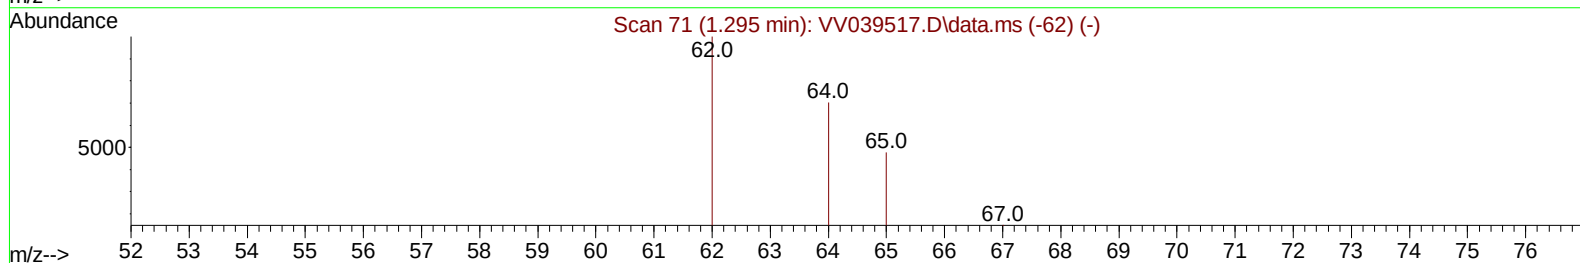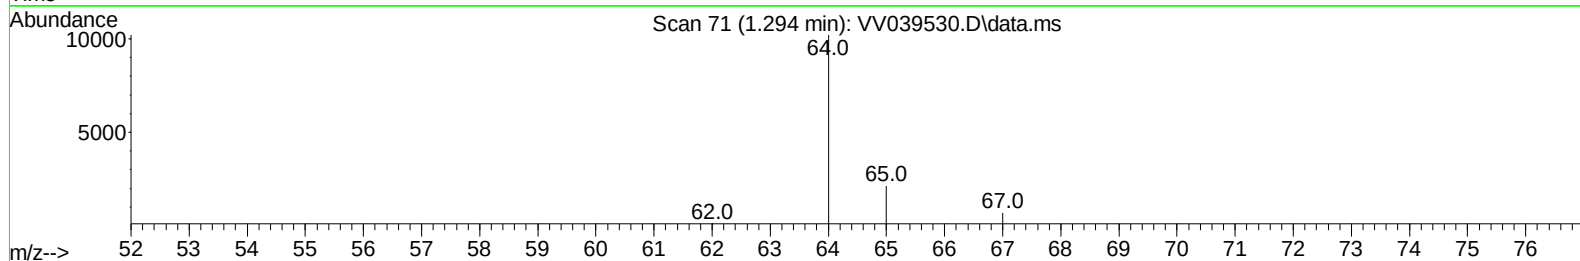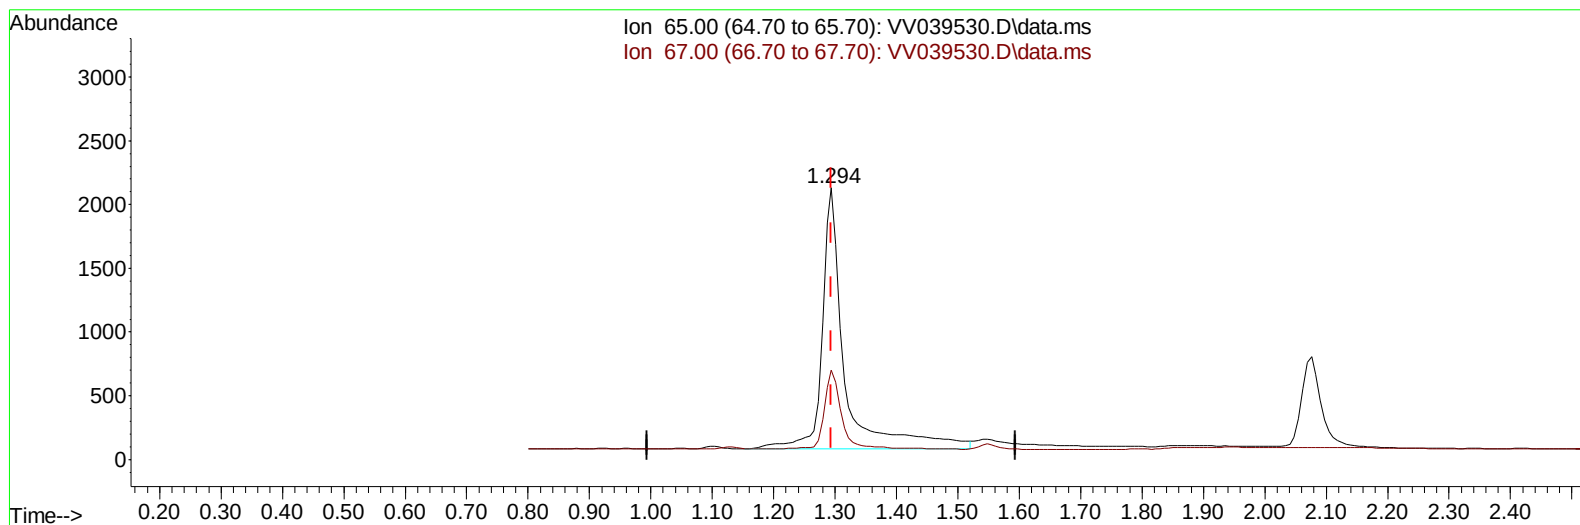

TIC: VV039530.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.294min (+ 0.000) 0.79 ug/L

response 5205

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	22.36
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039530.D
Acq On : 10 Dec 2025 14:54
Operator : SY/MD
Sample : Q3813-05
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Dec 11 00:07:26 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

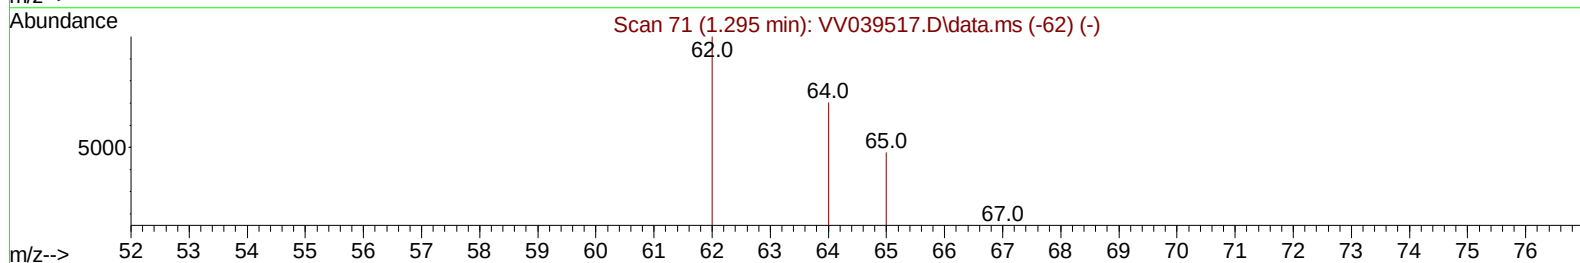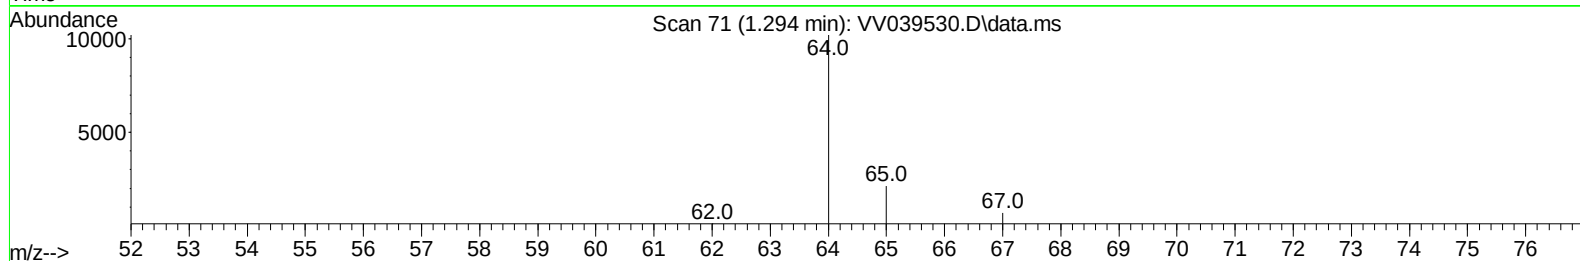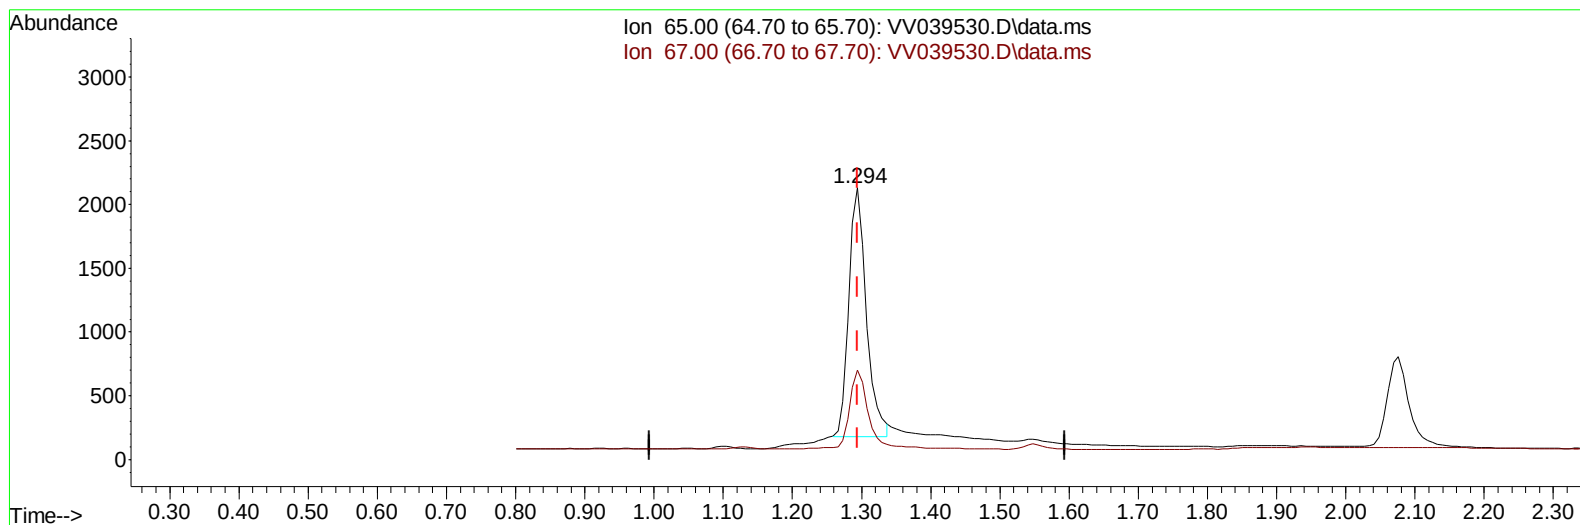

TIC: VV039530.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.294min (+ 0.000) 0.52 ug/L m

response 3429

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	33.95
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
 Data File : VV039530.D
 Acq On : 10 Dec 2025 14:54
 Operator : SY/MD
 Sample : Q3813-05
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/11/2025
 Supervised By :Semsettin Yesilyurt 12/12/2025

Quant Time: Dec 11 00:07:26 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 09 08:40:48 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	6680	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	6693	0.500	ug/L	0.01
12) 1,4-Dichlorobenzene-d4	11.197	152	3533	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.294	65	3429m	0.523	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	104.000%		
4) 1,2-Dichloroethane-d4	4.993	65	2003	0.450	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	90.000%		
7) 1,2-Dichloropropane-d6	5.995	67	2292	0.406	ug/L	-0.02
Spiked Amount 0.500	Range 60 - 140		Recovery =	82.000%		
8) Toluene-d8	7.253	98	4243	0.445	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	90.000%		
10) 1,1,2,2-Tetrachloroeth...	10.132	84	1709	0.537	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	108.000%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039530.D
Acq On : 10 Dec 2025 14:54
Operator : SY/MD
Sample : Q3813-05
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

Quant Time: Dec 11 00:07:26 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

