




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039531.D
Acq On : 10 Dec 2025 15:16
Operator : SY/MD
Sample : Q3788-14
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Dec 11 00:07:37 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

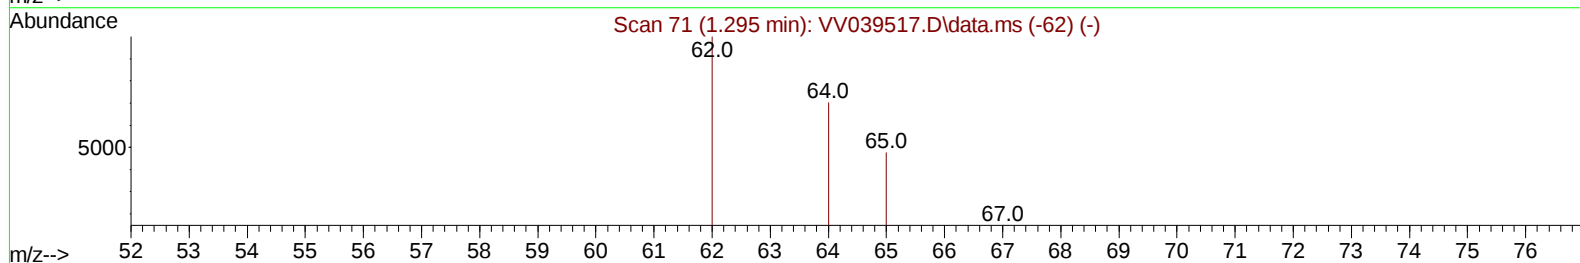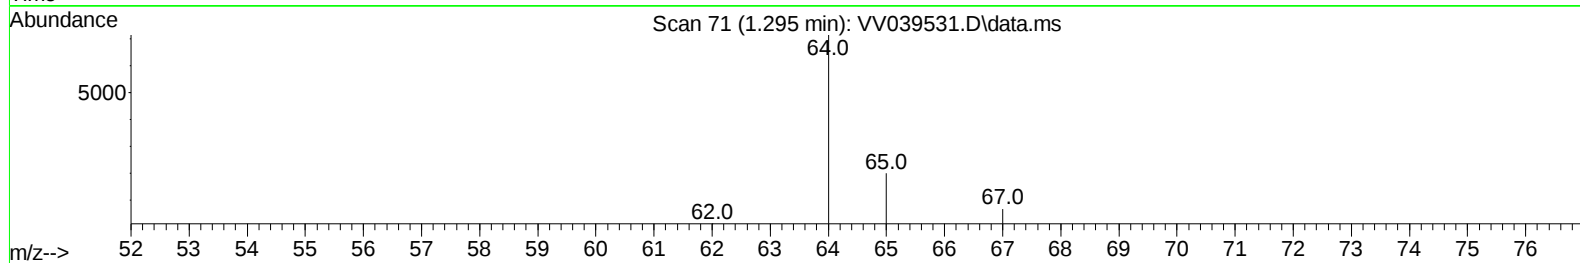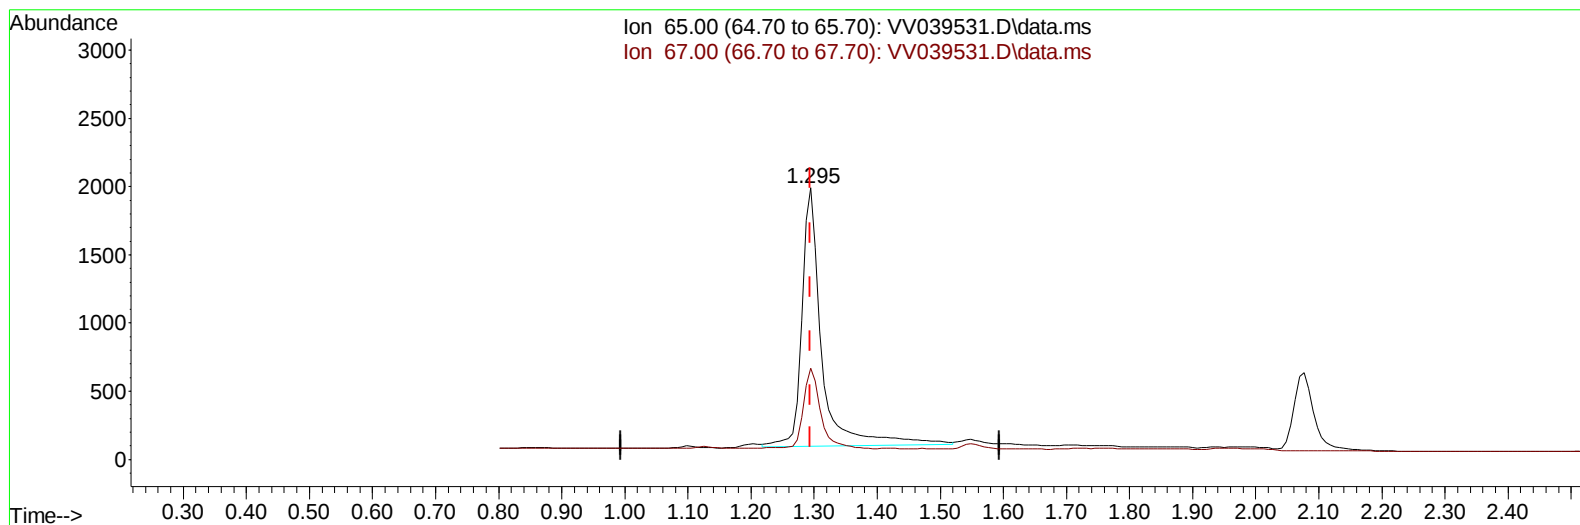

TIC: VV039531.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.295min (+ 0.001) 0.74 ug/L

response 4162

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	26.60
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039531.D
Acq On : 10 Dec 2025 15:16
Operator : SY/MD
Sample : Q3788-14
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Dec 11 00:07:37 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

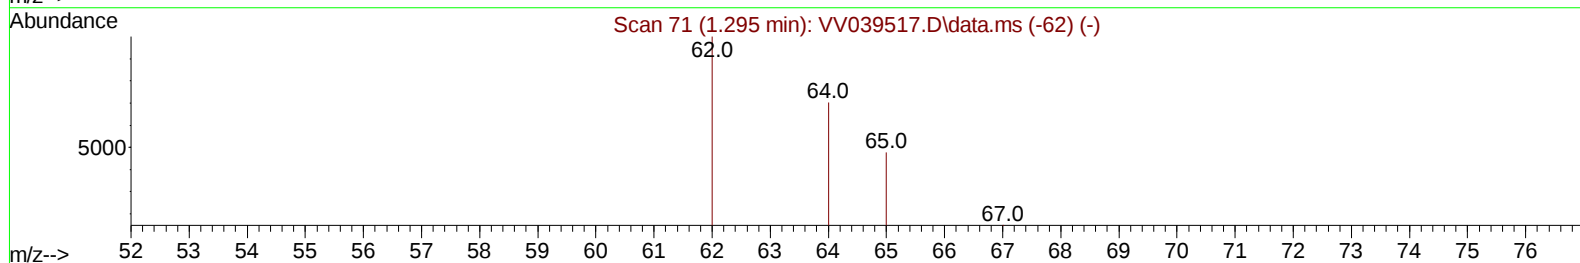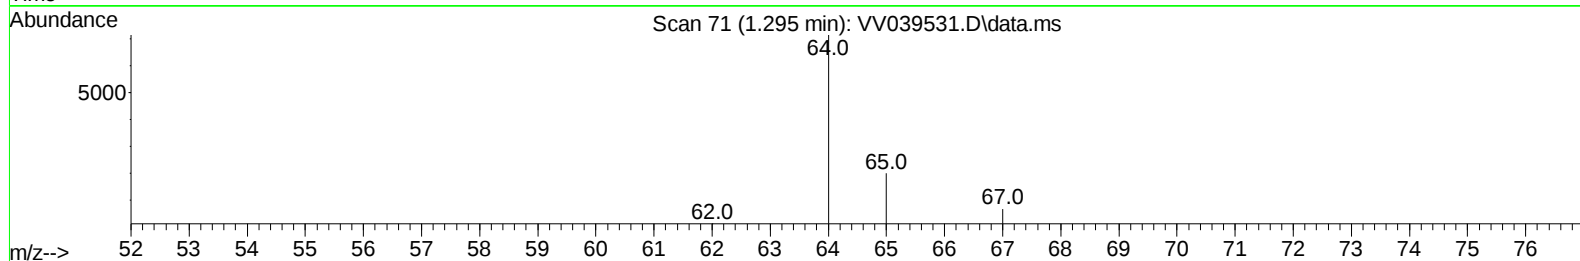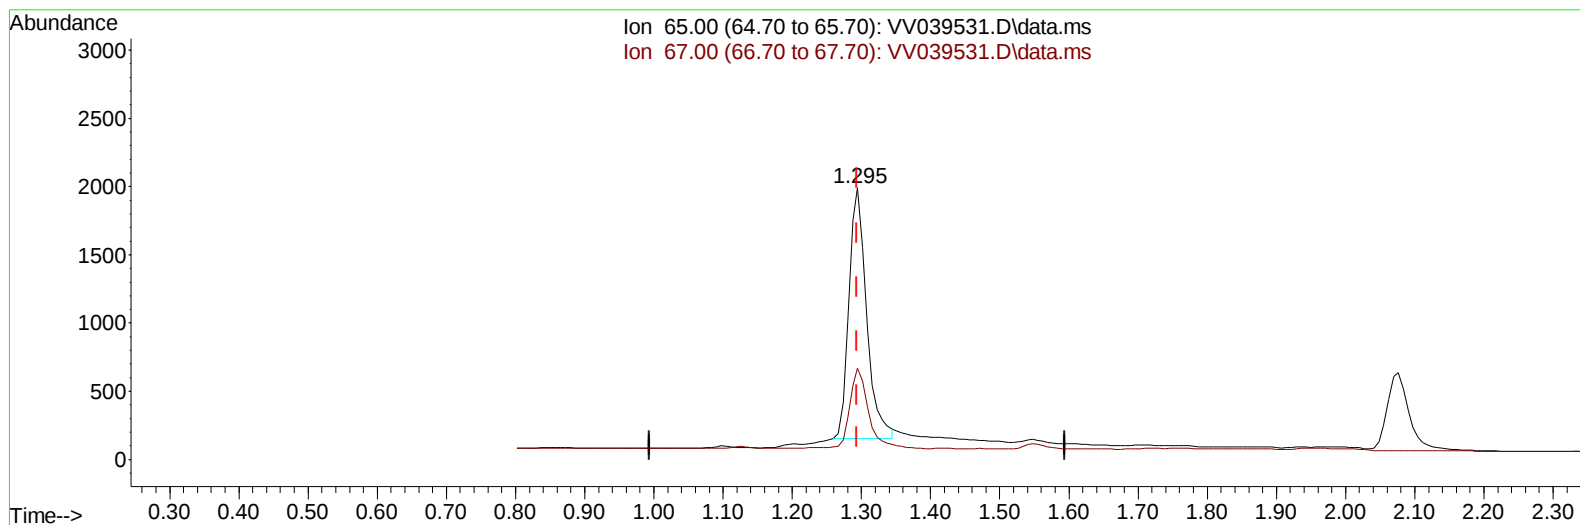

TIC: VV039531.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.295min (+ 0.001) 0.58 ug/L m

response 3269

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	33.86
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
 Data File : VV039531.D
 Acq On : 10 Dec 2025 15:16
 Operator : SY/MD
 Sample : Q3788-14
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/11/2025
 Supervised By :Semsettin Yesilyurt 12/12/2025

Quant Time: Dec 11 00:07:37 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 09 08:40:48 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5732	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	5821	0.500	ug/L	0.02
12) 1,4-Dichlorobenzene-d4	11.198	152	2993	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.295	65	3269m	0.581	ug/L	0.00
Spiked Amount	0.500	Range 40 - 130	Recovery	=	116.000%	
4) 1,2-Dichloroethane-d4	4.994	65	1880	0.493	ug/L	0.02
Spiked Amount	0.500	Range 70 - 130	Recovery	=	98.000%	
7) 1,2-Dichloropropane-d6	5.996	67	2195	0.447	ug/L	-0.02
Spiked Amount	0.500	Range 60 - 140	Recovery	=	90.000%	
8) Toluene-d8	7.254	98	4025	0.486	ug/L	0.02
Spiked Amount	0.500	Range 70 - 130	Recovery	=	98.000%	
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1606	0.580	ug/L	0.00
Spiked Amount	0.500	Range 65 - 120	Recovery	=	116.000%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121025\
Data File : VV039531.D
Acq On : 10 Dec 2025 15:16
Operator : SY/MD
Sample : Q3788-14
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/11/2025
Supervised By :Semsettin Yesilyurt 12/12/2025

Quant Time: Dec 11 00:07:37 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

