


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121118\
Data File : VV008890.D
Acq On : 11 Dec 2018 09:18
Operator : SY/MD
Sample : BFB58
Misc : 5.00g/10.0mL/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB58

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M
Title : VOC Analysis
Last Update : Wed Dec 12 04:31:38 2018

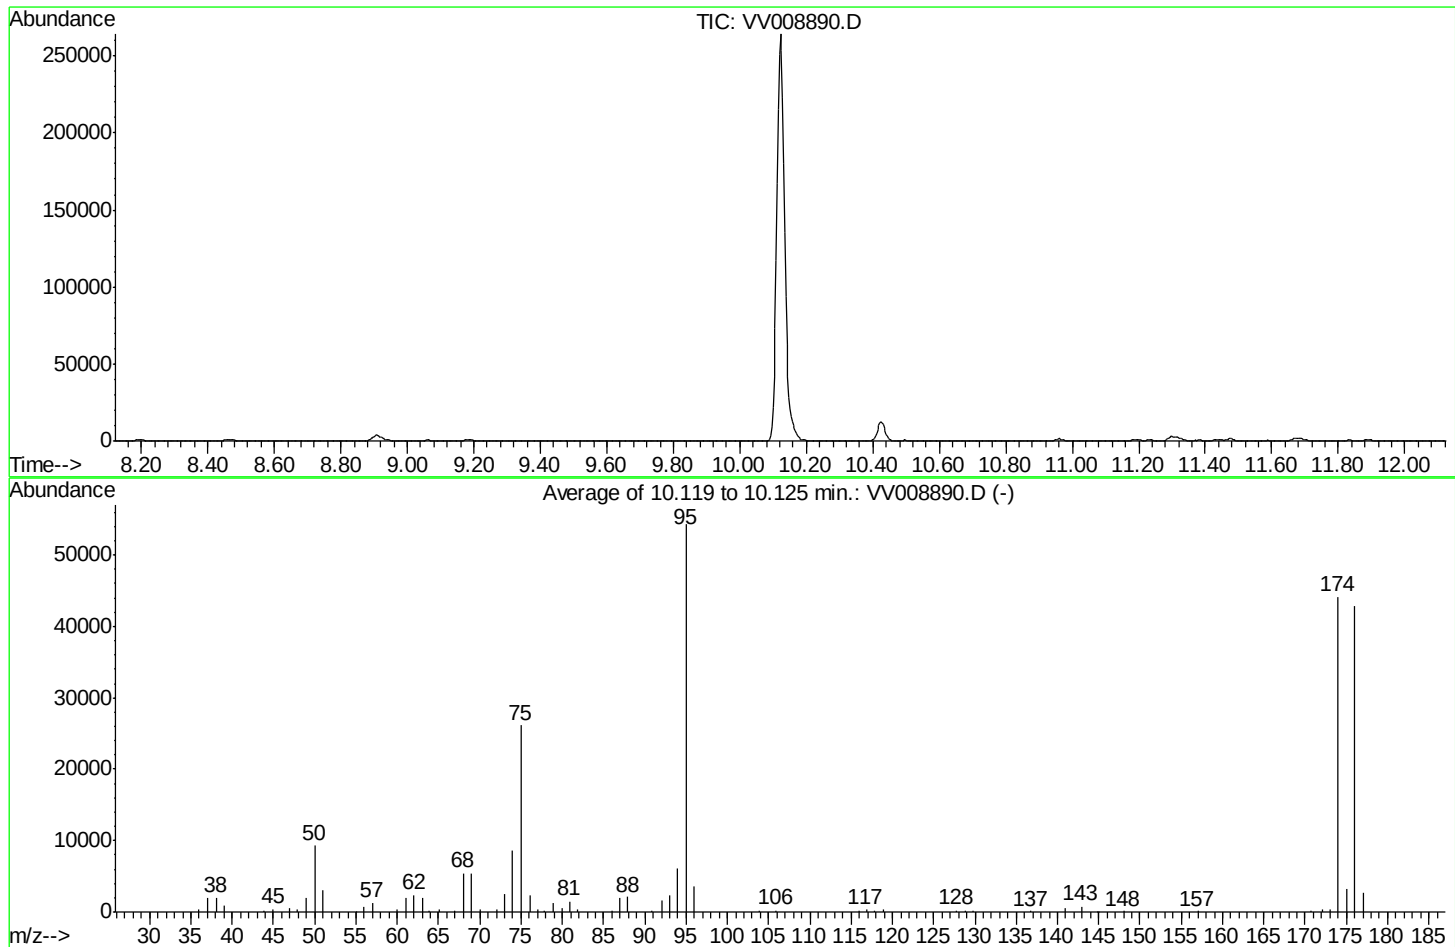

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	9281	PASS
75	95	30	80	48.1	26101	PASS
95	95	100	100	100.0	54288	PASS
96	95	5	9	6.6	3580	PASS
173	174	0.00	2	0.9	409	PASS
174	95	50	120	81.2	44104	PASS
175	174	5	9	7.5	3293	PASS
176	174	95	101	97.2	42882	PASS
177	176	5	9	6.4	2753	PASS

m/z	Abundance
35.90	432.0
37.00	2014.0
38.00	2075.0
39.00	841.0
43.90	423.0
45.00	433.0
47.00	534.0
47.80	317.0
49.00	2034.0
50.00	9361.0
51.00	3087.0
55.10	101.0
56.00	675.0
57.00	1237.0
59.90	357.0
61.00	2056.0
62.00	2340.0
63.00	1921.0
63.90	221.0
65.10	276.0
66.90	128.0
68.00	5014.0
69.00	5206.0
70.00	397.0
72.00	336.0
73.00	2548.0
74.00	8442.0
75.00	25664.0
76.10	2318.0
77.00	388.0
77.80	157.0
78.90	1322.0
79.90	520.0
80.90	1496.0
81.90	406.0
86.10	125.0
87.00	1929.0
87.90	2150.0
90.90	237.0
92.00	1730.0
93.00	2476.0
94.00	5963.0
95.00	53384.0
96.00	3565.0
103.90	183.0
105.90	265.0
115.90	133.0
116.80	332.0
117.80	263.0
119.00	337.0
127.80	179.0
128.90	116.0
129.80	178.0
136.80	136.0
140.90	619.0
142.90	695.0
144.80	159.0
147.90	132.0
170.80	115.0
172.00	430.0
173.00	588.0
174.00	42016.0
175.00	3194.0
176.00	41240.0
177.00	2693.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

m/z	Abundance
43.90	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

m/z	Abundance
35.90	332.0
37.00	1877.0
38.10	1850.0
39.00	784.0
43.90	356.0
45.00	306.0
47.00	556.0
47.80	249.0
49.00	1985.0
50.00	8917.0
51.00	2892.0
54.90	117.0
56.00	677.0
57.00	1330.0
60.00	368.0
61.00	1998.0
62.00	2303.0
63.00	1817.0
63.80	230.0
65.10	321.0
67.00	138.0
68.00	5541.0
69.00	5343.0
70.00	382.0
72.00	280.0
73.00	2255.0
74.00	8311.0
75.00	25832.0
76.00	2396.0
77.00	275.0
77.90	146.0
78.90	1240.0
79.90	563.0
80.90	1507.0
81.90	404.0
86.00	133.0
87.00	1791.0
87.90	2037.0
90.90	232.0
92.00	1532.0
93.00	2242.0
94.00	5960.0
95.00	53616.0
96.00	3489.0
103.90	268.0
105.90	230.0
115.90	156.0
116.90	319.0
117.90	176.0
118.80	313.0
127.80	241.0
128.90	108.0
129.80	165.0
136.80	130.0
140.90	614.0
143.00	754.0
145.00	133.0
148.10	117.0
157.00	151.0
170.70	107.0
172.10	433.0
174.00	44760.0
175.00	3276.0
176.00	43280.0
177.00	2736.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

m/z	Abundance
35.00	407.0
37.00	2048.0
38.00	2089.0
39.00	871.0
43.00	388.0
45.00	384.0
47.00	574.0
47.80	305.0
49.00	2143.0
50.00	9565.0
51.00	3173.0
56.00	709.0
57.00	1349.0
60.00	380.0
61.00	2103.0
62.00	2409.0
63.00	1991.0
63.90	241.0
65.10	307.0
66.90	131.0
68.00	5683.0
69.00	5515.0
70.00	385.0
72.00	331.0
73.00	2548.0
74.00	8885.0
75.00	26808.0
76.00	2459.0
77.00	368.0
77.80	156.0
78.90	1347.0
79.90	615.0
80.90	1560.0
81.90	425.0
86.00	171.0
87.00	1969.0
88.00	2243.0
90.90	238.0
92.00	1667.0
93.00	2497.0
94.00	6216.0
95.00	55864.0
96.00	3687.0
103.90	229.0
105.90	257.0
115.90	154.0
116.90	336.0
117.80	229.0
118.80	329.0
127.80	230.0
128.90	118.0
129.80	182.0
136.80	140.0
140.90	629.0
143.00	745.0
145.00	153.0
148.00	114.0
157.00	143.0
170.80	129.0
172.00	425.0
173.00	639.0
174.00	45536.0
175.00	3411.0
176.00	44128.0
177.00	2831.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58