

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121119\
 Data File : VV014011.D
 Acq On : 11 Dec 2019 14:38
 Operator : SY/MD
 Sample : K6202-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Dec 12 03:32:21 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 12 03:01:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	582476	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	578612	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	244383	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	186015	55.22	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	110.44%
7) Chloroethane-d5	1.56	69	195676	55.65	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	111.30%
11) 1,1-Dichloroethene-d2	2.12	63	296913	39.86	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.72%
21) 2-Butanone-d5	3.92	46	218504	92.15	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.15%
24) Chloroform-d	4.39	84	350331	49.52	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.04%
26) 1,2-Dichloroethane-d4	5.07	65	221635	49.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.88%
32) Benzene-d6	5.09	84	714847	47.68	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.36%
36) 1,2-Dichloropropane-d6	6.11	67	225335	50.07	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.14%
41) Toluene-d8	7.35	98	642836	47.03	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.06%
43) trans-1,3-Dichloropropene-	7.66	79	93271	42.59	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.18%
47) 2-Hexanone-d5	8.13	63	125296	74.56	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	74.56%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	290540	44.58	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.16%
64) 1,2-Dichlorobenzene-d4	11.67	152	265780	55.37	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	110.74%


Target Compounds					Ovalue
13) Acetone	2.19	43	8465	2.436 ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121119\
Data File : VV014011.D
Acq On : 11 Dec 2019 14:38
Operator : SY/MD
Sample : K6202-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Dec 12 03:32:21 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 12 03:01:11 2019
Response via : Initial Calibration

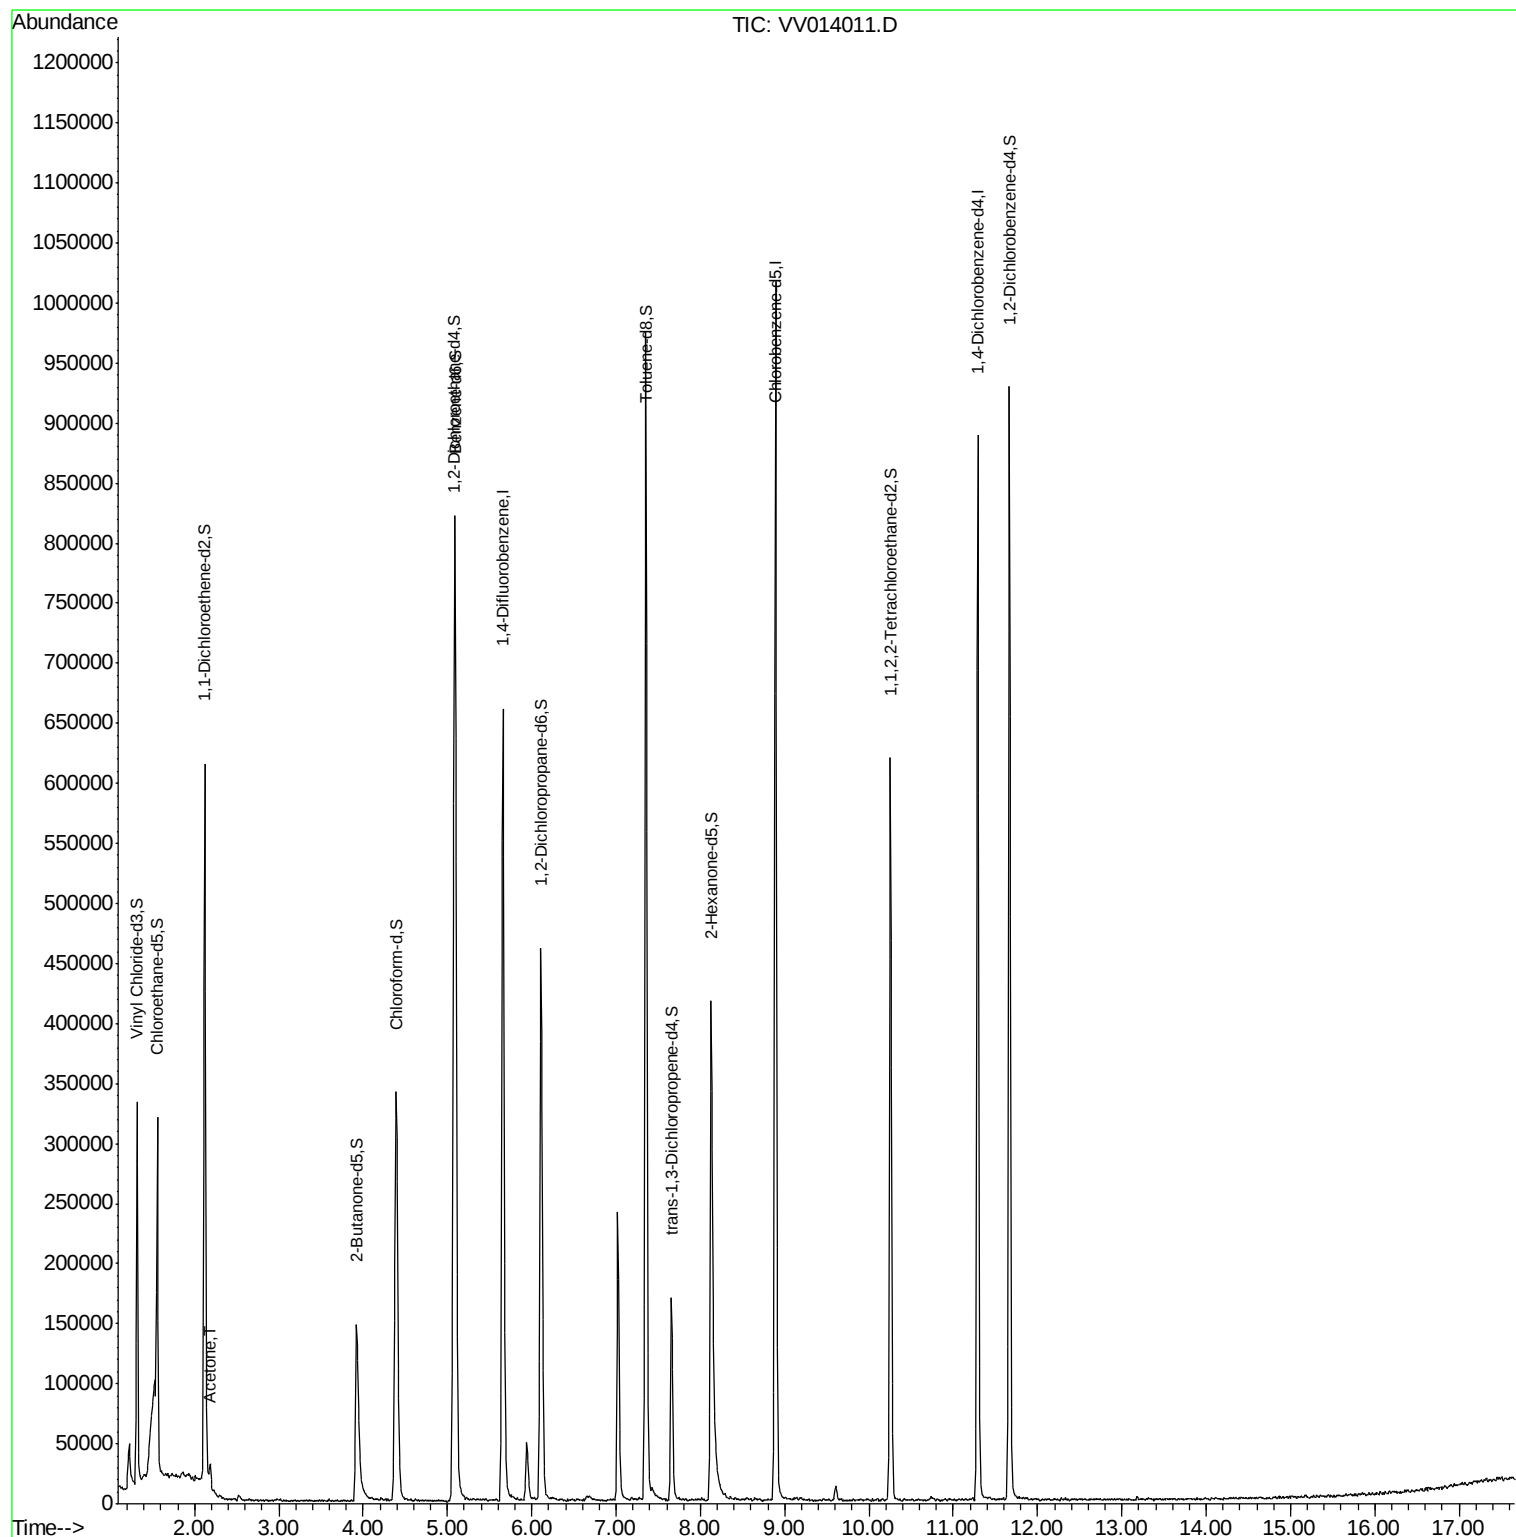

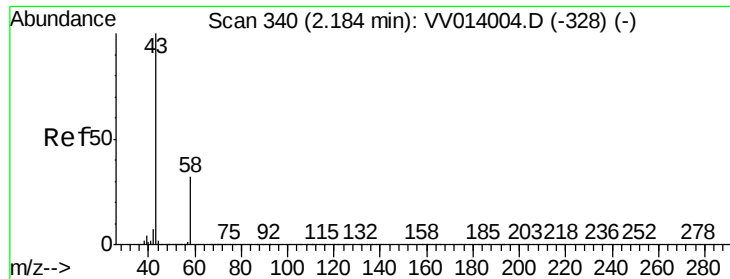

#13

Acetone

Concen: 2.436 ug/L

RT: 2.19 min Scan# 341

Delta R.T. 0.00 min

Lab File: VV014011.D

Acq: 11 Dec 2019 14:38

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Tot Ion: 43 Resp: 8465

Ion Ratio Lower Upper

43 100

58 19.5 0.0 60.8

