

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121119\
 Data File : VV014023.D
 Acq On : 11 Dec 2019 20:22
 Operator : SY/MD
 Sample : K6308-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C44

Quant Time: Dec 12 04:28:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 12 03:01:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	746327	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	711382	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	274511	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	194857	45.14	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	90.28%
7) Chloroethane-d5	1.56	69	205443	45.60	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.20%
11) 1,1-Dichloroethene-d2	2.12	63	315782	33.08	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.16%
21) 2-Butanone-d5	3.92	46	294844	97.05	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.05%
24) Chloroform-d	4.39	84	442266	48.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.58%
26) 1,2-Dichloroethane-d4	5.07	65	280785	48.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.76%
32) Benzene-d6	5.09	84	902109	48.94	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.88%
36) 1,2-Dichloropropane-d6	6.11	67	286632	51.80	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.60%
41) Toluene-d8	7.36	98	764528	45.49	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.98%
43) trans-1,3-Dichloropropene-	7.66	79	113482	42.15	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.30%
47) 2-Hexanone-d5	8.13	63	160175	77.52	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	77.52%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	341825	42.66	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.32%
64) 1,2-Dichlorobenzene-d4	11.67	152	284458	52.76	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.52%


Target Compounds					Ovalue
13) Acetone	2.19	43	7136	1.603 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121119\
Data File : VV014023.D
Acq On : 11 Dec 2019 20:22
Operator : SY/MD
Sample : K6308-15
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C44

Quant Time: Dec 12 04:28:56 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 12 03:01:11 2019
Response via : Initial Calibration

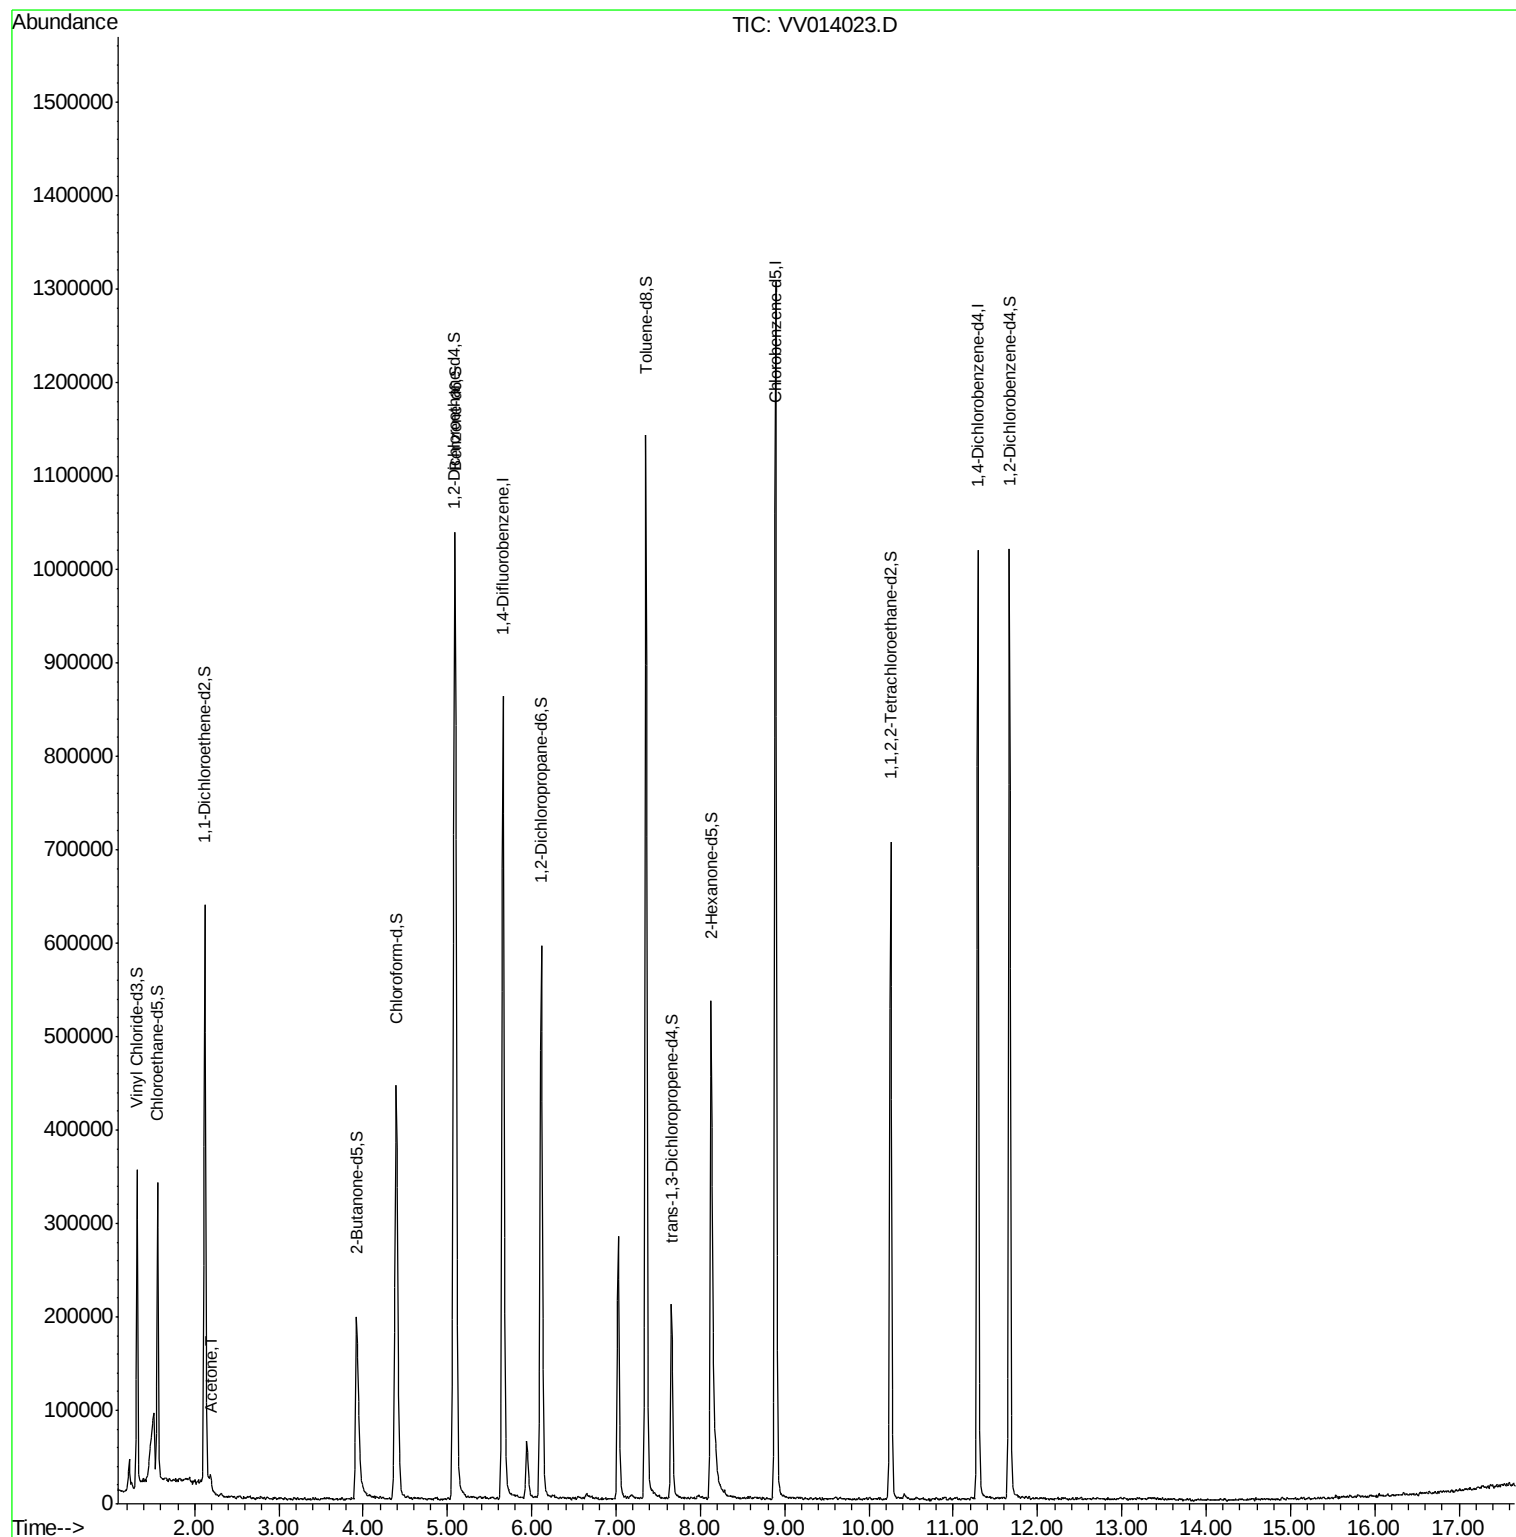

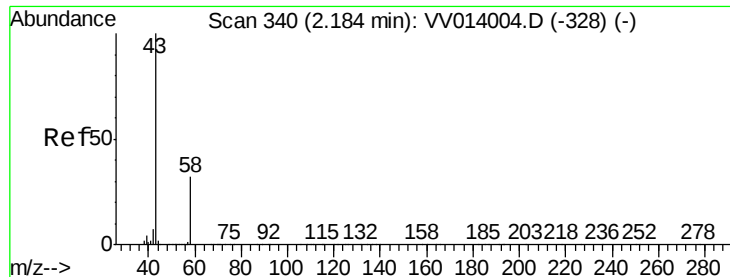

#13

Acetone

Concen: 1.603 ug/L

RT: 2.19 min Scan# 341

Delta R.T. 0.00 min

Lab File: VV014023.D

Acq: 11 Dec 2019 20:22

Instrument :
MSVOA_V
ClientSampleId :
C0C44

Tot Ion: 43 Resp: 7136

Ion Ratio Lower Upper

43 100

58 36.9 0.0 60.8

