

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121119\
 Data File : VV014017.D
 Acq On : 11 Dec 2019 17:54
 Operator : SY/MD
 Sample : K6200-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	81	rVB	316347	307060	12.67%	1.815%
2	1.560	140	146	158	rVB	304863	358430	14.79%	2.118%
3	2.122	313	321	335	rVB	588850	814884	33.63%	4.815%
4	3.164	643	645	646	rBV2	1176	486	0.02%	0.003%
5	3.261	673	675	678	rBV4	1113	829	0.03%	0.005%
6	3.328	693	696	699	rBV5	1404	1110	0.05%	0.007%
7	3.923	870	881	912	rBV	170375	483214	19.94%	2.855%
8	4.392	1013	1027	1050	rBV	407320	968548	39.97%	5.723%
9	5.090	1225	1244	1273	rBV2	966209	2423356	100.00%	14.320%
10	5.659	1408	1421	1447	rBV	802834	1574515	64.97%	9.304%
11	6.113	1550	1562	1588	rVB	559571	1123860	46.38%	6.641%
12	7.026	1835	1846	1868	rBV	246080	444509	18.34%	2.627%
13	7.354	1937	1948	1967	rBV	978527	1683810	69.48%	9.950%
14	7.659	2034	2043	2065	rBV	174411	288074	11.89%	1.702%
15	8.132	2178	2190	2228	rBV3	452702	1028617	42.45%	6.078%
16	8.447	2285	2288	2290	rBV3	1465	961	0.04%	0.006%
17	8.807	2398	2400	2401	rVB2	775	189	0.01%	0.001%
18	8.820	2401	2404	2406	rBV4	1395	698	0.03%	0.004%
19	8.891	2414	2426	2444	rBV	1019663	1633270	67.40%	9.651%
20	9.113	2493	2495	2498	rBV3	1493	1161	0.05%	0.007%
21	9.135	2498	2502	2503	rBV3	3413	2365	0.10%	0.014%
22	9.476	2605	2608	2610	rBV3	893	379	0.02%	0.002%
23	9.489	2610	2612	2615	rBV3	1664	1088	0.04%	0.006%
24	9.540	2624	2628	2631	rBV5	1320	1180	0.05%	0.007%
25	9.553	2631	2632	2634	rBV2	948	372	0.02%	0.002%
26	9.704	2673	2679	2682	rBV6	2881	3669	0.15%	0.022%
27	10.055	2784	2788	2790	rBV3	2784	1993	0.08%	0.012%
28	10.257	2837	2851	2868	rBV	703290	1119428	46.19%	6.615%
29	10.405	2893	2897	2898	rBV4	2466	1681	0.07%	0.010%
30	10.887	3043	3047	3051	rVB8	3414	2496	0.10%	0.015%
31	11.103	3109	3114	3117	rBV6	2325	2275	0.09%	0.013%
32	11.222	3144	3151	3160	rBV6	4206	7254	0.30%	0.043%
33	11.289	3161	3172	3191	rBV	838765	1274250	52.58%	7.530%
34	11.485	3231	3233	3237	rBV3	1303	939	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121119\
 Data File : VV014017.D
 Acq On : 11 Dec 2019 17:54
 Operator : SY/MD
 Sample : K6200-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	11.553	3249	3254	3257	rBV6	2031	2390	0.10%	0.014%
36	11.579	3260	3262	3263	rBV2	1104	435	0.02%	0.003%
37	11.665	3277	3289	3308	rBV	820456	1310339	54.07%	7.743%
38	12.013	3395	3397	3399	rBV2	933	545	0.02%	0.003%
39	12.055	3407	3410	3411	rBV2	1002	482	0.02%	0.003%
40	12.090	3418	3421	3422	rBV3	1107	476	0.02%	0.003%
41	12.112	3427	3428	3430	rBV	785	269	0.01%	0.002%
42	12.125	3430	3432	3433	rBV2	968	344	0.01%	0.002%
43	12.193	3449	3453	3456	rBV4	1473	938	0.04%	0.006%
44	12.283	3479	3481	3484	rBV3	1381	797	0.03%	0.005%
45	12.331	3494	3496	3498	rBV3	961	474	0.02%	0.003%
46	12.389	3513	3514	3516	rBV2	991	311	0.01%	0.002%
47	12.482	3540	3543	3544	rBV2	1204	616	0.03%	0.004%
48	12.563	3566	3568	3570	rBV2	721	362	0.01%	0.002%
49	12.620	3584	3586	3589	rVB2	1047	533	0.02%	0.003%
50	12.643	3589	3593	3596	rBV4	843	608	0.03%	0.004%
51	12.688	3600	3607	3613	rBV7	5284	8303	0.34%	0.049%
52	12.746	3623	3625	3629	rBV4	815	432	0.02%	0.003%
53	12.800	3639	3642	3644	rBV2	1318	1014	0.04%	0.006%
54	12.900	3669	3673	3675	rVB4	1078	699	0.03%	0.004%
55	12.916	3677	3678	3679	rVB	466	90	0.00%	0.001%
56	12.932	3681	3683	3684	rBV3	843	394	0.02%	0.002%
57	12.952	3684	3689	3691	rBV3	1040	856	0.04%	0.005%
58	13.006	3704	3706	3708	rVB3	1274	490	0.02%	0.003%
59	13.022	3708	3711	3713	rBV4	844	471	0.02%	0.003%
60	13.045	3715	3718	3720	rVV3	1200	665	0.03%	0.004%
61	13.074	3725	3727	3729	rVB3	1215	420	0.02%	0.002%
62	13.087	3729	3731	3736	rBV3	641	421	0.02%	0.002%
63	13.270	3784	3788	3790	rBV5	1145	806	0.03%	0.005%
64	13.373	3816	3820	3823	rBV5	1911	1554	0.06%	0.009%
65	13.421	3833	3835	3840	rVB3	1173	615	0.03%	0.004%
66	13.444	3840	3842	3847	rBV5	1176	908	0.04%	0.005%
67	13.482	3852	3854	3855	rBV	765	416	0.02%	0.002%
68	13.492	3855	3857	3861	rVB5	1105	636	0.03%	0.004%
69	13.514	3861	3864	3868	rBV4	1117	691	0.03%	0.004%
70	13.559	3869	3878	3890	rBV3	8373	16807	0.69%	0.099%
71	13.659	3906	3909	3913	rBV4	1826	1571	0.06%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121119\
Data File : VV014017.D
Acq On : 11 Dec 2019 17:54
Operator : SY/MD
Sample : K6200-12
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF40

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Title : VOC Analysis

72	13.765	3940	3942	3943	rBV	1073	332	0.01%	0.002%
73	13.842	3964	3966	3970	rVB3	1116	416	0.02%	0.002%
74	13.862	3970	3972	3975	rVB2	1832	902	0.04%	0.005%
75	13.894	3975	3982	3985	rBV7	1839	2315	0.10%	0.014%
76	13.948	3997	3999	4000	rBV2	1121	618	0.03%	0.004%
77	14.251	4091	4093	4094	rBV2	1188	467	0.02%	0.003%
78	14.315	4105	4113	4115	rBV3	2377	2277	0.09%	0.013%


Sum of corrected areas: 16922455

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121119\
Data File : VV014017.D
Acq On : 11 Dec 2019 17:54
Operator : SY/MD
Sample : K6200-12
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

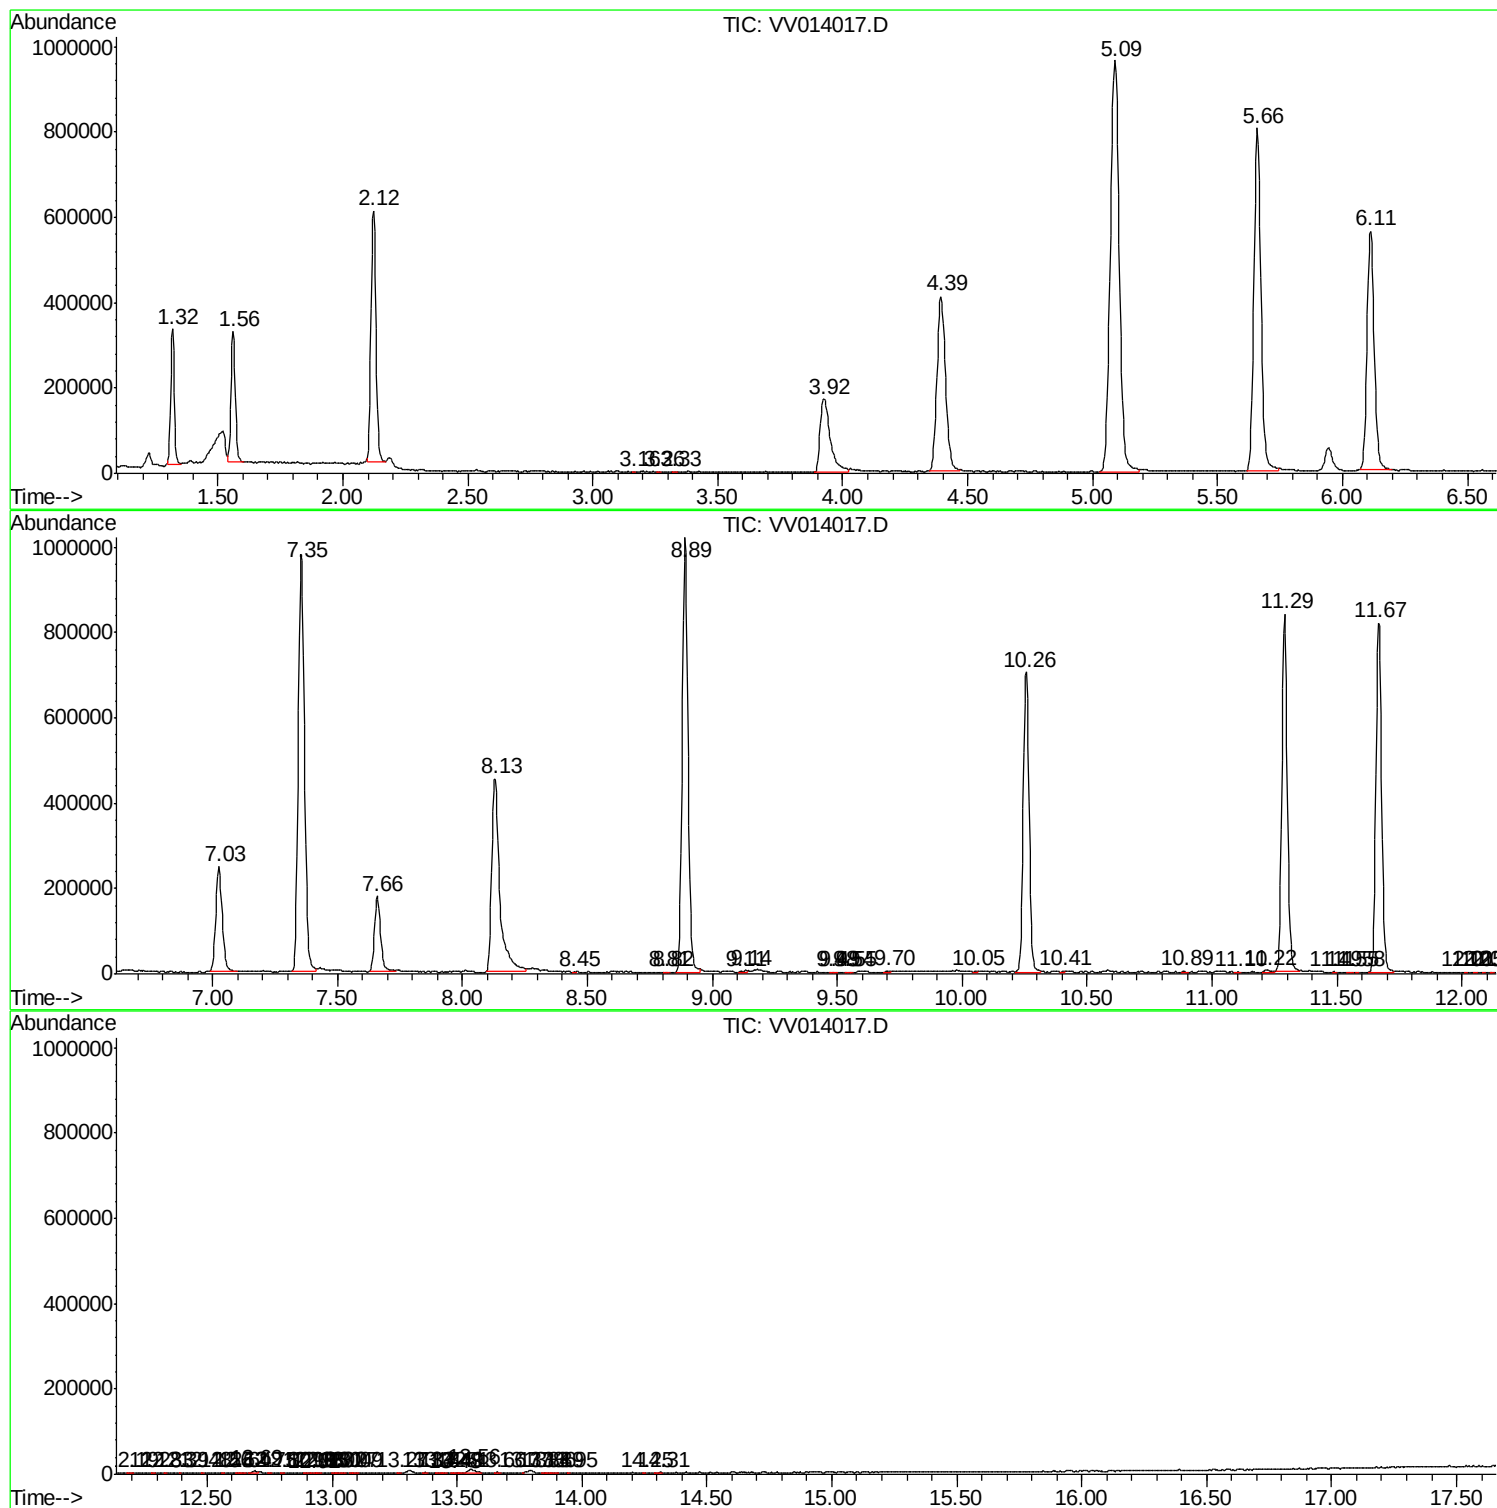

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121119\
Data File : VV014017.D
Acq On : 11 Dec 2019 17:54
Operator : SY/MD
Sample : K6200-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF40

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121119\
Data File : VV014017.D
Acq On : 11 Dec 2019 17:54
Operator : SY/MD
Sample : K6200-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF40

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc