

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121119\
 Data File : VV014023.D
 Acq On : 11 Dec 2019 20:22
 Operator : SY/MD
 Sample : K6308-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C44

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	79	rVB	332173	311646	11.92%	1.635%
2	1.563	141	147	164	rVB	318092	380063	14.54%	1.994%
3	2.122	313	321	335	rVB	613432	856407	32.77%	4.492%
4	2.582	462	464	466	rBV3	2667	1290	0.05%	0.007%
5	2.733	509	511	512	rBV2	1507	509	0.02%	0.003%
6	2.856	545	549	551	rBV5	2263	1883	0.07%	0.010%
7	2.930	570	572	576	rBV3	1746	1442	0.06%	0.008%
8	3.145	637	639	644	rBV5	1265	943	0.04%	0.005%
9	3.396	715	717	718	rBV2	1266	468	0.02%	0.002%
10	3.447	731	733	736	rBV4	1646	741	0.03%	0.004%
11	3.650	794	796	799	rBV5	1440	1025	0.04%	0.005%
12	3.672	801	803	805	rBV3	1138	516	0.02%	0.003%
13	3.785	836	838	842	rBV4	1427	1140	0.04%	0.006%
14	3.801	842	843	845	rBV2	1177	471	0.02%	0.002%
15	3.859	859	861	864	rBV4	1818	1037	0.04%	0.005%
16	3.923	870	881	908	rBV	195103	524426	20.06%	2.751%
17	4.392	1013	1027	1051	rVB	438186	1027839	39.32%	5.392%
18	4.595	1087	1090	1091	rBV3	1874	1128	0.04%	0.006%
19	4.762	1141	1142	1144	rBV2	1368	615	0.02%	0.003%
20	4.833	1163	1164	1168	rBV4	1318	1173	0.04%	0.006%
21	4.923	1191	1192	1195	rBV2	1090	570	0.02%	0.003%
22	5.090	1225	1244	1267	rBV2	1035117	2613754	100.00%	13.711%
23	5.585	1396	1398	1400	rBV3	2095	988	0.04%	0.005%
24	5.659	1407	1421	1446	rBV	858158	1697767	64.96%	8.906%
25	6.113	1549	1562	1586	rVB	588902	1175358	44.97%	6.166%
26	6.486	1673	1678	1681	rBV7	3156	3328	0.13%	0.017%
27	6.810	1775	1779	1780	rBV3	1245	805	0.03%	0.004%
28	6.833	1784	1786	1790	rBV4	1757	1156	0.04%	0.006%
29	6.878	1799	1800	1804	rVB5	1812	1124	0.04%	0.006%
30	7.026	1835	1846	1861	rBV2	279683	507179	19.40%	2.660%
31	7.309	1931	1934	1936	rBV3	2679	1682	0.06%	0.009%
32	7.354	1936	1948	1970	rVV	1137264	1986774	76.01%	10.422%
33	7.659	2034	2043	2063	rVB	204742	337681	12.92%	1.771%
34	7.968	2134	2139	2142	rBV6	3149	3960	0.15%	0.021%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121119\
 Data File : VV014023.D
 Acq On : 11 Dec 2019 20:22
 Operator : SY/MD
 Sample : K6308-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C44

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	8.129	2175	2189	2220	rBV2	533540	1183921	45.30%	6.210%
36	8.730	2374	2376	2380	rBV4	2348	1709	0.07%	0.009%
37	8.891	2414	2426	2447	rBV	1301699	2038928	78.01%	10.696%
38	9.338	2564	2565	2569	rBV4	1348	1087	0.04%	0.006%
39	9.447	2597	2599	2602	rBV4	2512	1233	0.05%	0.006%
40	9.518	2618	2621	2622	rBV2	1697	1109	0.04%	0.006%
41	9.736	2685	2689	2694	rBV7	1523	1598	0.06%	0.008%
42	9.804	2708	2710	2712	rBV2	888	371	0.01%	0.002%
43	9.903	2739	2741	2746	rVB4	1586	1118	0.04%	0.006%
44	9.929	2746	2749	2751	rBV4	2077	1311	0.05%	0.007%
45	10.167	2822	2823	2827	rVB4	1766	793	0.03%	0.004%
46	10.186	2827	2829	2830	rBV2	1059	447	0.02%	0.002%
47	10.257	2839	2851	2867	rBV	702393	1138491	43.56%	5.972%
48	10.540	2936	2939	2942	rBV4	1278	975	0.04%	0.005%
49	10.556	2942	2944	2948	rBV4	1759	1373	0.05%	0.007%
50	10.611	2959	2961	2963	rBV2	1405	805	0.03%	0.004%
51	10.704	2989	2990	2993	rVB	2278	962	0.04%	0.005%
52	10.720	2993	2995	2999	rBV5	1696	1231	0.05%	0.006%
53	10.749	2999	3004	3006	rBV4	2383	2388	0.09%	0.013%
54	10.829	3026	3029	3030	rBV3	1532	576	0.02%	0.003%
55	10.839	3030	3032	3035	rVV3	1522	756	0.03%	0.004%
56	10.984	3075	3077	3080	rBV3	1179	680	0.03%	0.004%
57	11.071	3101	3104	3108	rVB4	2131	1587	0.06%	0.008%
58	11.093	3108	3111	3112	rBV2	989	492	0.02%	0.003%
59	11.215	3141	3149	3153	rBV10	2601	4241	0.16%	0.022%
60	11.289	3160	3172	3194	rBV	1016209	1562518	59.78%	8.196%
61	11.665	3277	3289	3309	rBV	1016373	1629174	62.33%	8.546%
62	12.103	3424	3425	3426	rBV	1122	399	0.02%	0.002%
63	12.183	3447	3450	3451	rBV3	1452	745	0.03%	0.004%
64	12.286	3479	3482	3484	rBV3	2638	1963	0.08%	0.010%
65	12.376	3505	3510	3514	rBV8	2079	2007	0.08%	0.011%
66	12.540	3557	3561	3563	rVB4	1452	981	0.04%	0.005%
67	12.553	3563	3565	3567	rBV2	1200	559	0.02%	0.003%
68	12.585	3573	3575	3577	rBV3	1470	824	0.03%	0.004%
69	12.836	3651	3653	3655	rBV3	1598	554	0.02%	0.003%
70	12.855	3658	3659	3662	rVB3	1144	403	0.02%	0.002%
71	12.981	3695	3698	3702	rBV3	1969	1421	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121119\
 Data File : VV014023.D
 Acq On : 11 Dec 2019 20:22
 Operator : SY/MD
 Sample : K6308-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C44

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	13.479	3850	3853	3859	rVB7	2731	2725	0.10%	0.014%
73	13.508	3859	3862	3867	rBV6	2281	2262	0.09%	0.012%
74	13.698	3918	3921	3924	rBV4	1772	895	0.03%	0.005%
75	13.733	3929	3932	3936	rBV5	906	707	0.03%	0.004%
76	13.765	3941	3942	3944	rBV2	1125	459	0.02%	0.002%
77	13.826	3959	3961	3963	rBV3	559	315	0.01%	0.002%
78	13.868	3966	3974	3978	rBV6	1524	1648	0.06%	0.009%
79	13.903	3980	3985	3991	rBV10	1429	1387	0.05%	0.007%
80	13.939	3993	3996	3998	rBV4	1303	730	0.03%	0.004%
81	13.974	4003	4007	4008	rBV4	1144	582	0.02%	0.003%
82	13.987	4008	4011	4014	rBV4	1102	531	0.02%	0.003%
83	14.006	4015	4017	4020	rVB3	671	305	0.01%	0.002%
84	14.019	4020	4021	4023	rBV3	1082	404	0.02%	0.002%
85	14.077	4037	4039	4040	rBV2	707	279	0.01%	0.001%
86	14.128	4052	4055	4056	rBV3	527	246	0.01%	0.001%
87	14.141	4057	4059	4061	rVB2	976	264	0.01%	0.001%
88	14.167	4061	4067	4071	rBV6	2158	1958	0.07%	0.010%
89	14.215	4080	4082	4084	rVB3	1591	703	0.03%	0.004%
90	14.231	4084	4087	4090	rVB5	1655	1261	0.05%	0.007%
91	14.260	4092	4096	4099	rBV4	1005	843	0.03%	0.004%
92	14.299	4106	4108	4109	rBV2	927	266	0.01%	0.001%
93	14.373	4129	4131	4135	rVB4	1178	786	0.03%	0.004%
94	14.398	4135	4139	4141	rBV3	1350	1129	0.04%	0.006%
95	14.479	4161	4164	4165	rBV4	1038	642	0.02%	0.003%
96	14.521	4175	4177	4178	rBV2	840	226	0.01%	0.001%
97	14.530	4178	4180	4182	rBV4	1341	633	0.02%	0.003%
98	14.588	4194	4198	4201	rBV5	3734	2935	0.11%	0.015%
99	14.611	4201	4205	4207	rVV5	981	802	0.03%	0.004%
100	14.653	4216	4218	4220	rBV3	1718	849	0.03%	0.004%


Sum of corrected areas: 19063390

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121119\
Data File : VV014023.D
Acq On : 11 Dec 2019 20:22
Operator : SY/MD
Sample : K6308-15
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C44

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

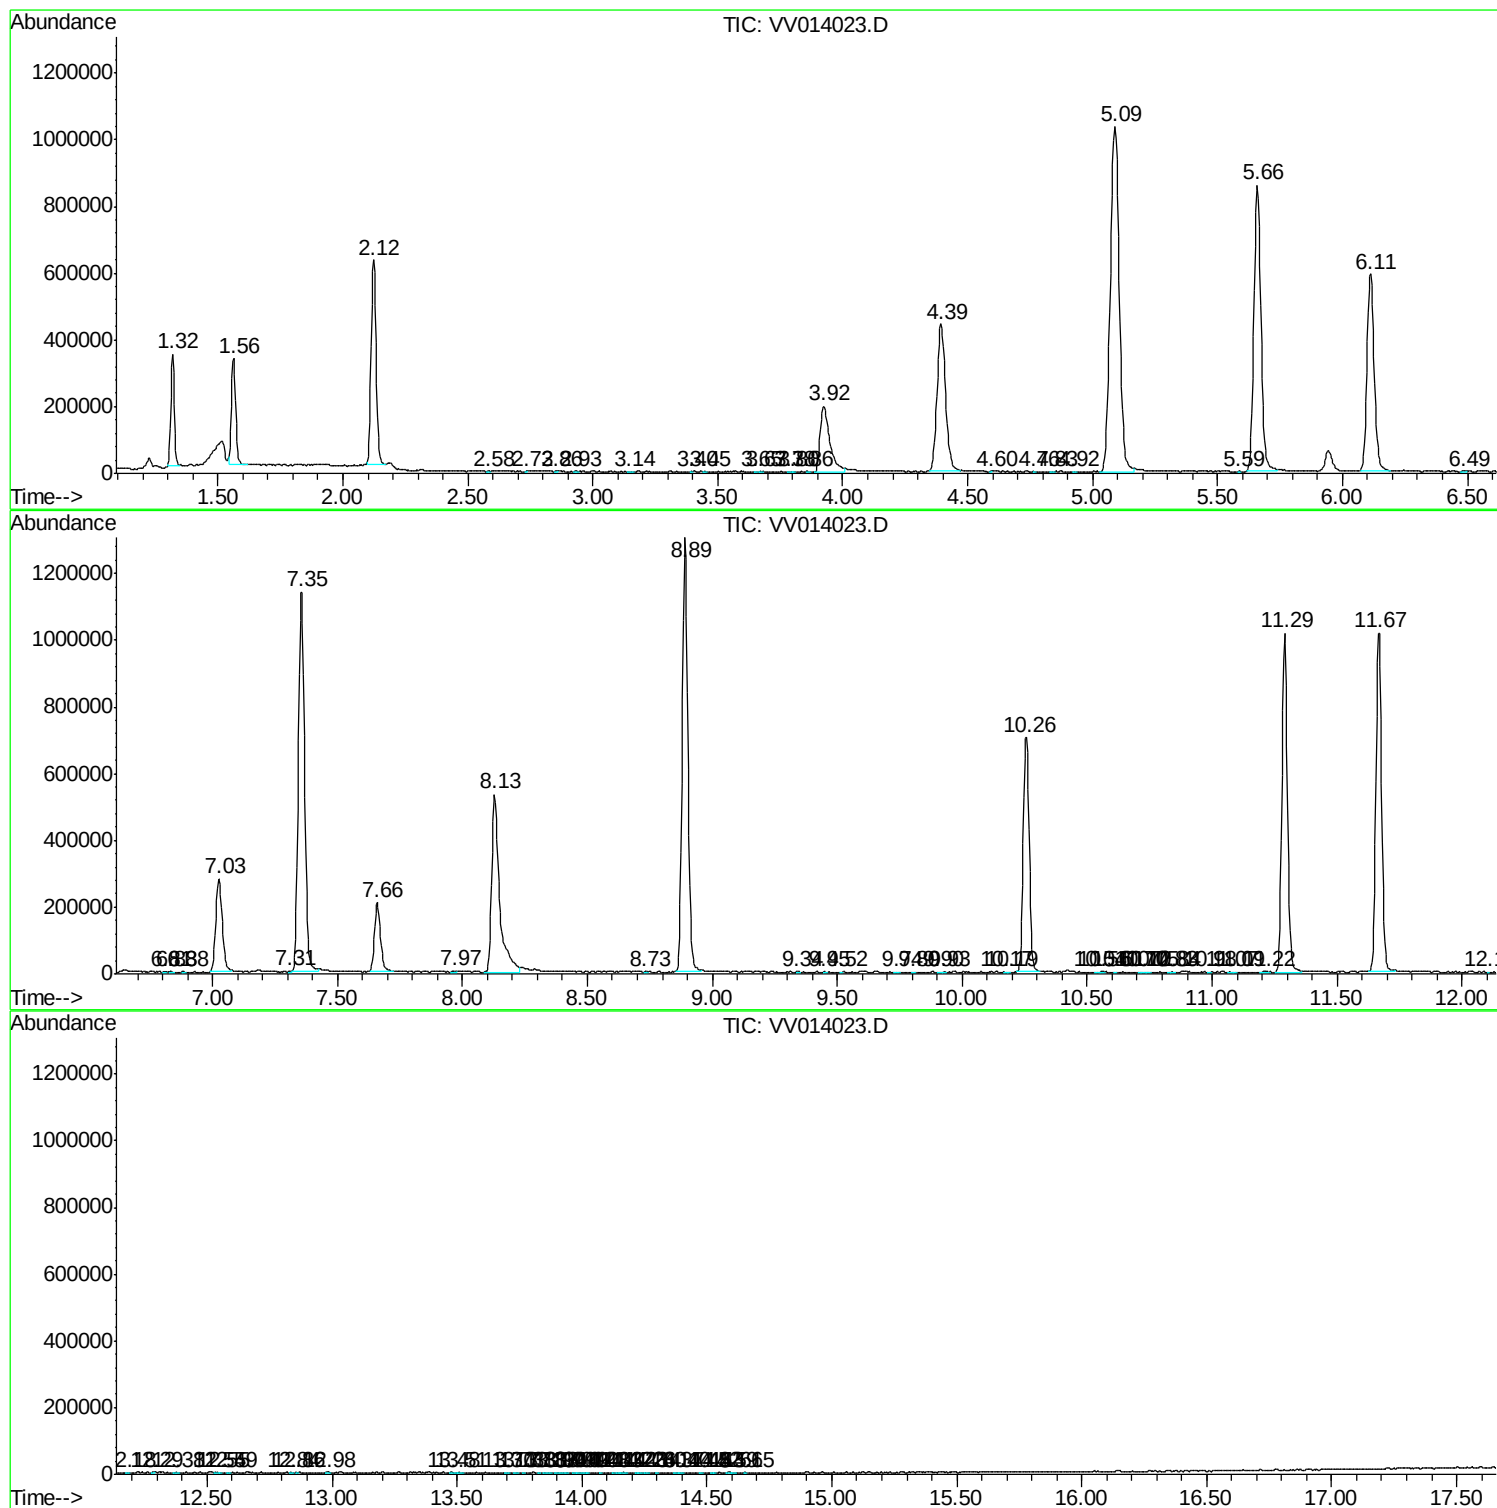

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121119\
Data File : VV014023.D
Acq On : 11 Dec 2019 20:22
Operator : SY/MD
Sample : K6308-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C44

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121119\
Data File : VV014023.D
Acq On : 11 Dec 2019 20:22
Operator : SY/MD
Sample : K6308-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C44

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc