


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121119\
 Data File : VV014003.D
 Acq On : 11 Dec 2019 09:23
 Operator : SY/MD
 Sample : BFB80
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB80

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis
 Last Update : Thu Dec 12 03:01:11 2019

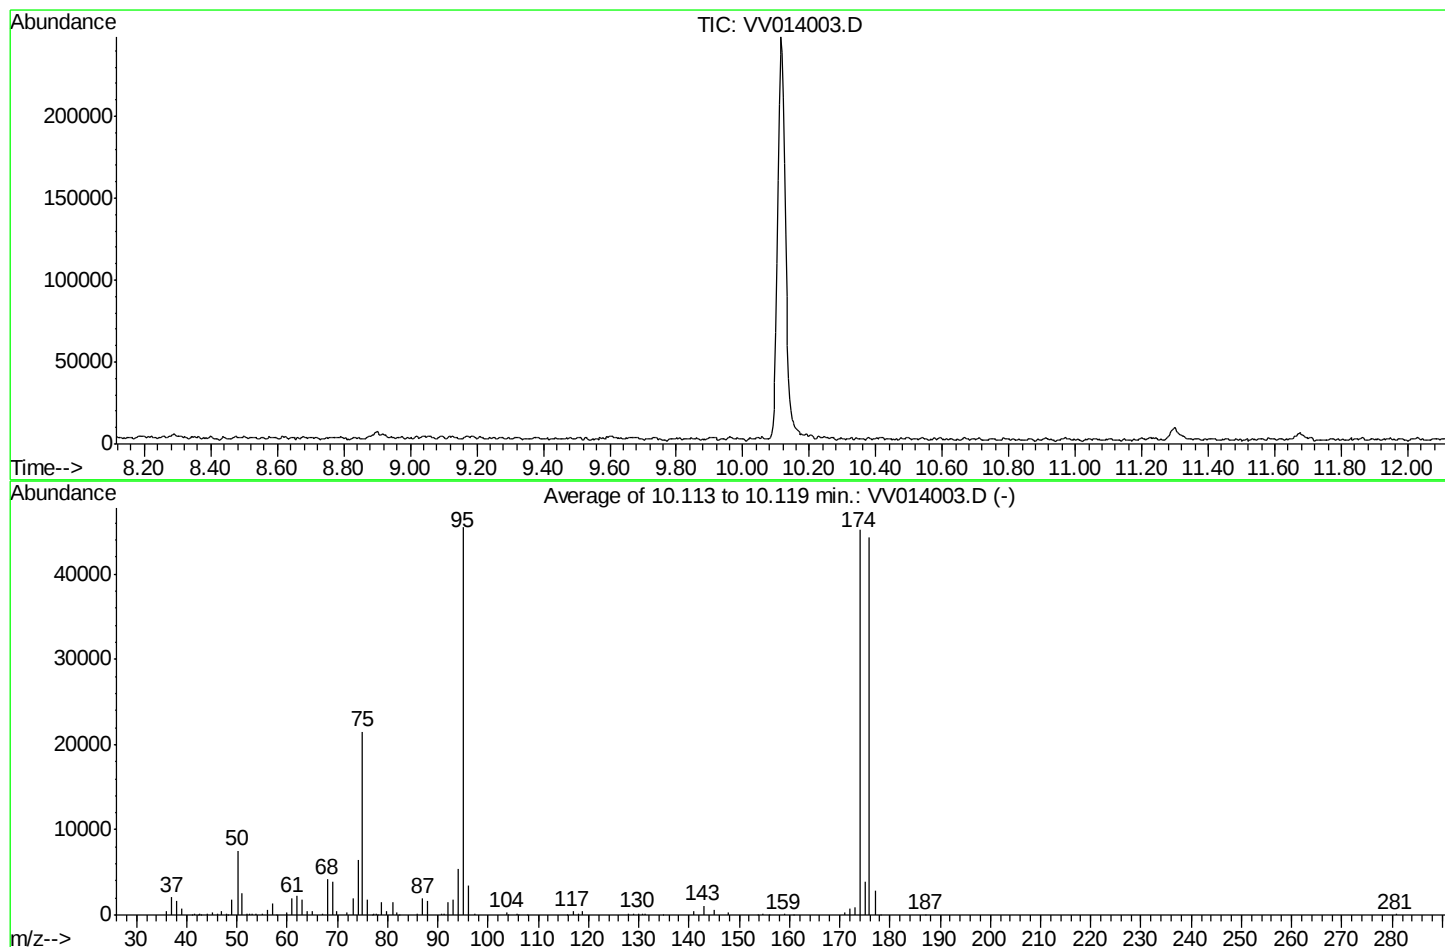

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	7568	PASS
75	95	30	80	47.3	21517	PASS
95	95	100	100	100.0	45496	PASS
96	95	5	9	7.4	3388	PASS
173	174	0.00	2	1.9	878	PASS
174	95	50	120	99.3	45170	PASS
175	174	5	9	8.6	3869	PASS
176	174	95	101	98.1	44322	PASS
177	176	5	9	6.6	2927	PASS

m/z	Abundance
36.00	471.0
37.00	2002.0
38.00	1940.0
39.00	826.0
39.90	659.0
41.60	138.0
42.20	109.0
42.80	136.0
44.00	799.0
45.00	436.0
46.00	161.0
46.90	518.0
48.10	289.0
49.00	1842.0
50.10	7725.0
51.00	2666.0
52.00	175.0
53.00	154.0
53.80	160.0
55.00	217.0
55.90	545.0
57.00	1412.0
59.80	460.0
61.00	2120.0
62.00	2265.0
63.00	1855.0
64.10	501.0
65.00	464.0
67.00	188.0
68.00	4178.0
69.00	3927.0
69.90	397.0
71.90	363.0
73.10	1858.0
74.10	6367.0
75.10	21192.0
76.10	2123.0
76.90	227.0
77.80	324.0
78.80	1389.0
80.00	465.0
81.00	1588.0
81.80	366.0
85.70	119.0
86.90	1718.0
87.90	1709.0
90.70	150.0
91.20	194.0
92.00	1458.0
93.00	1813.0
94.00	5146.0
95.00	44768.0
96.10	3488.0
97.20	121.0
103.80	230.0
104.10	215.0
106.10	103.0
107.80	115.0
115.80	166.0
116.80	413.0
117.90	133.0
118.90	421.0
128.10	188.0
129.80	261.0
130.90	141.0
141.00	350.0
142.90	1045.0
144.90	517.0
147.90	193.0
153.80	104.0
154.90	123.0
159.00	139.0
170.90	288.0
172.00	764.0
173.00	867.0
174.00	43872.0
175.00	3846.0
175.90	42896.0
177.00	2855.0
187.10	134.0
280.80	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.00	491.0
37.10	2167.0
38.10	1909.0
39.00	961.0
39.90	715.0
41.60	160.0
42.50	126.0
42.90	143.0
44.10	777.0
45.10	446.0
46.00	156.0
46.90	569.0
48.00	290.0
49.00	1976.0
50.10	7725.0
51.10	2687.0
51.90	170.0
52.40	168.0
53.00	164.0
53.80	109.0
55.00	238.0
56.00	625.0
57.00	1319.0
59.80	419.0
61.00	2068.0
62.00	2366.0
63.00	1804.0
64.10	477.0
64.90	531.0
67.00	211.0
68.10	4337.0
69.00	3931.0
70.00	405.0
71.90	301.0
73.00	1990.0
74.00	6517.0
75.10	22168.0
76.00	2048.0
77.10	295.0
77.80	244.0
78.90	1483.0
79.80	486.0
81.00	1519.0
81.80	371.0
82.30	181.0
85.80	199.0
87.00	2005.0
87.90	1630.0
90.70	180.0
91.10	206.0
92.00	1533.0
93.00	1859.0
94.00	5589.0
95.00	46640.0
96.10	3590.0
97.30	152.0
103.80	229.0
105.70	153.0
107.80	110.0
115.80	138.0
116.80	412.0
117.90	167.0
118.80	413.0
128.10	218.0
128.90	116.0
129.80	224.0
130.80	151.0
131.20	145.0
140.90	407.0
142.90	1167.0
144.90	557.0
147.80	280.0
154.80	127.0
159.00	176.0
171.00	327.0
171.90	770.0
173.00	897.0
174.00	46272.0
175.00	4043.0
176.00	45728.0
177.00	3042.0
178.10	121.0
280.80	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.00	449.0
37.00	2088.0
38.00	1695.0
39.00	1012.0
39.90	741.0
41.00	111.0
41.70	167.0
42.50	157.0
42.90	156.0
44.10	850.0
45.10	389.0
45.70	121.0
46.90	548.0
47.80	325.0
49.00	1814.0
50.10	7256.0
51.10	2370.0
51.90	158.0
52.50	165.0
52.90	212.0
55.00	226.0
56.10	715.0
57.00	1137.0
57.90	125.0
60.00	440.0
61.00	1904.0
62.00	2247.0
63.00	1669.0
64.00	472.0
65.00	522.0
67.00	200.0
68.10	3991.0
69.00	3767.0
70.00	344.0
72.00	273.0
73.00	1939.0
74.00	6390.0
75.00	21192.0
76.10	1614.0
77.10	336.0
78.00	187.0
78.90	1438.0
79.80	573.0
81.00	1540.0
81.80	338.0
85.90	213.0
87.00	1937.0
88.00	1606.0
91.10	211.0
92.00	1452.0
93.00	1793.0
94.10	5478.0
95.00	45080.0
96.10	3088.0
97.40	154.0
103.80	237.0
105.70	207.0
115.70	149.0
116.90	439.0
117.90	180.0
118.80	377.0
127.90	239.0
128.90	153.0
129.90	179.0
130.80	139.0
131.20	129.0
134.90	149.0
140.80	491.0
143.00	1086.0
144.90	551.0
147.80	285.0
154.70	171.0
156.00	137.0
159.00	136.0
160.90	101.0
171.00	296.0
171.90	832.0
172.90	870.0
174.00	45368.0
175.00	3720.0
176.00	44344.0
177.00	2886.0
280.80	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

Scan 2795 (10.077 min): VV014003.D
BFB80

m/z	Abundance
37.90	138.0
39.10	133.0
40.00	782.0
42.80	137.0
44.00	661.0
45.10	122.0
45.80	194.0
47.10	108.0
48.20	133.0
55.70	123.0
76.00	114.0
115.80	111.0
206.90	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80