




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121121\
Data File : VV023930.D
Acq On : 11 Dec 2021 14:54
Operator : SY/MD
Sample : M4984-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/13/2021
Supervised By :Mahesh Dadoda 12/13/2021

Quant Time: Dec 12 00:27:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 11 04:33:17 2021
Response via : Initial Calibration

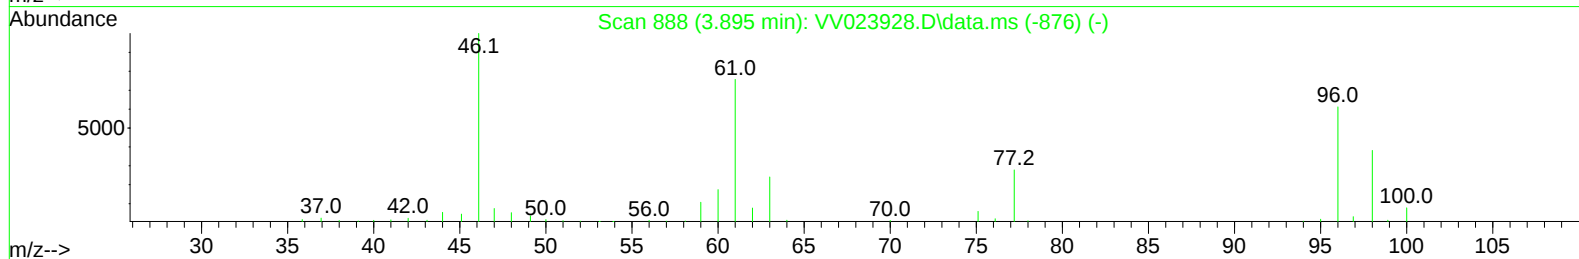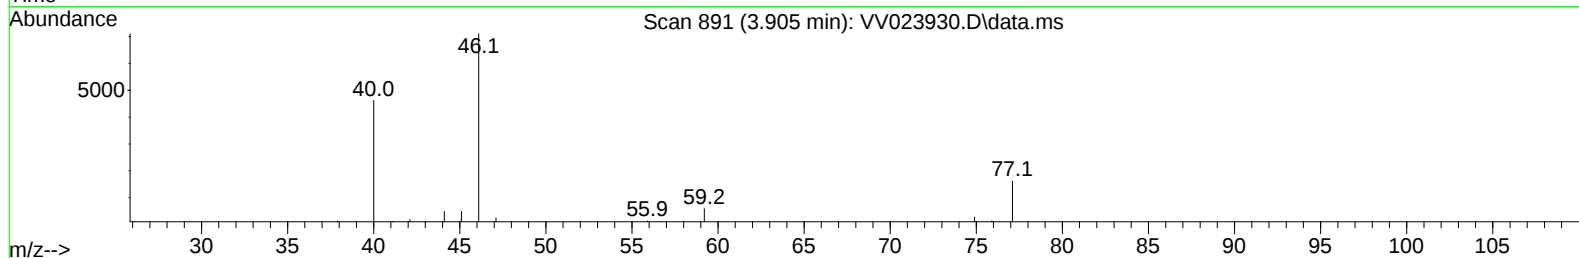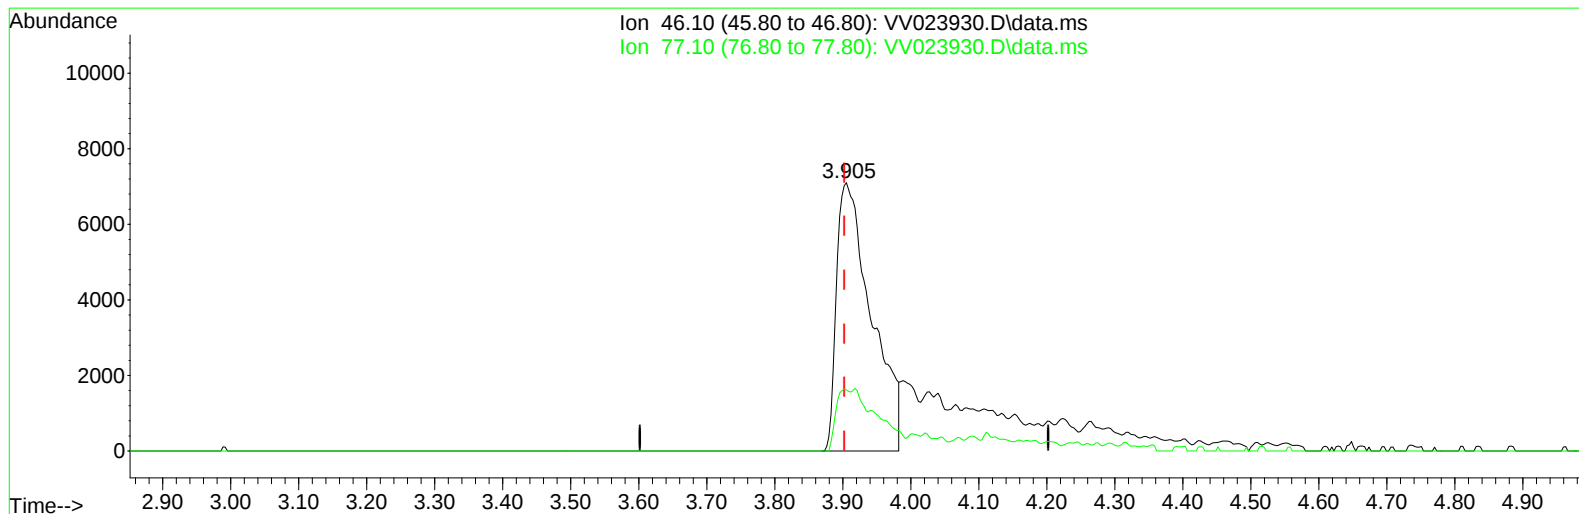

TIC: VV023930.D\data.ms

(20) 2-Butanone-d5 (S)

3.905min (+ 0.003) 24.70 ug/L

response 25282

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.40	9.67
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121121\
Data File : VV023930.D
Acq On : 11 Dec 2021 14:54
Operator : SY/MD
Sample : M4984-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/13/2021
Supervised By :Mahesh Dadoda 12/13/2021

Quant Time: Dec 12 00:27:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 11 04:33:17 2021
Response via : Initial Calibration

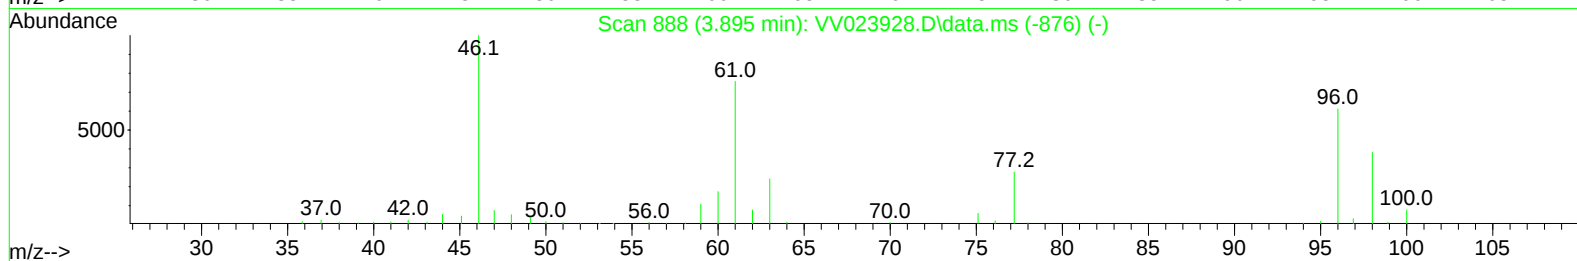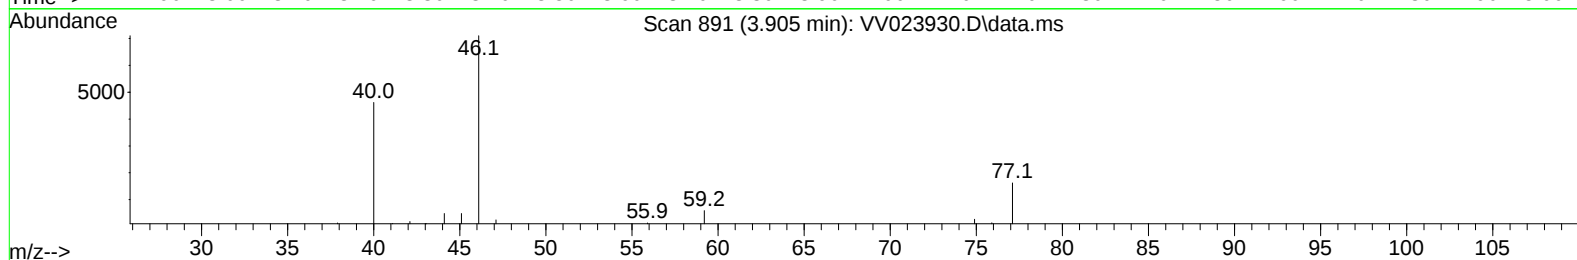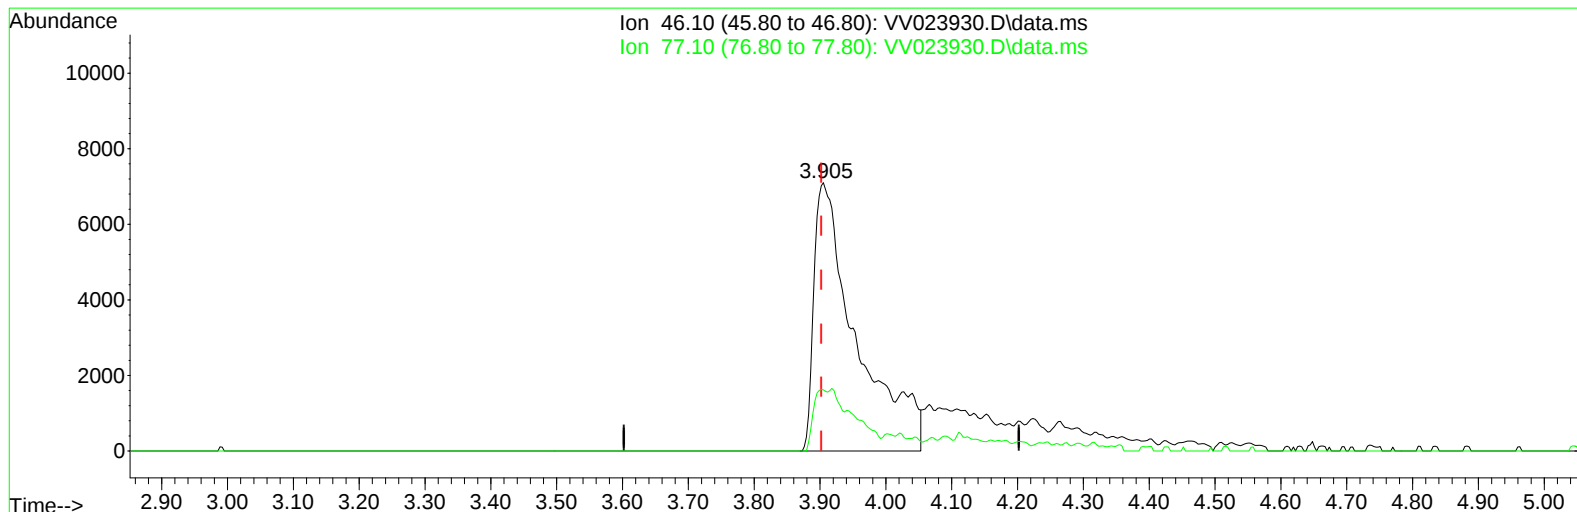

TIC: VV023930.D\data.ms

(20) 2-Butanone-d5 (S)

3.905min (+ 0.003) 30.96 ug/L m

response 31693

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.40	7.71
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121121\
 Data File : VW023930.D
 Acq On : 11 Dec 2021 14:54
 Operator : SY/MD
 Sample : M4984-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/13/2021
 Supervised By :Mahesh Dadoda 12/13/2021

Quant Time: Dec 12 00:27:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	97469	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	101882	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	51384	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	25587	4.883	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	97.600%	
7) Chloroethane-d5	1.568	69	20338	4.652	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	93.000%	
11) 1,1-Dichloroethene-d2	2.105	63	37631	3.679	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	73.600%	
20) 2-Butanone-d5	3.905	46	31693m	30.959	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	61.920%	
24) Chloroform-d	4.349	84	51221	4.316	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.400%	
26) 1,2-Dichloroethane-d4	5.034	65	24018	4.346	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	87.000%	
32) Benzene-d6	5.050	84	95521	4.734	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.600%	
36) 1,2-Dichloropropane-d6	6.069	67	26786	4.400	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	88.000%	
41) Toluene-d8	7.317	98	84678	4.661	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	93.200%	
43) trans-1,3-Dichloroprop...	7.622	79	9859	3.904	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	78.000%	
46) 2-Hexanone-d5	8.091	63	34051	30.117	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	60.240%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	18448	3.653	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	73.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	32083	4.674	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	93.400%	
Target Compounds						
16) Methylene chloride	2.503	84	7584	0.886	ug/L	92
64) 1,3-Dichlorobenzene	11.185	146	1733	0.112	ug/L	90
65) 1,4-Dichlorobenzene	11.271	146	5016	0.324	ug/L	99
67) 1,2-Dichlorobenzene	11.641	146	5941	0.420	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121121\
Data File : VV023930.D
Acq On : 11 Dec 2021 14:54
Operator : SY/MD
Sample : M4984-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/13/2021
Supervised By :Mahesh Dadoda 12/13/2021

Quant Time: Dec 12 00:27:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 11 04:33:17 2021
Response via : Initial Calibration

