
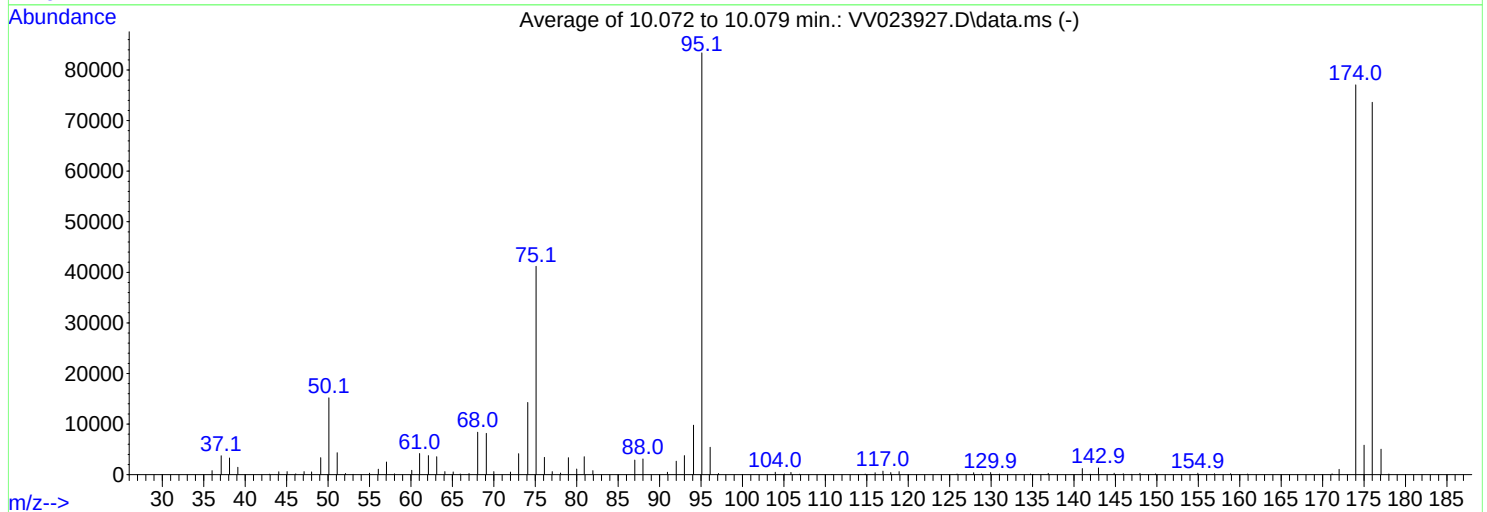


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121121\
 Data File : VV023927.D
 Acq On : 11 Dec 2021 09:10
 Operator : SY/MD
 Sample : BFB250
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB250

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Dec 11 04:33:17 2021

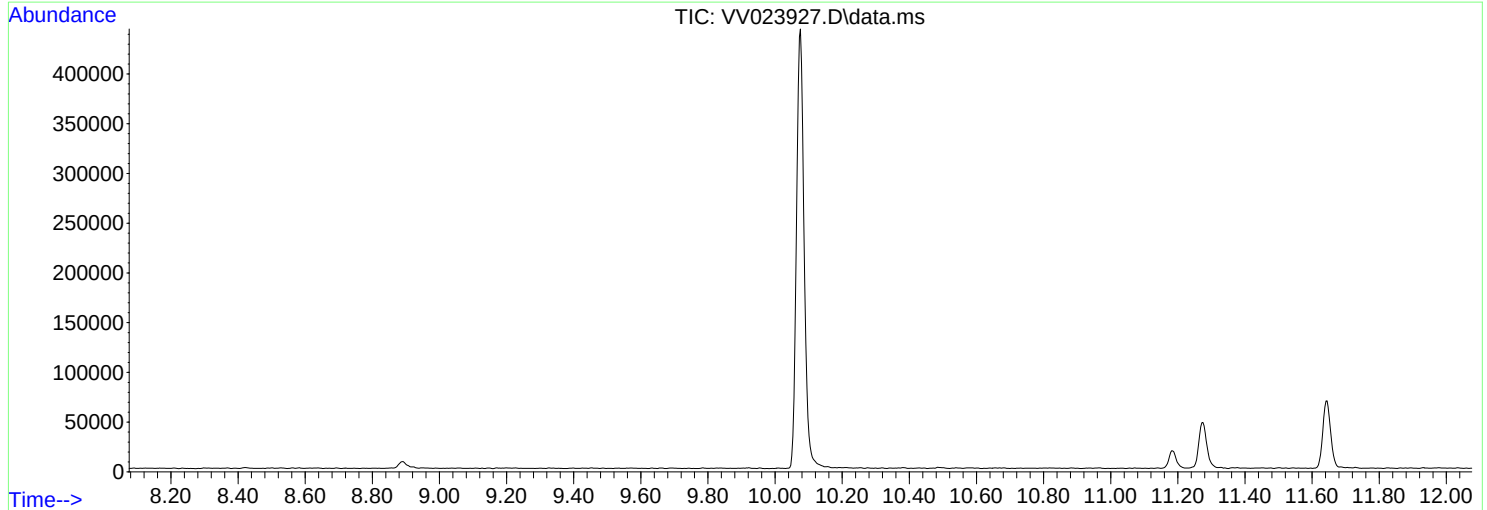

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	15179	PASS
75	95	30	80	49.4	41179	PASS
95	95	100	100	100.0	83397	PASS
96	95	5	9	6.5	5405	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.4	77075	PASS
175	174	5	9	7.6	5822	PASS
176	174	95	105	95.5	73613	PASS
177	176	5	10	6.9	5047	PASS

m/z	Abundance
40.00	3469.0
44.00	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB250

m/z	Abundance
36.00	751.0
37.10	3354.0
38.10	3161.0
39.10	1452.0
40.00	3662.0
43.00	145.0
44.10	663.0
45.00	612.0
46.10	148.0
47.10	585.0
48.00	444.0
49.10	3076.0
50.10	14267.0
51.10	4209.0
52.20	226.0
55.00	292.0
56.00	928.0
57.00	2268.0
58.00	147.0
60.10	794.0
61.10	3893.0
62.10	3492.0
63.10	3277.0
64.10	506.0
65.10	429.0
66.00	105.0
67.00	219.0
68.00	8023.0
69.10	7636.0
70.00	685.0
72.00	471.0
73.00	3855.0
74.10	13576.0
75.10	38616.0
76.10	3216.0
77.10	602.0
78.10	306.0
79.00	3044.0
80.00	1066.0
80.90	3181.0
82.00	776.0
87.00	2709.0
88.00	2837.0
91.00	441.0
92.00	2496.0
93.00	3575.0
94.10	9324.0
95.10	78928.0
96.10	5148.0
97.10	216.0
103.90	487.0
105.80	418.0
110.80	101.0
114.80	129.0
116.00	295.0
117.00	642.0
117.90	447.0
118.90	610.0
125.90	107.0
127.90	329.0
128.80	119.0
130.00	363.0
131.10	104.0
134.70	111.0
136.90	245.0
141.00	1124.0
142.00	153.0
142.90	1272.0
144.90	221.0
146.00	192.0
148.00	249.0
149.80	144.0
154.90	290.0
156.90	253.0
158.90	189.0
161.00	126.0
171.10	160.0
172.00	979.0
174.00	74496.0
175.00	5695.0
176.00	71240.0
177.10	4902.0
178.00	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB250

m/z	Abundance
36.00	839.0
37.10	3878.0
38.10	3419.0
39.10	1496.0
40.00	3523.0
42.90	128.0
44.10	678.0
45.10	622.0
46.10	188.0
47.10	626.0
48.00	552.0
49.10	3442.0
50.10	15619.0
51.10	4443.0
52.10	210.0
53.00	104.0
55.00	314.0
56.00	1092.0
57.00	2595.0
58.00	160.0
60.10	913.0
61.10	4375.0
62.10	3875.0
63.10	3717.0
64.10	597.0
65.10	557.0
65.90	137.0
67.00	225.0
68.00	8728.0
69.10	8442.0
70.00	597.0
72.00	501.0
73.00	4293.0
74.10	14687.0
75.10	42392.0
76.10	3532.0
77.10	609.0
78.10	345.0
79.00	3466.0
80.00	1167.0
80.90	3710.0
81.90	829.0
87.00	2888.0
88.00	3177.0
91.00	461.0
92.00	2726.0
93.00	3904.0
94.10	10063.0
95.10	86800.0
96.10	5551.0
97.10	220.0
103.90	484.0
105.00	166.0
105.80	487.0
106.90	138.0
114.80	151.0
116.00	410.0
117.00	712.0
117.90	416.0
118.90	634.0
125.90	122.0
127.90	390.0
128.80	120.0
129.90	418.0
131.00	106.0
134.80	117.0
135.10	100.0
136.90	250.0
141.00	1231.0
141.90	112.0
143.00	1334.0
144.90	285.0
145.90	187.0
146.90	115.0
148.00	273.0
149.80	165.0
154.90	306.0
157.00	210.0
158.90	197.0
161.00	132.0
171.10	171.0
172.00	1081.0
174.00	79504.0
175.00	6013.0
176.00	75888.0
177.00	5241.0
178.00	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB250

m/z	Abundance
36.00	786.0
37.10	4017.0
38.10	3301.0
39.10	1401.0
40.00	3294.0
44.10	667.0
45.00	583.0
46.10	184.0
47.10	637.0
48.00	646.0
49.10	3558.0
50.10	15650.0
51.10	4380.0
52.00	203.0
53.00	110.0
55.00	288.0
56.10	1205.0
57.10	2660.0
58.00	170.0
60.10	896.0
61.00	4244.0
62.10	3980.0
63.10	3645.0
64.10	666.0
65.10	592.0
65.90	162.0
67.00	208.0
68.10	8404.0
69.10	8454.0
70.00	522.0
72.00	521.0
73.00	4251.0
74.10	14551.0
75.10	42528.0
76.10	3545.0
77.00	564.0
78.00	304.0
79.00	3596.0
80.00	1074.0
80.90	3746.0
82.00	800.0
87.00	3061.0
88.00	3264.0
90.90	499.0
92.00	2714.0
93.00	3800.0
94.10	9983.0
95.10	84464.0
96.10	5515.0
97.10	196.0
104.00	465.0
105.10	193.0
105.90	473.0
106.90	159.0
114.80	149.0
116.00	492.0
116.90	762.0
117.90	346.0
118.90	576.0
125.90	135.0
127.90	403.0
128.90	142.0
129.90	468.0
130.90	143.0
134.80	170.0
136.90	237.0
141.00	1228.0
143.00	1364.0
144.80	350.0
145.90	160.0
146.90	129.0
147.90	223.0
149.90	137.0
152.90	119.0
155.00	294.0
157.00	143.0
158.90	189.0
160.90	153.0
171.20	173.0
172.00	1041.0
174.00	77224.0
175.00	5759.0
176.00	73712.0
177.00	4998.0
178.00	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB250