

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033208.D
 Acq On : 11 Dec 2023 13:27
 Operator : SY/MD
 Sample : 05685-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHK2

Quant Time: Dec 12 00:41:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 21:51:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	257967	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	265921	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	135313	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	58910	38.201	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	76.400%
7) Chloroethane-d5	1.532	69	48695	45.319	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.640%
11) 1,1-Dichloroethene-d2	2.063	65	24235	41.310	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.620%
21) 2-Butanone-d5	3.783	46	85515	111.647	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	111.650%
24) Chloroform-d	4.249	84	162824	49.752	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.500%
26) 1,2-Dichloroethane-d4	4.944	65	111785	54.939	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.880%
32) Benzene-d6	4.963	84	299302	48.125	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.240%
36) 1,2-Dichloropropane-d6	5.989	67	83310	49.820	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.640%
41) Toluene-d8	7.243	98	272183	45.877	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.760%
43) trans-1,3-Dichloroprop...	7.554	79	49480	46.793	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.580%
47) 2-Hexanone-d5	8.024	63	69813	103.921	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.920%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	119078	50.093	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.180%
66) 1,2-Dichlorobenzene-d4	11.561	152	128973	53.571	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.140%
Target Compounds						
					Qvalue	
13) Acetone	2.114	43	4675	6.393	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033208.D
Acq On : 11 Dec 2023 13:27
Operator : SY/MD
Sample : 05685-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHK2

Quant Time: Dec 12 00:41:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 21:51:12 2023
Response via : Initial Calibration

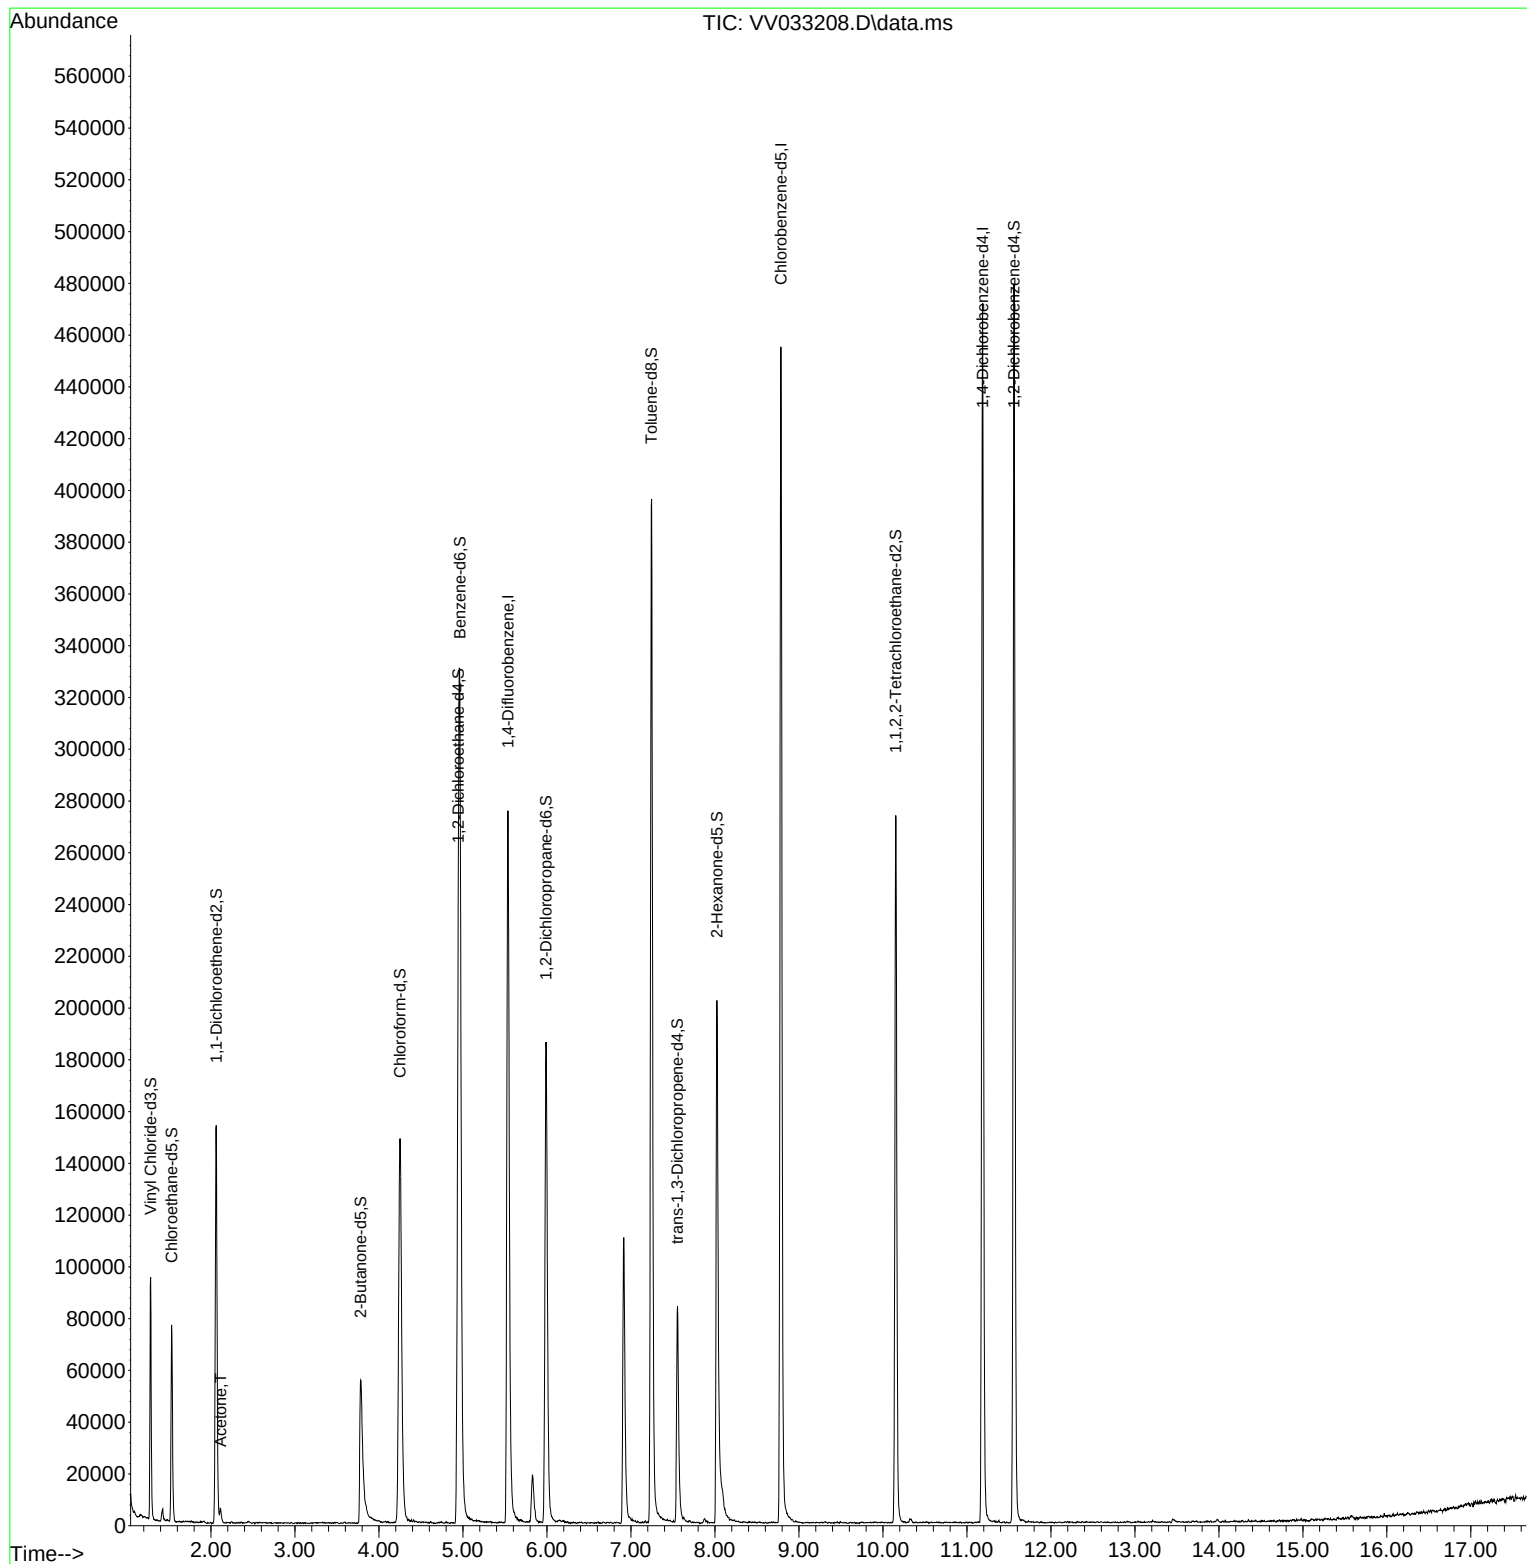

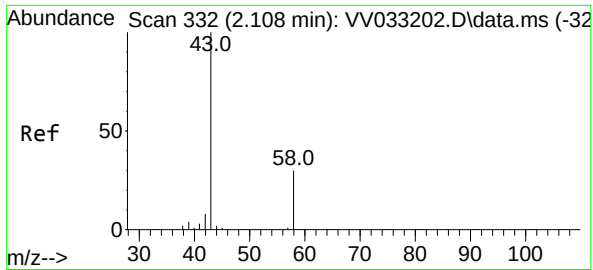

#13
 Acetone
 Concen: 6.393 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VV033208.D
 Acq: 11 Dec 2023 13:27

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHK2

Tgt Ion: 43 Resp: 4675
 Ion Ratio Lower Upper
 43 100
 58 31.6 0.0 62.8

