

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033213.D
 Acq On : 11 Dec 2023 15:21
 Operator : SY/MD
 Sample : 05685-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCH87

Quant Time: Dec 12 00:42:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 21:51:12 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 12/12/2023
 Supervised By :Semsettin Yesilyurt 12/12/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	270719	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	275193	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	141140	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	63777	39.408	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	78.820%		
7) Chloroethane-d5	1.532	69	50761	45.016	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	90.040%		
11) 1,1-Dichloroethene-d2	2.059	65	28418	46.158	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.320%		
21) 2-Butanone-d5	3.780	46	85862	106.819	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	106.820%		
24) Chloroform-d	4.249	84	165690	48.243	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.480%		
26) 1,2-Dichloroethane-d4	4.940	65	107475	50.332	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.660%		
32) Benzene-d6	4.960	84	309473	48.084	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.160%		
36) 1,2-Dichloropropane-d6	5.989	67	81309	46.985	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.980%		
41) Toluene-d8	7.246	98	287461	46.820	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.640%		
43) trans-1,3-Dichloroprop...	7.554	79	49457	45.196	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.400%		
47) 2-Hexanone-d5	8.024	63	66798	96.083	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	96.080%		
56) 1,1,2,2-Tetrachloroeth...	10.152	84	121904	49.554	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	99.100%		
66) 1,2-Dichlorobenzene-d4	11.561	152	136600	54.396	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.800%		
Target Compounds					Qvalue	
13) Acetone	2.111	43	29350	38.248	ug/L	99
18) Methyl tert-butyl Ether	2.709	73	7507	1.387	ug/L #	93
22) 2-Butanone	3.876	43	21845m	22.370	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033213.D
Acq On : 11 Dec 2023 15:21
Operator : SY/MD
Sample : 05685-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
YCH87

Quant Time: Dec 12 00:42:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 21:51:12 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 12/12/2023
Supervised By :Semsettin Yesilyurt 12/12/2023

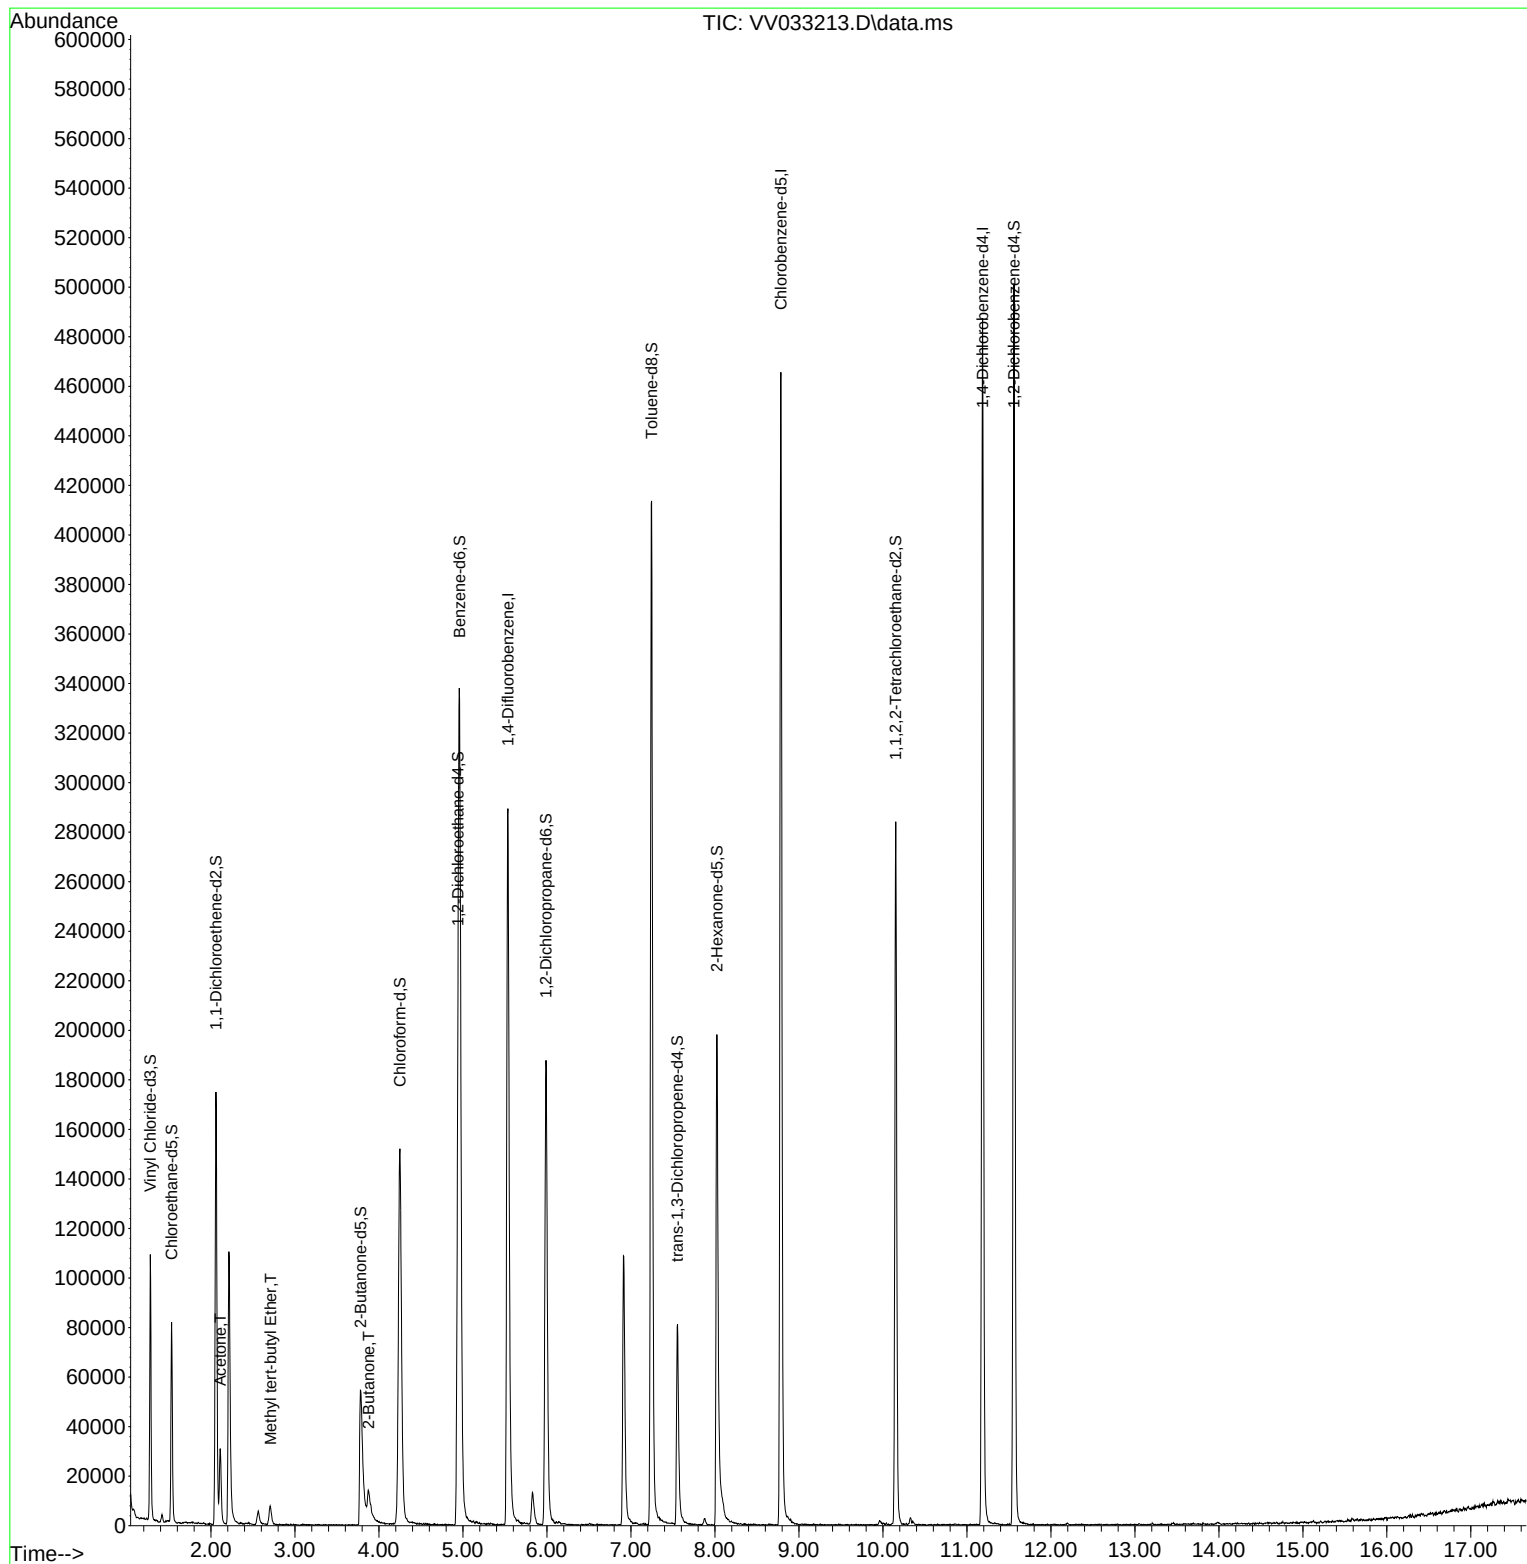

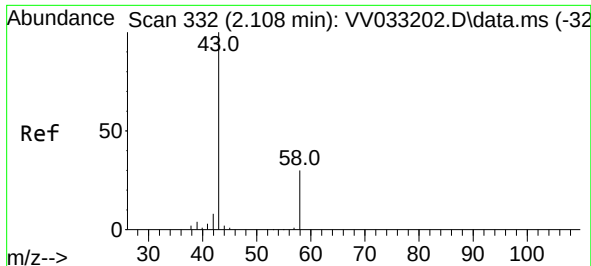

#13

Acetone

Concen: 38.248 ug/L

RT: 2.111 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV033213.D

Acq: 11 Dec 2023 15:21

Instrument :

MSVOA_V

ClientSampleId :

YCH87

Tgt Ion: 43 Resp: 29350

Ion Ratio Lower Upper

43 100





58 31.9 0.0 62.8

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 12/12/2023

Supervised By :Semsettin Yesilyurt 12/12/2023

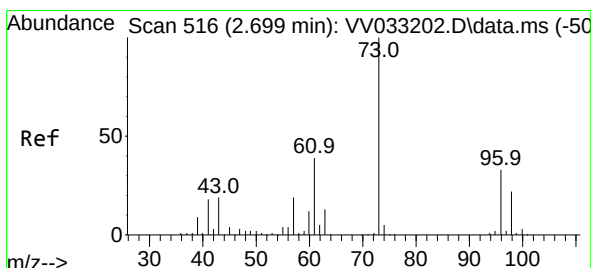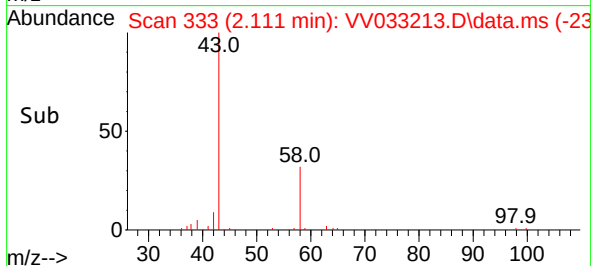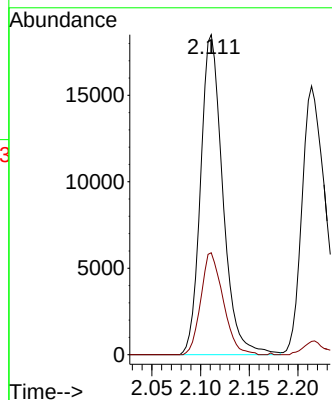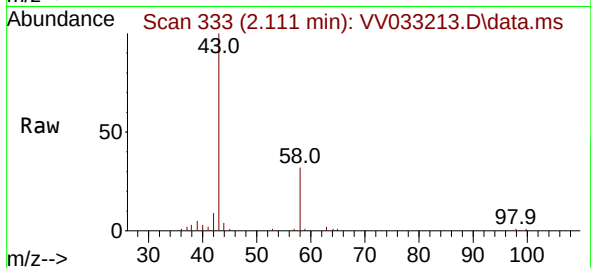

#18

Methyl tert-butyl Ether

Concen: 1.387 ug/L

RT: 2.709 min Scan# 519

Delta R.T. 0.010 min

Lab File: VV033213.D

Acq: 11 Dec 2023 15:21




Tgt Ion: 73 Resp: 7507


Ion Ratio Lower Upper

73 100

43 21.9 15.4 23.2


57 16.1 16.1 24.1#

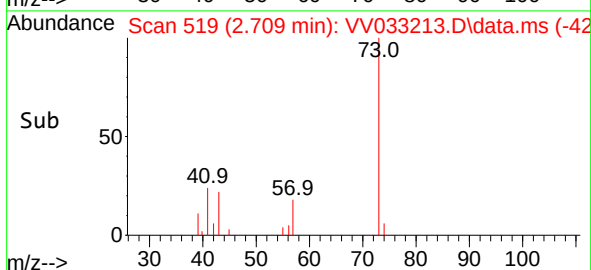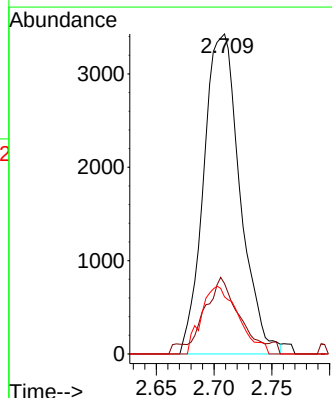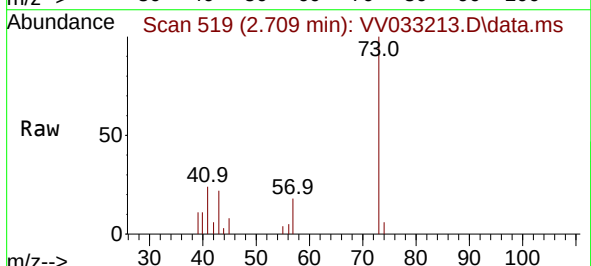

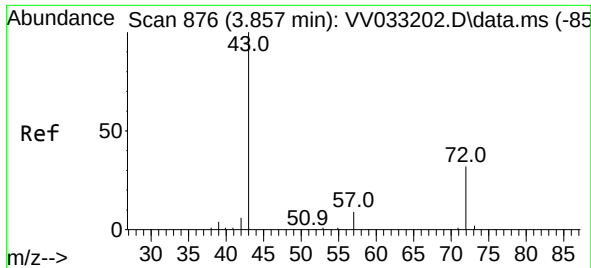

#22
2-Butanone
Concen: 22.370 ug/L m
RT: 3.876 min Scan# 882
Delta R.T. 0.019 min
Lab File: VV033213.D
Acq: 11 Dec 2023 15:21

Instrument :
MSVOA_V
ClientSampleId :
YCH87

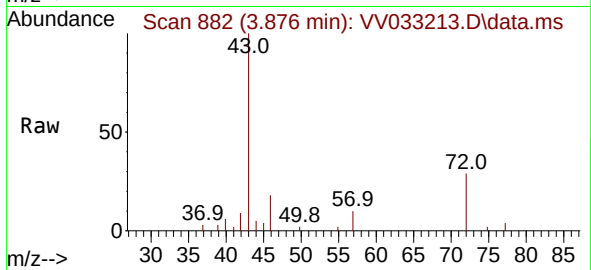

Tgt Ion: 43 Resp: 2184
Ion Ratio Lower Upper
43 100
72 14.6 14.6 43.8

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 12/12/2023
Supervised By :Semsettin Yesilyurt 12/12/2023

