

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033224.D
 Acq On : 11 Dec 2023 19:37
 Operator : SY/MD
 Sample : 05730-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GB8

Quant Time: Dec 12 00:43:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 21:51:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	263574	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	264045	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	138991	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	57686	36.611	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	73.220%		
7) Chloroethane-d5	1.532	69	48594	44.263	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	88.520%		
11) 1,1-Dichloroethene-d2	2.060	65	25370	42.325	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.640%		
21) 2-Butanone-d5	3.780	46	79493	101.577	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.580%		
24) Chloroform-d	4.249	84	157412	47.075	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.160%		
26) 1,2-Dichloroethane-d4	4.941	65	104700	50.362	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.720%		
32) Benzene-d6	4.960	84	288081	46.650	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.300%		
36) 1,2-Dichloropropane-d6	5.989	67	79980	48.168	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	96.340%		
41) Toluene-d8	7.243	98	266119	45.174	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.340%		
43) trans-1,3-Dichloroprop...	7.551	79	44231	42.126	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.260%		
47) 2-Hexanone-d5	8.021	63	65830	98.688	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	98.690%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	118775	50.321	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	100.640%		
66) 1,2-Dichlorobenzene-d4	11.561	152	129630	52.419	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	104.840%		
Target Compounds					Qvalue	
12) 1,1-Dichloroethene	2.066	96	1947	1.473	ug/L #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033224.D
Acq On : 11 Dec 2023 19:37
Operator : SY/MD
Sample : 05730-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GB8

Quant Time: Dec 12 00:43:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 21:51:12 2023
Response via : Initial Calibration

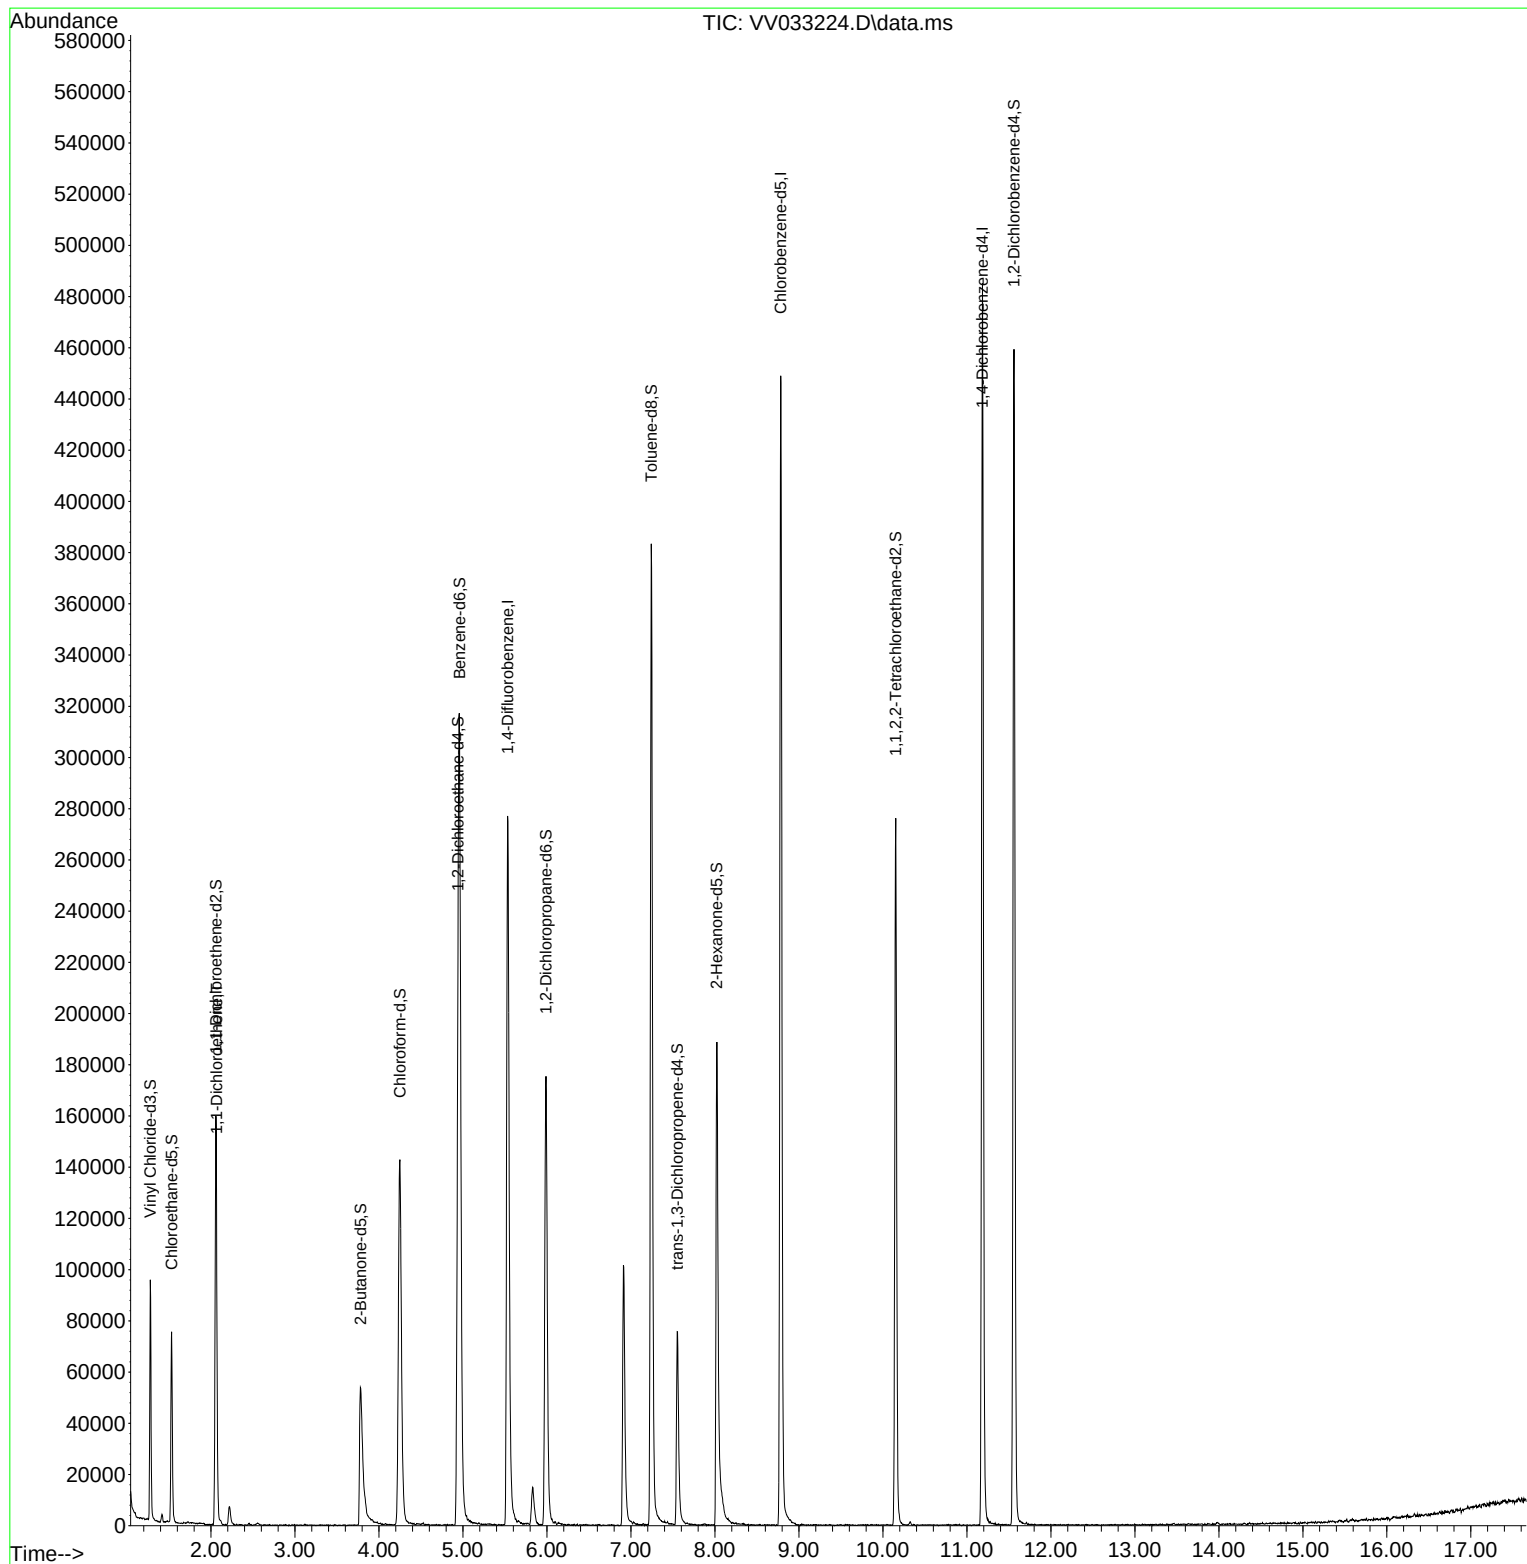

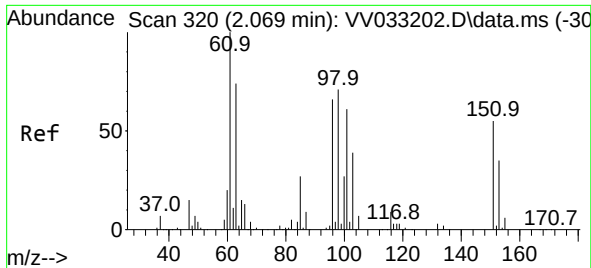

#12

1,1-Dichloroethene

Concen: 1.473 ug/L

RT: 2.066 min Scan# 31

Delta R.T. -0.003 min

Lab File: VV033224.D


Acq: 11 Dec 2023 19:37

Instrument :

MSVOA_V

ClientSampleId :

C0GB8

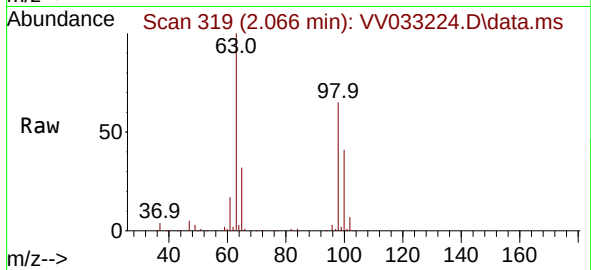

Tgt Ion:	96	Resp:	1947
Ion	Ratio	Lower	Upper
96	100		
61	582.0	109.1	202.7#
63	3511.9	85.3	158.3#

