

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033230.D
 Acq On : 11 Dec 2023 22:19
 Operator : SY/MD
 Sample : 05730-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC1

Quant Time: Dec 12 03:27:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 21:51:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	272778	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	269840	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	140656	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	56951	34.925	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	69.860%	
7) Chloroethane-d5	1.532	69	47234	41.572	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	83.140%	
11) 1,1-Dichloroethene-d2	2.060	65	25305	40.792	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	81.580%	
21) 2-Butanone-d5	3.780	46	82123	101.396	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	101.400%	
24) Chloroform-d	4.249	84	157917	45.633	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.260%	
26) 1,2-Dichloroethane-d4	4.941	65	102631	47.701	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.400%	
32) Benzene-d6	4.960	84	288191	45.665	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.340%	
36) 1,2-Dichloropropane-d6	5.986	67	81153	47.825	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	95.660%	
41) Toluene-d8	7.243	98	260474	43.266	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	86.540%	
43) trans-1,3-Dichloroprop...	7.551	79	45319	42.236	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	84.480%	
47) 2-Hexanone-d5	8.021	63	67214	98.599	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	98.600%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	118506	49.129	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	98.260%	
66) 1,2-Dichlorobenzene-d4	11.561	152	129323	51.675	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	103.360%	
Target Compounds						
12) 1,1-Dichloroethene	2.069	96	4525	3.309	ug/L	Qvalue # 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033230.D
Acq On : 11 Dec 2023 22:19
Operator : SY/MD
Sample : 05730-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC1

Quant Time: Dec 12 03:27:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 21:51:12 2023
Response via : Initial Calibration

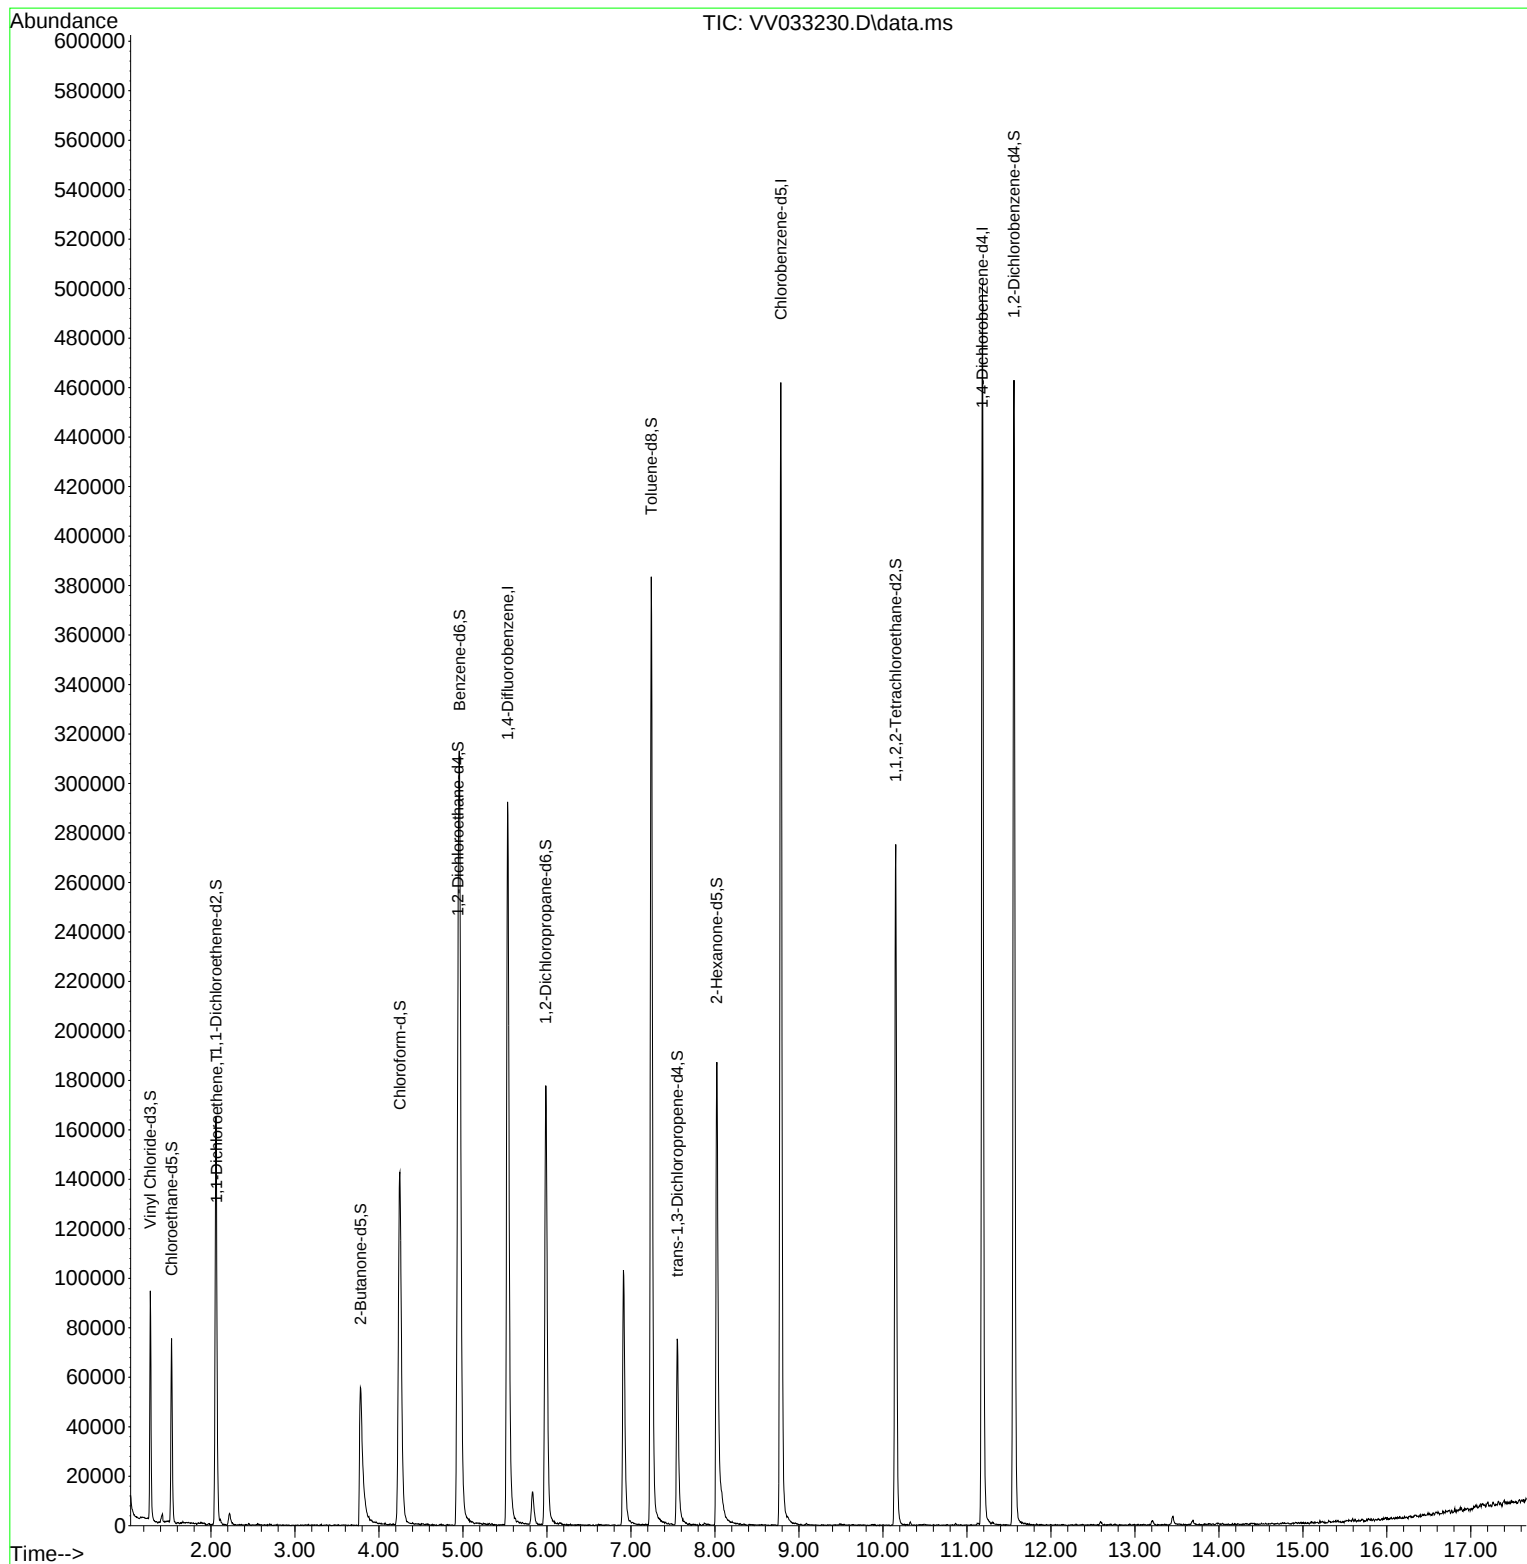

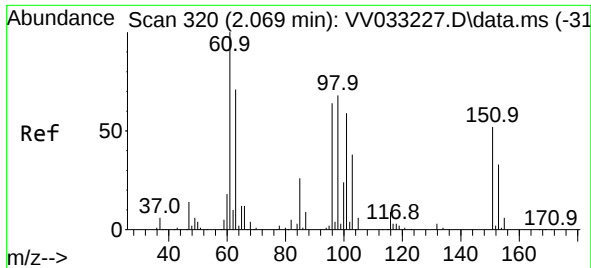

#12

1,1-Dichloroethene

Concen: 3.309 ug/L

RT: 2.069 min Scan# 31

Delta R.T. 0.000 min

Lab File: VV033230.D


Acq: 11 Dec 2023 22:19

Instrument :

MSVOA_V

ClientSampleId :

C0GC1

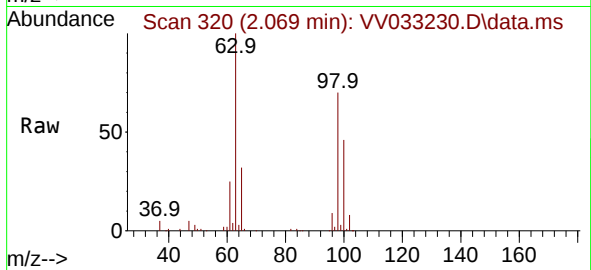

Tgt Ion:	96	Resp:	4525
Ion	Ratio	Lower	Upper
96	100		
61	290.8	109.1	202.7#
63	1160.9	85.3	158.3#

