

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033220.D
 Acq On : 11 Dec 2023 18:04
 Operator : SY/MD
 Sample : 05730-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	97408	97108	11.87%	1.443%
2	1.532	145	153	167	rVB	73914	89354	10.92%	1.328%
3	2.060	303	317	329	rBV	157236	228493	27.92%	3.396%
4	2.175	350	353	354	rBV2	248	163	0.02%	0.002%
5	2.220	358	367	385	rVV2	12872	23033	2.81%	0.342%
6	2.336	401	403	407	rBV	321	212	0.03%	0.003%
7	2.452	434	439	444	rBV2	853	940	0.11%	0.014%
8	2.603	483	486	488	rBV2	279	172	0.02%	0.003%
9	2.632	493	495	501	rVB2	288	296	0.04%	0.004%
10	2.680	506	510	511	rBV	296	206	0.03%	0.003%
11	2.751	529	532	536	rVB	350	324	0.04%	0.005%
12	2.773	536	539	542	rBV	243	205	0.03%	0.003%
13	2.793	542	545	547	rVV2	426	235	0.03%	0.003%
14	2.851	559	563	566	rBV2	306	244	0.03%	0.004%
15	3.024	614	617	620	rVB	231	141	0.02%	0.002%
16	3.069	628	631	632	rBV2	269	194	0.02%	0.003%
17	3.121	643	647	652	rBV3	411	463	0.06%	0.007%
18	3.182	662	666	669	rBV2	329	306	0.04%	0.005%
19	3.240	680	684	685	rBV	241	179	0.02%	0.003%
20	3.433	742	744	753	rVB2	381	372	0.05%	0.006%
21	3.471	753	756	759	rBV2	318	277	0.03%	0.004%
22	3.561	780	784	787	rBV2	400	328	0.04%	0.005%
23	3.654	809	813	814	rBV2	241	185	0.02%	0.003%
24	3.709	827	830	832	rVB	327	221	0.03%	0.003%
25	3.738	833	839	841	rBV	313	281	0.03%	0.004%
26	3.780	841	852	884	rBV	56541	157478	19.24%	2.341%
27	4.114	953	956	958	rBV2	313	248	0.03%	0.004%
28	4.249	983	998	1032	rBV	141036	359537	43.93%	5.344%
29	4.397	1039	1044	1050	rBV3	668	965	0.12%	0.014%
30	4.510	1070	1079	1087	rBV5	1245	2489	0.30%	0.037%
31	4.597	1104	1106	1110	rVB	422	216	0.03%	0.003%
32	4.715	1138	1143	1145	rVV	341	266	0.03%	0.004%
33	4.773	1159	1161	1163	rBV	288	142	0.02%	0.002%
34	4.892	1197	1198	1201	rVB	272	137	0.02%	0.002%
35	4.957	1201	1218	1256	rBV2	306044	818380	100.00%	12.164%
36	5.407	1356	1358	1362	rBV3	309	293	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033220.D
 Acq On : 11 Dec 2023 18:04
 Operator : SY/MD
 Sample : 05730-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COGA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.442	1368	1369	1371	rBV3	447	223	0.03%	0.003%
38	5.478	1376	1380	1382	rBV	257	192	0.02%	0.003%
39	5.532	1386	1397	1424	rBV	279853	576750	70.47%	8.572%
40	5.828	1479	1489	1508	rBV4	10774	24532	3.00%	0.365%
41	5.928	1516	1520	1522	rVB2	390	234	0.03%	0.003%
42	5.989	1525	1539	1563	rBV2	171709	359910	43.98%	5.349%
43	6.268	1624	1626	1632	rVB2	356	218	0.03%	0.003%
44	6.294	1632	1634	1638	rBV	236	139	0.02%	0.002%
45	6.317	1638	1641	1643	rBV	269	184	0.02%	0.003%
46	6.330	1643	1645	1650	rVB	363	217	0.03%	0.003%
47	6.375	1656	1659	1660	rBV	291	141	0.02%	0.002%
48	6.481	1688	1692	1694	rBV2	267	234	0.03%	0.003%
49	6.574	1716	1721	1729	rBV	2316	2406	0.29%	0.036%
50	6.609	1729	1732	1733	rBV	280	160	0.02%	0.002%
51	6.641	1738	1742	1745	rVV	263	194	0.02%	0.003%
52	6.760	1777	1779	1784	rVB2	184	175	0.02%	0.003%
53	6.912	1816	1826	1847	rBV	99698	186779	22.82%	2.776%
54	7.175	1906	1908	1910	rBV	314	161	0.02%	0.002%
55	7.243	1917	1929	1956	rBV	373742	653588	79.86%	9.714%
56	7.555	2013	2026	2047	rBV	72730	133353	16.29%	1.982%
57	7.722	2076	2078	2081	rBV3	334	174	0.02%	0.003%
58	7.796	2098	2101	2104	rBV	187	165	0.02%	0.002%
59	7.883	2121	2128	2133	rBV3	1291	1411	0.17%	0.021%
60	7.937	2143	2145	2149	rBV	348	317	0.04%	0.005%
61	7.979	2154	2158	2159	rBV	262	219	0.03%	0.003%
62	8.024	2162	2172	2202	rBV	190180	366841	44.83%	5.452%
63	8.445	2301	2303	2306	rBV2	377	175	0.02%	0.003%
64	8.577	2341	2344	2348	rBV2	249	235	0.03%	0.003%
65	8.783	2398	2408	2439	rBV	452187	745167	91.05%	11.075%
66	8.953	2458	2461	2463	rBV2	764	403	0.05%	0.006%
67	9.085	2498	2502	2504	rBV2	510	302	0.04%	0.004%
68	9.201	2535	2538	2540	rBV	422	271	0.03%	0.004%
69	9.326	2574	2577	2581	rVB2	463	339	0.04%	0.005%
70	9.349	2581	2584	2586	rBV2	341	295	0.04%	0.004%
71	9.416	2599	2605	2609	rVB2	313	339	0.04%	0.005%
72	9.442	2609	2613	2618	rBV2	353	338	0.04%	0.005%
73	9.484	2622	2626	2628	rBV2	215	175	0.02%	0.003%
74	9.500	2628	2631	2633	rVV2	389	248	0.03%	0.004%
75	9.519	2633	2637	2640	rVB2	273	142	0.02%	0.002%
76	9.677	2679	2686	2690	rBV2	231	356	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
 Data File : VV033220.D
 Acq On : 11 Dec 2023 18:04
 Operator : SY/MD
 Sample : 05730-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	9.780	2715	2718	2720	rBV	211	161	0.02%	0.002%
78	10.034	2793	2797	2801	rBV2	452	568	0.07%	0.008%
79	10.111	2818	2821	2823	rBV	328	234	0.03%	0.003%
80	10.153	2823	2834	2857	rBV	269297	425901	52.04%	6.330%
81	10.329	2880	2889	2896	rBV5	1887	2709	0.33%	0.040%
82	10.538	2951	2954	2958	rBV	313	284	0.03%	0.004%
83	10.873	3055	3058	3060	rBV2	425	279	0.03%	0.004%
84	11.136	3138	3140	3144	rVB2	384	209	0.03%	0.003%
85	11.185	3144	3155	3182	rBV	470368	739627	90.38%	10.993%
86	11.561	3260	3272	3293	rBV	461752	711754	86.97%	10.579%
87	11.950	3391	3393	3396	rBV	252	178	0.02%	0.003%
88	12.095	3435	3438	3442	rBV2	350	321	0.04%	0.005%
89	12.143	3448	3453	3455	rBV2	419	303	0.04%	0.005%
90	12.297	3496	3501	3507	rVB3	413	538	0.07%	0.008%
91	12.333	3507	3512	3513	rBV2	256	250	0.03%	0.004%
92	13.214	3784	3786	3794	rVB5	410	389	0.05%	0.006%
93	13.268	3801	3803	3806	rBV2	409	217	0.03%	0.003%
94	13.448	3856	3859	3861	rBV	390	245	0.03%	0.004%
95	13.506	3876	3877	3880	rBV	360	231	0.03%	0.003%
96	13.590	3901	3903	3905	rBV2	303	155	0.02%	0.002%
97	13.738	3947	3949	3952	rBV	344	180	0.02%	0.003%
98	13.982	4022	4025	4027	rBV2	1040	749	0.09%	0.011%
99	14.480	4177	4180	4183	rBV2	595	363	0.04%	0.005%
100	14.876	4301	4303	4305	rBV	730	442	0.05%	0.007%




Sum of corrected areas: 6728072

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033220.D
Acq On : 11 Dec 2023 18:04
Operator : SY/MD
Sample : 05730-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

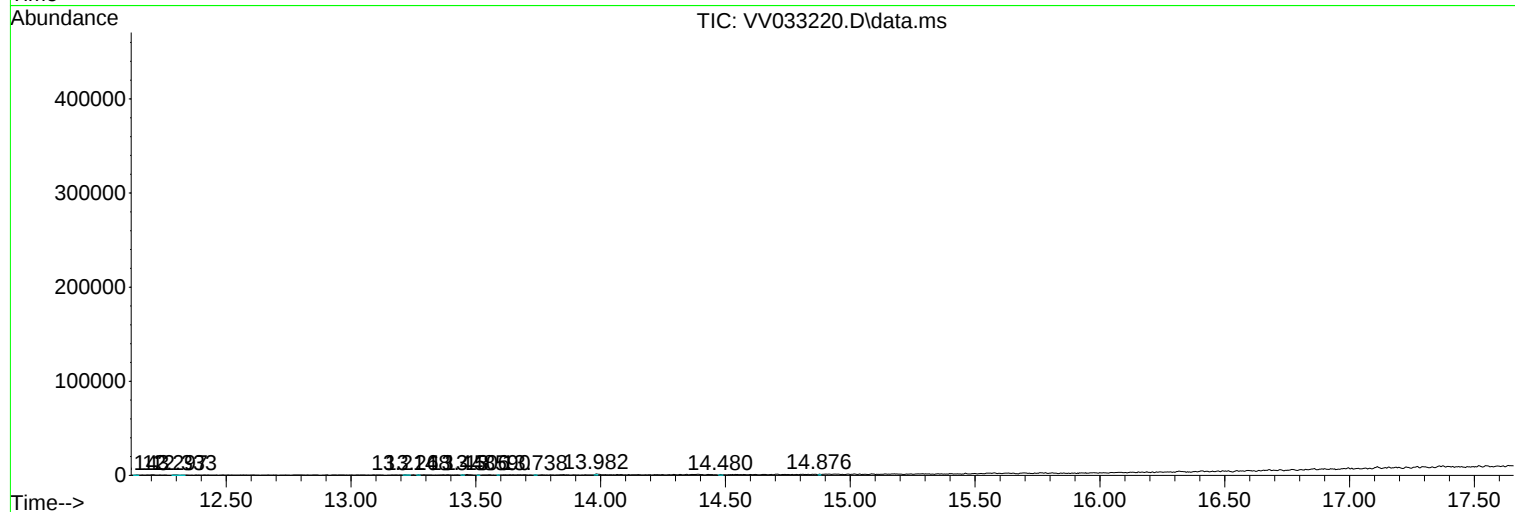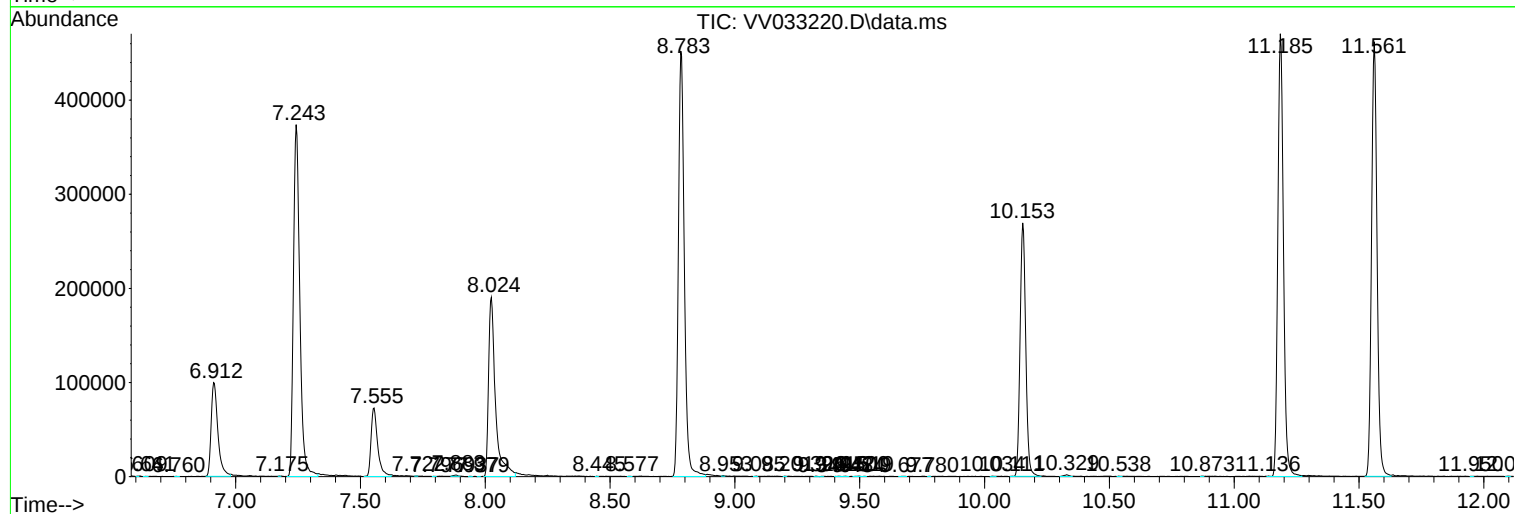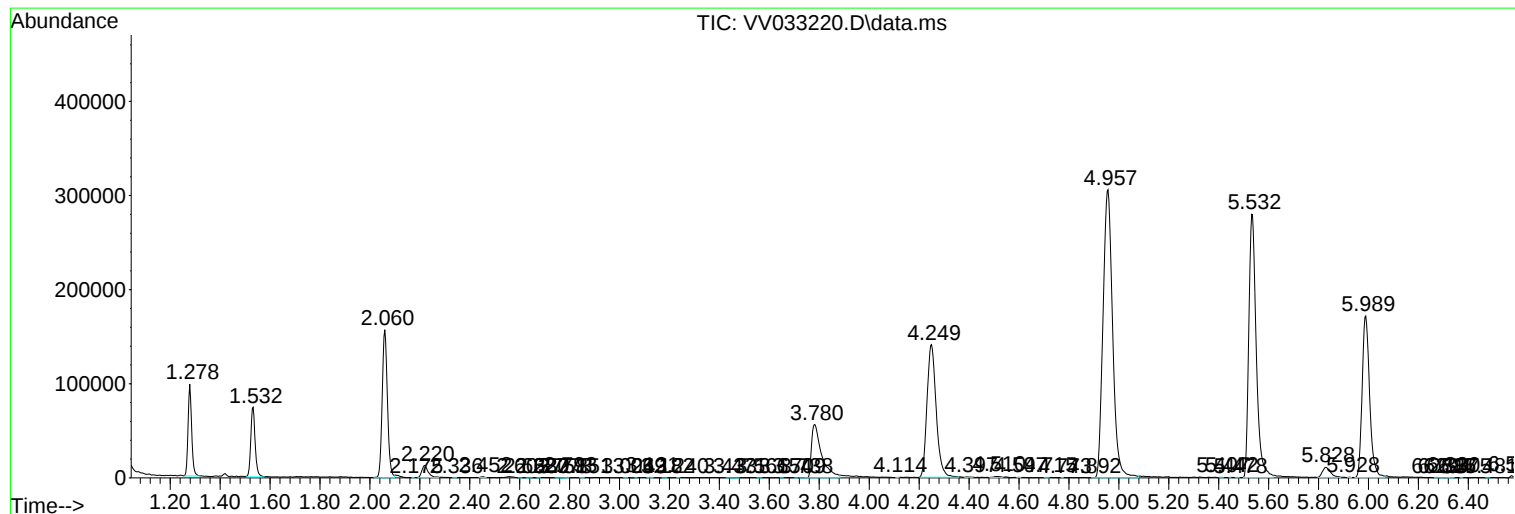

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033220.D
Acq On : 11 Dec 2023 18:04
Operator : SY/MD
Sample : 05730-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033220.D
Acq On : 11 Dec 2023 18:04
Operator : SY/MD
Sample : 05730-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc