

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
 Data File : VV033221.D
 Acq On : 11 Dec 2023 18:27
 Operator : SY/MD
 Sample : 05730-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	91791	96080	11.00%	1.244%
2	1.532	145	153	168	rVB	72716	87880	10.06%	1.138%
3	1.999	296	298	301	rVB2	571	238	0.03%	0.003%
4	2.060	305	317	334	rBV2	166707	264892	30.33%	3.430%
5	2.175	349	353	355	rBV	308	216	0.02%	0.003%
6	2.220	355	367	381	rBV2	7178	13600	1.56%	0.176%
7	2.362	408	411	413	rBV	354	206	0.02%	0.003%
8	2.413	425	427	430	rVB	289	163	0.02%	0.002%
9	2.429	430	432	433	rBV	335	158	0.02%	0.002%
10	2.449	433	438	439	rBV3	944	816	0.09%	0.011%
11	2.548	466	469	471	rBV2	488	362	0.04%	0.005%
12	2.619	489	491	495	rVB	377	210	0.02%	0.003%
13	2.764	534	536	544	rVB2	312	430	0.05%	0.006%
14	2.802	545	548	549	rBV	399	258	0.03%	0.003%
15	2.902	573	579	581	rVB2	230	212	0.02%	0.003%
16	3.015	611	614	617	rBV2	226	177	0.02%	0.002%
17	3.079	632	634	637	rBV	268	149	0.02%	0.002%
18	3.117	637	646	650	rVV5	1045	1541	0.18%	0.020%
19	3.140	650	653	656	rVB	289	198	0.02%	0.003%
20	3.179	661	665	667	rBV2	325	220	0.03%	0.003%
21	3.262	685	691	695	rBV	378	438	0.05%	0.006%
22	3.281	695	697	699	rVV2	222	138	0.02%	0.002%
23	3.310	703	706	709	rVB	360	265	0.03%	0.003%
24	3.429	739	743	744	rBV	166	142	0.02%	0.002%
25	3.474	753	757	761	rBV2	399	386	0.04%	0.005%
26	3.529	770	774	777	rBV2	269	246	0.03%	0.003%
27	3.593	791	794	796	rVV	254	142	0.02%	0.002%
28	3.645	807	810	813	rBB2	348	185	0.02%	0.002%
29	3.690	821	824	827	rVB2	401	260	0.03%	0.003%
30	3.712	827	831	832	rBV	410	296	0.03%	0.004%
31	3.780	843	852	899	rBV3	59929	231113	26.46%	2.993%
32	4.249	981	998	1024	rBV	139151	357526	40.94%	4.630%
33	4.513	1066	1080	1098	rBV3	13015	32269	3.69%	0.418%
34	4.635	1116	1118	1121	rBV	223	179	0.02%	0.002%
35	4.748	1150	1153	1156	rBV	413	272	0.03%	0.004%
36	4.825	1174	1177	1182	rVB2	329	302	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033221.D
 Acq On : 11 Dec 2023 18:27
 Operator : SY/MD
 Sample : 05730-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.850	1182	1185	1187	rBV	281	221	0.03%	0.003%
38	4.957	1200	1218	1247	rBV2	302537	816335	93.47%	10.571%
39	5.394	1350	1354	1359	rVB3	514	485	0.06%	0.006%
40	5.423	1359	1363	1366	rVB2	428	316	0.04%	0.004%
41	5.532	1386	1397	1428	rBV	280879	581835	66.62%	7.534%
42	5.831	1477	1490	1514	rBV	435253	873361	100.00%	11.309%
43	5.989	1527	1539	1562	rBV2	176577	355924	40.75%	4.609%
44	6.178	1596	1598	1603	rVB3	938	762	0.09%	0.010%
45	6.201	1603	1605	1607	rVB2	441	166	0.02%	0.002%
46	6.307	1636	1638	1642	rBV	312	240	0.03%	0.003%
47	6.326	1642	1644	1648	rVB	362	241	0.03%	0.003%
48	6.481	1688	1692	1698	rVB2	238	264	0.03%	0.003%
49	6.519	1702	1704	1712	rVB2	320	447	0.05%	0.006%
50	6.561	1713	1717	1719	rBV2	358	359	0.04%	0.005%
51	6.690	1751	1757	1762	rBV2	367	486	0.06%	0.006%
52	6.722	1762	1767	1769	rBV	318	254	0.03%	0.003%
53	6.786	1784	1787	1792	rBB	238	195	0.02%	0.003%
54	6.821	1794	1798	1801	rBV2	216	185	0.02%	0.002%
55	6.911	1816	1826	1850	rBV	97929	185479	21.24%	2.402%
56	7.159	1899	1903	1907	rBV3	578	445	0.05%	0.006%
57	7.243	1917	1929	1951	rBV	374130	659371	75.50%	8.538%
58	7.551	2016	2025	2047	rBV	73770	132329	15.15%	1.714%
59	7.770	2091	2093	2095	rBV2	749	456	0.05%	0.006%
60	7.809	2101	2105	2106	rBV2	313	157	0.02%	0.002%
61	7.844	2112	2116	2118	rBV2	323	251	0.03%	0.003%
62	8.024	2162	2172	2207	rBV	189283	371946	42.59%	4.816%
63	8.667	2369	2372	2373	rBV2	199	140	0.02%	0.002%
64	8.699	2379	2382	2386	rVB	357	240	0.03%	0.003%
65	8.725	2386	2390	2393	rBV2	337	310	0.04%	0.004%
66	8.783	2398	2408	2439	rBV	443558	742522	85.02%	9.615%
67	8.956	2461	2462	2465	rVB2	696	242	0.03%	0.003%
68	9.095	2501	2505	2508	rBV	440	293	0.03%	0.004%
69	9.381	2591	2594	2597	rVB2	367	227	0.03%	0.003%
70	9.413	2600	2604	2606	rBV	160	159	0.02%	0.002%
71	9.429	2606	2609	2611	rVB2	503	230	0.03%	0.003%
72	9.741	2699	2706	2708	rBV	371	482	0.06%	0.006%
73	9.783	2715	2719	2721	rBV2	197	165	0.02%	0.002%
74	9.860	2738	2743	2746	rBV	184	202	0.02%	0.003%
75	9.966	2772	2776	2781	rBV	366	394	0.05%	0.005%
76	10.021	2792	2793	2798	rVB2	286	145	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033221.D
 Acq On : 11 Dec 2023 18:27
 Operator : SY/MD
 Sample : 05730-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	10.095	2813	2816	2821	rVB2	222	256	0.03%	0.003%
78	10.153	2821	2834	2853	rBV	272279	430283	49.27%	5.572%
79	10.326	2881	2888	2894	rVB2	640	1000	0.11%	0.013%
80	10.448	2923	2926	2929	rBV2	371	251	0.03%	0.003%
81	10.474	2930	2934	2937	rVB3	337	281	0.03%	0.004%
82	10.500	2937	2942	2945	rVB2	386	376	0.04%	0.005%
83	10.529	2946	2951	2954	rBV2	217	210	0.02%	0.003%
84	10.628	2980	2982	2985	rBV	295	162	0.02%	0.002%
85	10.747	3016	3019	3022	rBV	355	276	0.03%	0.004%
86	10.802	3032	3036	3040	rVB2	524	367	0.04%	0.005%
87	11.185	3144	3155	3179	rBV	489413	750710	85.96%	9.721%
88	11.490	3247	3250	3254	rBV3	400	249	0.03%	0.003%
89	11.561	3260	3272	3291	rBV	450712	714555	81.82%	9.253%
90	11.905	3376	3379	3382	rBV	321	165	0.02%	0.002%
91	12.197	3466	3470	3474	rBV	418	385	0.04%	0.005%
92	12.567	3581	3585	3587	rBV	223	178	0.02%	0.002%
93	12.599	3593	3595	3599	rBV2	333	193	0.02%	0.002%
94	12.741	3636	3639	3643	rBV2	459	373	0.04%	0.005%
95	12.889	3682	3685	3689	rBV	378	375	0.04%	0.005%
96	13.252	3796	3798	3802	rVB3	341	209	0.02%	0.003%
97	13.574	3894	3898	3900	rBV3	386	316	0.04%	0.004%
98	13.728	3944	3946	3947	rBV3	436	197	0.02%	0.003%
99	14.098	4058	4061	4066	rVB2	640	518	0.06%	0.007%
100	14.622	4221	4224	4226	rBV2	567	398	0.05%	0.005%




Sum of corrected areas: 7722709

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033221.D
Acq On : 11 Dec 2023 18:27
Operator : SY/MD
Sample : 05730-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

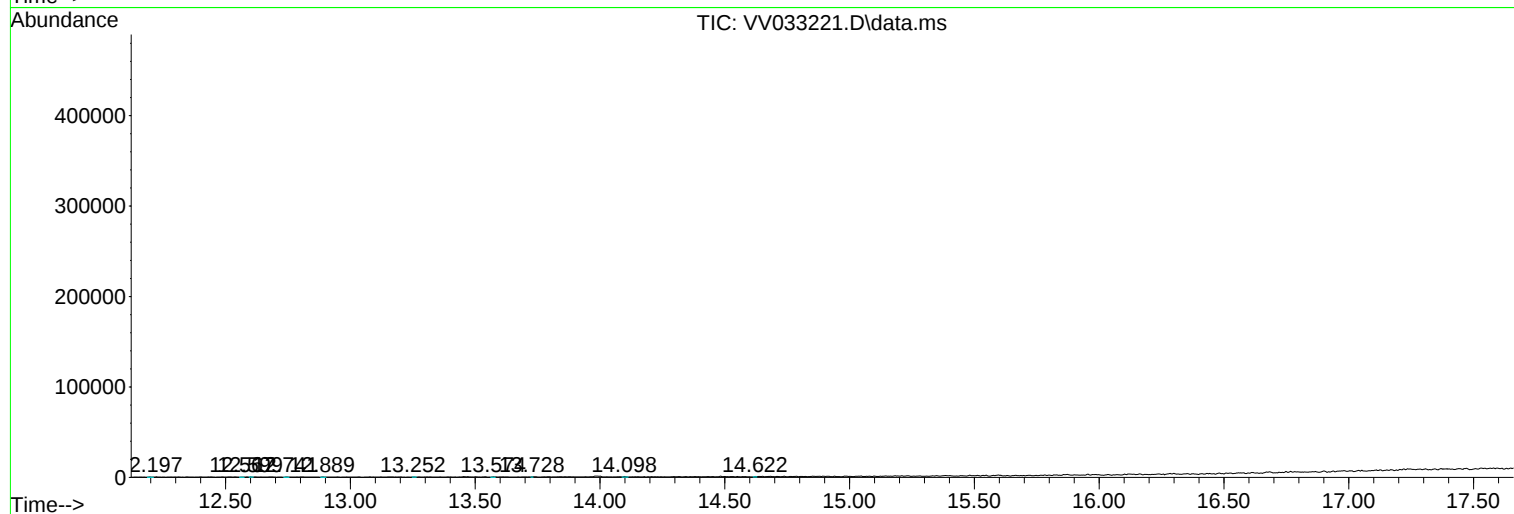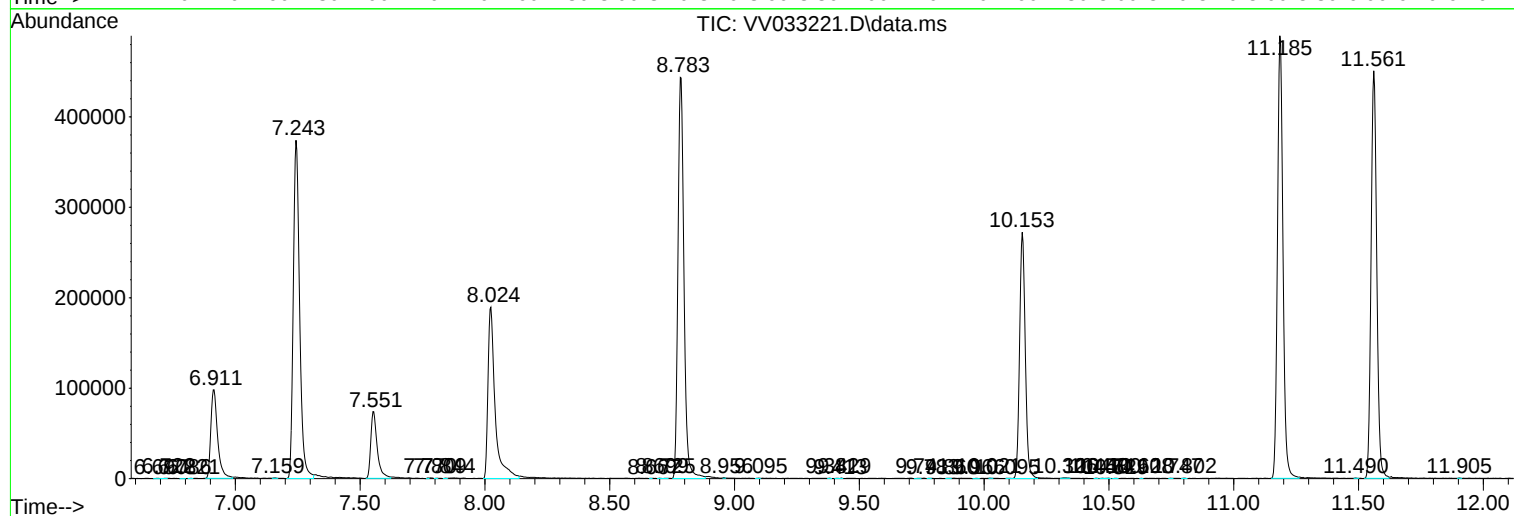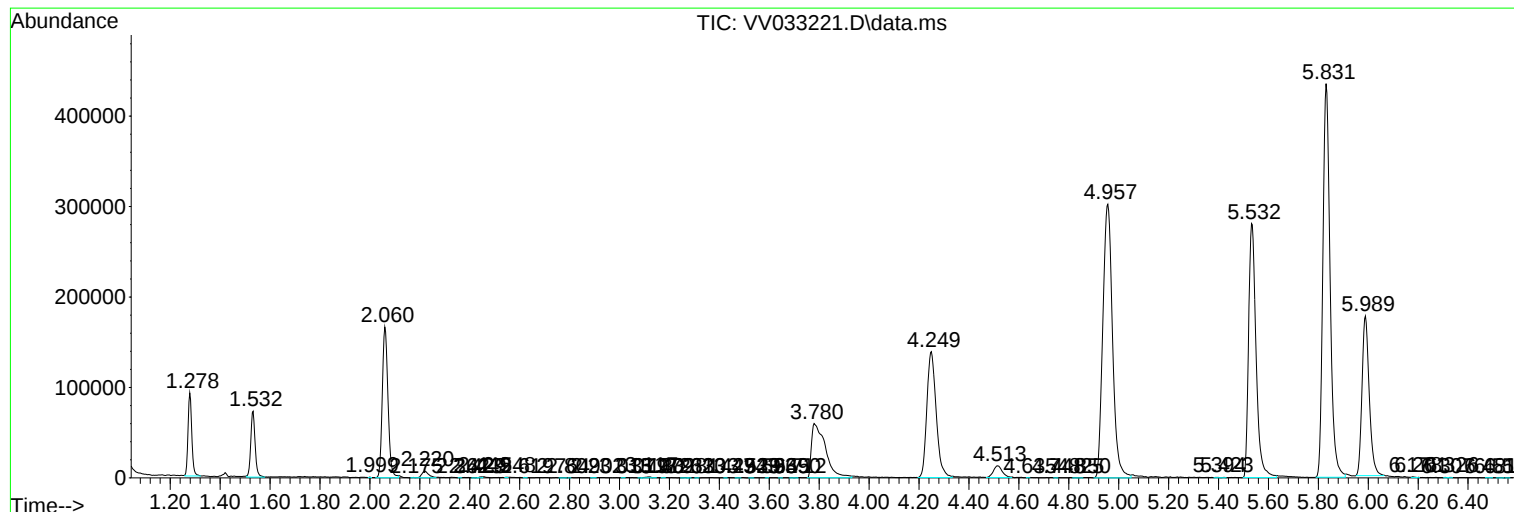

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033221.D
Acq On : 11 Dec 2023 18:27
Operator : SY/MD
Sample : 05730-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033221.D
Acq On : 11 Dec 2023 18:27
Operator : SY/MD
Sample : 05730-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc