

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
 Data File : VV033229.D
 Acq On : 11 Dec 2023 21:56
 Operator : SY/MD
 Sample : 05730-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	95264	97118	11.47%	1.322%
2	1.532	145	153	171	rVB	75666	91340	10.79%	1.243%
3	2.060	306	317	331	rBV	164395	245900	29.05%	3.346%
4	2.220	358	367	376	rBV2	8239	15082	1.78%	0.205%
5	2.320	396	398	400	rBV	308	179	0.02%	0.002%
6	2.343	403	405	408	rVV	455	273	0.03%	0.004%
7	2.372	412	414	426	rVB3	681	1065	0.13%	0.014%
8	2.420	427	429	430	rBV	395	186	0.02%	0.003%
9	2.445	433	437	441	rVV2	812	792	0.09%	0.011%
10	2.516	457	459	462	rVB2	507	221	0.03%	0.003%
11	2.552	462	470	473	rBV2	1058	1110	0.13%	0.015%
12	3.056	624	627	628	rBV2	273	165	0.02%	0.002%
13	3.105	637	642	645	rBV3	352	283	0.03%	0.004%
14	3.117	645	646	649	rBV	366	196	0.02%	0.003%
15	3.156	654	658	661	rBV	153	165	0.02%	0.002%
16	3.217	673	677	679	rBV	316	328	0.04%	0.004%
17	3.259	688	690	693	rVB	275	152	0.02%	0.002%
18	3.281	693	697	699	rBV	192	191	0.02%	0.003%
19	3.355	717	720	723	rBV2	245	176	0.02%	0.002%
20	3.429	740	743	745	rBV	257	190	0.02%	0.003%
21	3.490	757	762	763	rBV	337	206	0.02%	0.003%
22	3.552	779	781	785	rBV	151	163	0.02%	0.002%
23	3.674	816	819	821	rBV2	271	157	0.02%	0.002%
24	3.741	836	840	842	rBV	302	215	0.03%	0.003%
25	3.783	842	853	882	rBV	56722	172823	20.42%	2.352%
26	4.146	964	966	968	rBV2	393	250	0.03%	0.003%
27	4.249	981	998	1029	rBV	145922	374423	44.24%	5.095%
28	4.474	1065	1068	1070	rBV2	438	235	0.03%	0.003%
29	4.516	1070	1081	1093	rVV5	3399	7696	0.91%	0.105%
30	4.844	1180	1183	1189	rVB2	380	430	0.05%	0.006%
31	4.873	1189	1192	1195	rBV	424	357	0.04%	0.005%
32	4.957	1201	1218	1244	rBV3	318050	846358	100.00%	11.517%
33	5.297	1321	1324	1329	rVB	533	409	0.05%	0.006%
34	5.400	1353	1356	1361	rBV3	491	457	0.05%	0.006%
35	5.532	1385	1397	1422	rBV	298661	618022	73.02%	8.410%
36	5.834	1478	1491	1512	rBV4	150018	315070	37.23%	4.287%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121123\
 Data File : VW033229.D
 Acq On : 11 Dec 2023 21:56
 Operator : SY/MD
 Sample : 05730-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.989	1527	1539	1561	rBV2	178024	368919	43.59%	5.020%
38	6.204	1604	1606	1611	rVB	595	399	0.05%	0.005%
39	6.265	1621	1625	1628	rBV2	311	226	0.03%	0.003%
40	6.330	1642	1645	1648	rBV2	226	155	0.02%	0.002%
41	6.629	1736	1738	1742	rVB	238	151	0.02%	0.002%
42	6.786	1781	1787	1790	rVV2	362	363	0.04%	0.005%
43	6.812	1791	1795	1797	rBV	188	160	0.02%	0.002%
44	6.912	1816	1826	1855	rBV	104079	195599	23.11%	2.662%
45	7.098	1882	1884	1887	rBV2	368	226	0.03%	0.003%
46	7.140	1894	1897	1899	rBV	447	294	0.03%	0.004%
47	7.243	1918	1929	1956	rBV	394741	690980	81.64%	9.402%
48	7.551	2016	2025	2052	rBV	74176	139421	16.47%	1.897%
49	7.789	2098	2099	2107	rVB4	631	492	0.06%	0.007%
50	7.834	2110	2113	2115	rBV	391	168	0.02%	0.002%
51	7.863	2120	2122	2125	rBV2	692	544	0.06%	0.007%
52	7.979	2154	2158	2162	rBV2	183	212	0.03%	0.003%
53	8.024	2162	2172	2201	rBV	187505	363574	42.96%	4.947%
54	8.368	2277	2279	2282	rBV2	461	246	0.03%	0.003%
55	8.426	2295	2297	2300	rBV2	261	166	0.02%	0.002%
56	8.783	2395	2408	2435	rBV	468263	784000	92.63%	10.668%
57	9.037	2485	2487	2488	rBV	308	151	0.02%	0.002%
58	9.165	2522	2527	2530	rVV2	212	210	0.02%	0.003%
59	9.249	2550	2553	2555	rBV2	332	155	0.02%	0.002%
60	9.606	2662	2664	2668	rBV2	354	268	0.03%	0.004%
61	9.735	2699	2704	2706	rBV	344	290	0.03%	0.004%
62	9.747	2706	2708	2712	rVB2	492	326	0.04%	0.004%
63	9.792	2714	2722	2725	rBV	303	433	0.05%	0.006%
64	9.873	2743	2747	2750	rBV2	570	547	0.06%	0.007%
65	9.985	2780	2782	2785	rBV	328	159	0.02%	0.002%
66	10.043	2796	2800	2802	rVB2	393	291	0.03%	0.004%
67	10.059	2803	2805	2808	rBV2	259	173	0.02%	0.002%
68	10.101	2814	2818	2820	rBV	194	160	0.02%	0.002%
69	10.153	2823	2834	2858	rVV	275722	428356	50.61%	5.829%
70	10.374	2900	2903	2906	rBV2	303	240	0.03%	0.003%
71	10.474	2931	2934	2935	rBV	588	301	0.04%	0.004%
72	10.673	2994	2996	2998	rBV2	270	155	0.02%	0.002%
73	10.754	3014	3021	3024	rVB2	260	264	0.03%	0.004%
74	10.792	3028	3033	3037	rBV2	291	328	0.04%	0.004%
75	10.866	3050	3056	3057	rBV2	756	624	0.07%	0.008%
76	11.101	3125	3129	3131	rBV2	329	268	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
 Data File : VV033229.D
 Acq On : 11 Dec 2023 21:56
 Operator : SY/MD
 Sample : 05730-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.127	3131	3137	3145	rVV3	1213	1712	0.20%	0.023%
78	11.185	3145	3155	3180	rBV	519067	800326	94.56%	10.890%
79	11.410	3221	3225	3227	rBV3	365	250	0.03%	0.003%
80	11.445	3233	3236	3238	rBV3	433	267	0.03%	0.004%
81	11.519	3256	3259	3260	rBV2	511	262	0.03%	0.004%
82	11.561	3260	3272	3291	rBV	479151	748074	88.39%	10.179%
83	11.773	3337	3338	3346	rVB3	431	288	0.03%	0.004%
84	11.886	3369	3373	3377	rBV2	526	467	0.06%	0.006%
85	11.934	3385	3388	3392	rBV	223	199	0.02%	0.003%
86	11.953	3392	3394	3399	rBV	286	215	0.03%	0.003%
87	12.284	3495	3497	3500	rBV2	347	214	0.03%	0.003%
88	12.381	3522	3527	3528	rBV	298	226	0.03%	0.003%
89	12.480	3553	3558	3561	rBV2	333	376	0.04%	0.005%
90	12.590	3589	3592	3595	rBV3	1114	889	0.11%	0.012%
91	12.699	3624	3626	3628	rBV	377	218	0.03%	0.003%
92	12.902	3686	3689	3691	rBV	451	256	0.03%	0.003%
93	13.001	3718	3720	3722	rBV2	382	149	0.02%	0.002%
94	13.075	3740	3743	3746	rBV	346	197	0.02%	0.003%
95	13.210	3778	3785	3793	rVB7	2437	4126	0.49%	0.056%
96	13.345	3825	3827	3829	rBV	295	151	0.02%	0.002%
97	13.403	3842	3845	3849	rBV2	282	239	0.03%	0.003%
98	13.448	3852	3859	3875	rVB	7056	11730	1.39%	0.160%
99	13.683	3926	3932	3943	rBV4	3658	5460	0.65%	0.074%
100	14.474	4174	4178	4181	rBV3	440	310	0.04%	0.004%


Sum of corrected areas: 7348978

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033229.D
Acq On : 11 Dec 2023 21:56
Operator : SY/MD
Sample : 05730-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

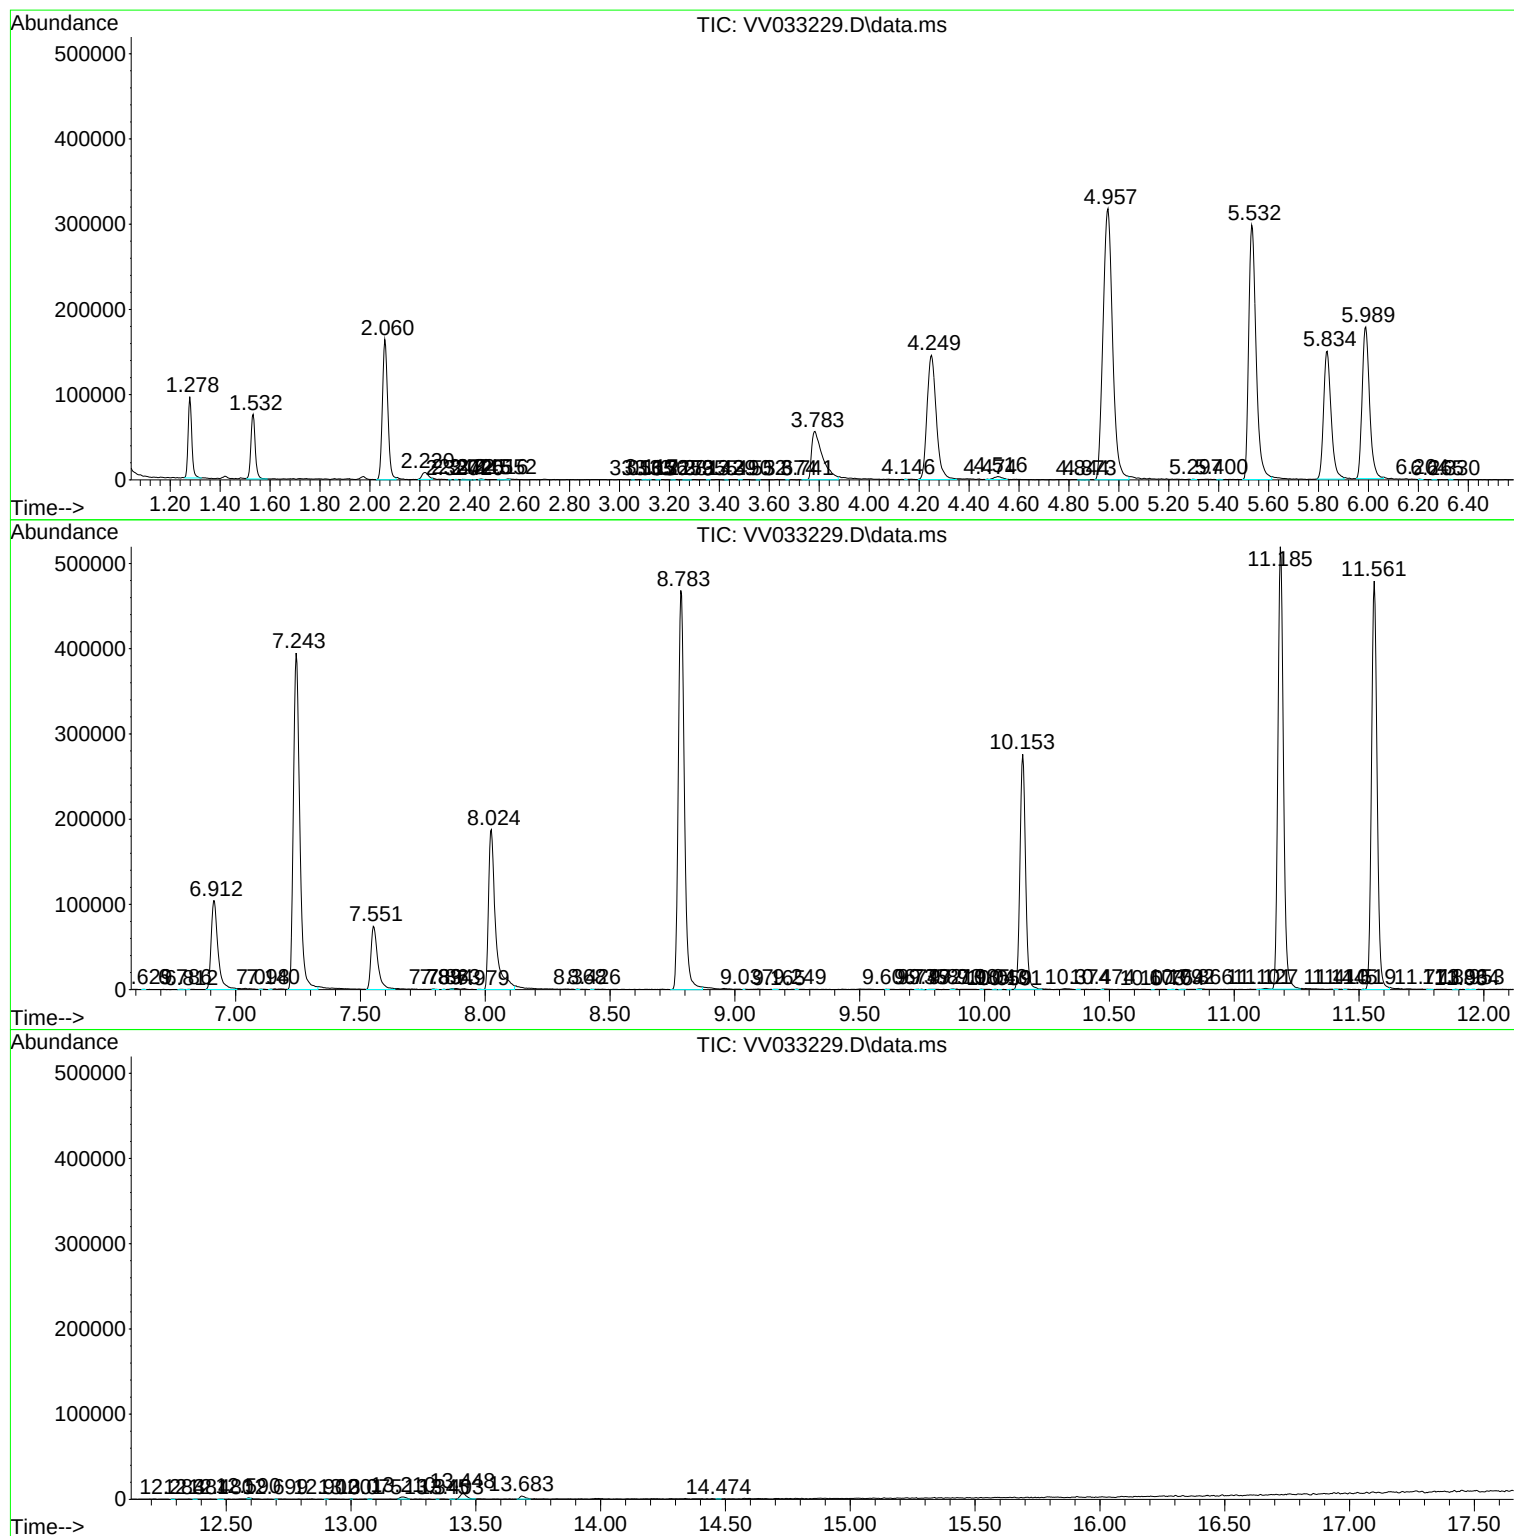

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033229.D
Acq On : 11 Dec 2023 21:56
Operator : SY/MD
Sample : 05730-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121123\
Data File : VV033229.D
Acq On : 11 Dec 2023 21:56
Operator : SY/MD
Sample : 05730-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc